

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020079.D
 Acq On : 20 Jan 2021 16:32
 Operator : SY/MD
 Sample : VV0120WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

Signal : TIC: VV020079.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	80	rVB	175000	173489	13.07%	1.654%
2	1.569	141	149	159	rBV	131651	146930	11.07%	1.400%
3	1.984	274	278	281	rBV3	628	511	0.04%	0.005%
4	2.110	306	317	348	rVB	304984	458620	34.56%	4.371%
5	2.357	391	394	396	rBV	243	165	0.01%	0.002%
6	2.512	433	442	450	rBV4	1714	2539	0.19%	0.024%
7	2.566	455	459	462	rBV2	477	293	0.02%	0.003%
8	2.624	474	477	482	rVB2	250	185	0.01%	0.002%
9	2.775	517	524	528	rBV3	567	606	0.05%	0.006%
10	2.807	531	534	537	rVB2	206	144	0.01%	0.001%
11	2.827	537	540	545	rBV2	233	232	0.02%	0.002%
12	2.881	555	557	560	rVB2	285	139	0.01%	0.001%
13	2.930	570	572	575	rBV	320	186	0.01%	0.002%
14	3.023	596	601	603	rBV	231	143	0.01%	0.001%
15	3.036	603	605	611	rVB	312	174	0.01%	0.002%
16	3.061	611	613	616	rBV	242	163	0.01%	0.002%
17	3.129	629	634	636	rBV	145	130	0.01%	0.001%
18	3.251	670	672	675	rBV	218	142	0.01%	0.001%
19	3.312	687	691	694	rVV2	215	167	0.01%	0.002%
20	3.335	696	698	701	rVB	355	158	0.01%	0.002%
21	3.354	701	704	709	rBV2	299	251	0.02%	0.002%
22	3.428	725	727	730	rBV	230	166	0.01%	0.002%
23	3.444	730	732	735	rVB2	272	162	0.01%	0.002%
24	3.483	738	744	746	rBV2	195	238	0.02%	0.002%
25	3.518	749	755	756	rBV2	185	146	0.01%	0.001%
26	3.685	804	807	810	rBV	274	160	0.01%	0.002%
27	3.704	810	813	815	rBV2	215	138	0.01%	0.001%
28	3.891	861	871	904	rBV	86113	250951	18.91%	2.392%
29	4.354	999	1015	1044	rBV	219822	539680	40.67%	5.144%
30	4.756	1137	1140	1143	rVB2	222	169	0.01%	0.002%
31	4.836	1162	1165	1166	rBV	199	143	0.01%	0.001%
32	4.952	1195	1201	1203	rBV	259	249	0.02%	0.002%
33	5.052	1214	1232	1261	rBV2	519576	1326959	100.00%	12.647%
34	5.367	1327	1330	1331	rBV2	239	162	0.01%	0.002%
35	5.418	1342	1346	1350	rBV3	282	274	0.02%	0.003%
36	5.621	1396	1409	1432	rBV	422131	841291	63.40%	8.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020079.D
 Acq On : 20 Jan 2021 16:32
 Operator : SY/MD
 Sample : VV0120WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

37	5.910	1487	1499	1520	rVB	27240	57709	4.35%	0.550%
38	6.074	1537	1550	1581	rBV	288419	587749	44.29%	5.602%
39	6.277	1609	1613	1618	rVB3	498	464	0.03%	0.004%
40	6.299	1618	1620	1621	rBV3	297	149	0.01%	0.001%
41	6.492	1674	1680	1685	rBV2	259	364	0.03%	0.003%
42	6.537	1691	1694	1696	rVB2	331	174	0.01%	0.002%
43	6.556	1696	1700	1705	rBV2	176	208	0.02%	0.002%
44	6.820	1779	1782	1789	rVB	172	170	0.01%	0.002%
45	6.865	1789	1796	1800	rBV	345	428	0.03%	0.004%
46	6.990	1823	1835	1861	rBV	168375	303304	22.86%	2.891%
47	7.203	1897	1901	1903	rBV2	402	347	0.03%	0.003%
48	7.318	1921	1937	1961	rBV	629326	1097085	82.68%	10.456%
49	7.589	2016	2021	2022	rBV2	350	239	0.02%	0.002%
50	7.627	2022	2033	2055	rVV	119342	206261	15.54%	1.966%
51	7.765	2074	2076	2080	rVB2	368	255	0.02%	0.002%
52	7.952	2131	2134	2136	rBV	173	131	0.01%	0.001%
53	7.984	2136	2144	2152	rVV4	1403	1913	0.14%	0.018%
54	8.093	2167	2178	2211	rBV2	298614	584979	44.08%	5.575%
55	8.383	2266	2268	2272	rVB2	357	156	0.01%	0.001%
56	8.492	2299	2302	2305	rVB2	356	199	0.01%	0.002%
57	8.524	2308	2312	2314	rBV	273	189	0.01%	0.002%
58	8.569	2322	2326	2330	rBV2	230	298	0.02%	0.003%
59	8.601	2333	2336	2342	rBV	231	285	0.02%	0.003%
60	8.859	2402	2416	2442	rBV	644309	1044353	78.70%	9.954%
61	9.026	2465	2468	2475	rVB	974	811	0.06%	0.008%
62	9.148	2499	2506	2509	rBV3	529	661	0.05%	0.006%
63	9.331	2558	2563	2566	rBV2	399	447	0.03%	0.004%
64	9.521	2618	2622	2626	rBV2	246	237	0.02%	0.002%
65	9.556	2626	2633	2639	rBV4	597	919	0.07%	0.009%
66	9.659	2661	2665	2669	rBV2	202	219	0.02%	0.002%
67	9.887	2733	2736	2742	rVB2	339	363	0.03%	0.003%
68	9.936	2748	2751	2761	rVB2	910	1082	0.08%	0.010%
69	9.981	2761	2765	2767	rBV2	185	162	0.01%	0.002%
70	10.003	2767	2772	2773	rBV	165	130	0.01%	0.001%
71	10.100	2798	2802	2804	rBV	181	147	0.01%	0.001%
72	10.174	2820	2825	2828	rBV	246	263	0.02%	0.003%
73	10.222	2828	2840	2862	rVV	385350	597934	45.06%	5.699%
74	10.338	2872	2876	2879	rVB2	454	311	0.02%	0.003%
75	10.437	2904	2907	2911	rBV	236	150	0.01%	0.001%
76	10.543	2936	2940	2941	rBV	592	458	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020079.D
 Acq On : 20 Jan 2021 16:32
 Operator : SY/MD
 Sample : VV0120WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

77	10.576	2948	2950	2953	rVB	294	134	0.01%	0.001%
78	10.698	2985	2988	2992	rBV	199	172	0.01%	0.002%
79	10.768	3004	3010	3013	rBV2	202	226	0.02%	0.002%
80	10.868	3034	3041	3044	rBV2	244	347	0.03%	0.003%
81	10.923	3054	3058	3062	rBV4	930	1068	0.08%	0.010%
82	11.093	3107	3111	3118	rVB2	237	210	0.02%	0.002%
83	11.122	3118	3120	3122	rBV	223	147	0.01%	0.001%
84	11.196	3136	3143	3150	rVB3	1204	1828	0.14%	0.017%
85	11.257	3150	3162	3182	rBV	729880	1130084	85.16%	10.771%
86	11.450	3219	3222	3226	rBV2	269	178	0.01%	0.002%
87	11.630	3266	3278	3302	rBV	706445	1110658	83.70%	10.586%
88	11.891	3355	3359	3362	rBV2	289	244	0.02%	0.002%
89	12.096	3417	3423	3428	rBV2	241	330	0.02%	0.003%
90	12.186	3446	3451	3452	rBV	261	198	0.01%	0.002%
91	12.264	3473	3475	3478	rBV	229	134	0.01%	0.001%
92	12.302	3485	3487	3490	rBV2	288	185	0.01%	0.002%
93	12.485	3540	3544	3549	rVB2	343	378	0.03%	0.004%
94	12.527	3553	3557	3561	rBV2	268	344	0.03%	0.003%
95	12.656	3590	3597	3606	rBV3	2430	3096	0.23%	0.030%
96	12.765	3628	3631	3633	rBV	398	236	0.02%	0.002%
97	12.981	3695	3698	3699	rBV	251	142	0.01%	0.001%
98	13.199	3762	3766	3769	rBV2	349	260	0.02%	0.002%
99	13.762	3933	3941	3949	rBV4	2245	3151	0.24%	0.030%
100	13.936	3993	3995	4001	rBV3	276	255	0.02%	0.002%


Sum of corrected areas: 10491963

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020079.D
Acq On : 20 Jan 2021 16:32
Operator : SY/MD
Sample : VV0120WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

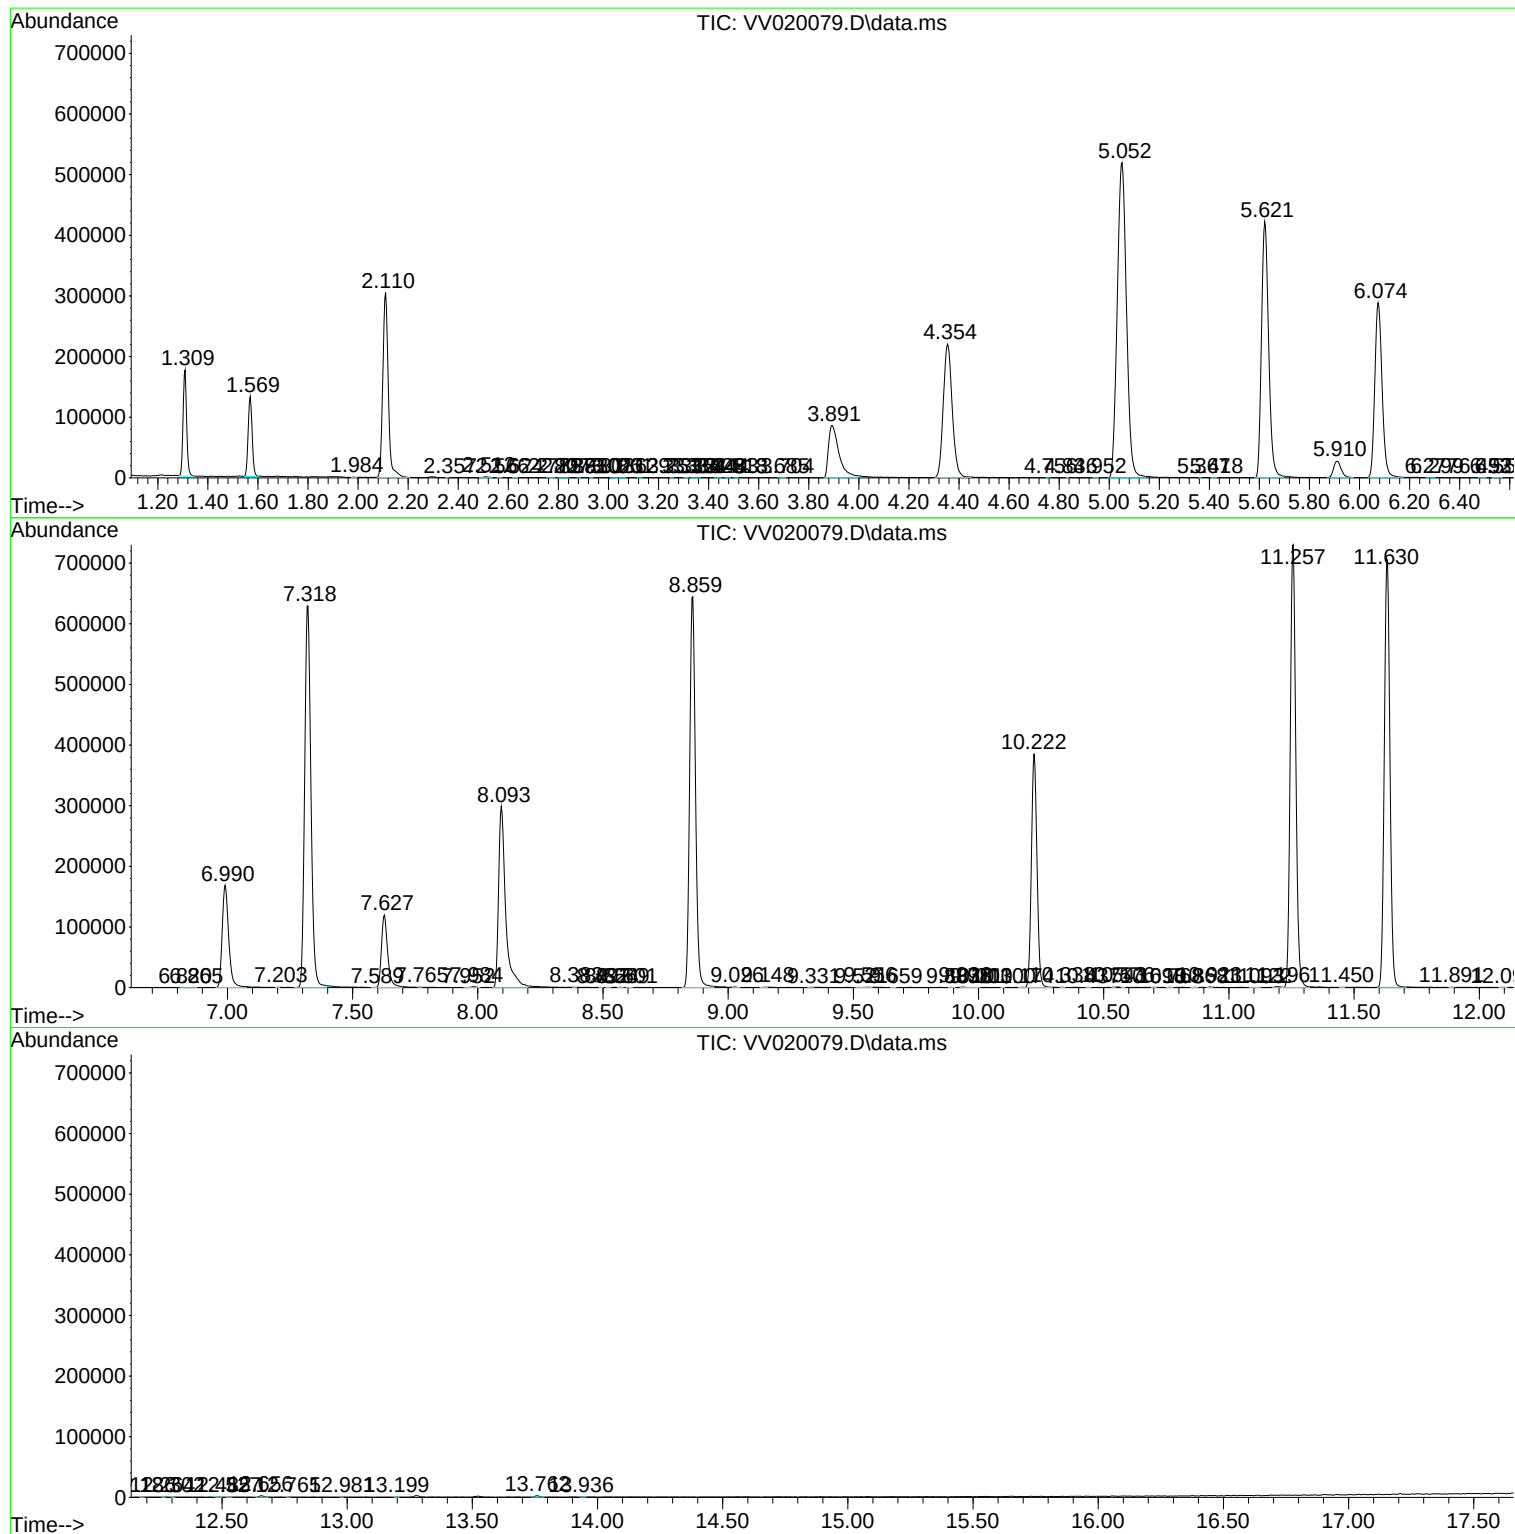

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020079.D
Acq On : 20 Jan 2021 16:32
Operator : SY/MD
Sample : VV0120WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020079.D
Acq On : 20 Jan 2021 16:32
Operator : SY/MD
Sample : VV0120WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
