

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020080.D
 Acq On : 20 Jan 2021 16:59
 Operator : SY/MD
 Sample : M1147-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

Signal : TIC: VV020080.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	87	rVB	188871	187108	13.76%	1.728%
2	1.570	141	149	161	rBV	144908	157904	11.61%	1.458%
3	2.110	305	317	349	rBV	322368	486865	35.81%	4.496%
4	2.389	402	404	408	rVB2	236	145	0.01%	0.001%
5	2.512	434	442	452	rVB3	1267	2004	0.15%	0.019%
6	2.615	470	474	475	rBV2	329	220	0.02%	0.002%
7	2.759	515	519	521	rBV2	500	254	0.02%	0.002%
8	2.814	533	536	539	rVB2	270	195	0.01%	0.002%
9	2.852	545	548	550	rVV2	207	138	0.01%	0.001%
10	2.975	582	586	588	rBV	179	141	0.01%	0.001%
11	3.000	591	594	598	rVB	329	248	0.02%	0.002%
12	3.090	618	622	623	rBV	218	146	0.01%	0.001%
13	3.206	656	658	666	rVB	248	214	0.02%	0.002%
14	3.450	729	734	736	rBV2	205	162	0.01%	0.001%
15	3.496	746	748	752	rBV2	183	145	0.01%	0.001%
16	3.894	861	872	908	rBV2	78339	247013	18.17%	2.281%
17	4.351	998	1014	1046	rBV	223747	552479	40.63%	5.102%
18	4.528	1066	1069	1072	rBV	293	190	0.01%	0.002%
19	4.582	1083	1086	1088	rVB	219	140	0.01%	0.001%
20	4.643	1102	1105	1107	rBV2	204	137	0.01%	0.001%
21	4.656	1107	1109	1113	rVV2	312	228	0.02%	0.002%
22	4.679	1113	1116	1120	rVV2	381	252	0.02%	0.002%
23	4.717	1123	1128	1132	rBV2	355	277	0.02%	0.003%
24	4.740	1132	1135	1137	rVB	216	141	0.01%	0.001%
25	4.833	1160	1164	1165	rBV	254	184	0.01%	0.002%
26	4.875	1173	1177	1180	rBV2	223	185	0.01%	0.002%
27	4.917	1187	1190	1193	rBV2	266	195	0.01%	0.002%
28	4.939	1193	1197	1199	rBV2	169	140	0.01%	0.001%
29	4.981	1204	1210	1214	rBV2	312	494	0.04%	0.005%
30	5.048	1214	1231	1270	rBV2	527503	1359761	100.00%	12.558%
31	5.299	1307	1309	1312	rBV3	274	141	0.01%	0.001%
32	5.415	1341	1345	1350	rBV3	429	407	0.03%	0.004%
33	5.470	1359	1362	1365	rBV	199	160	0.01%	0.001%
34	5.524	1375	1379	1380	rBV	178	141	0.01%	0.001%
35	5.563	1387	1391	1393	rBV	185	137	0.01%	0.001%
36	5.621	1396	1409	1431	rBV	448335	898097	66.05%	8.294%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020080.D
 Acq On : 20 Jan 2021 16:59
 Operator : SY/MD
 Sample : M1147-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

37	5.907	1487	1498	1519	rBV3	28170	57878	4.26%	0.535%
38	6.074	1535	1550	1576	rBV	294526	596436	43.86%	5.508%
39	6.277	1610	1613	1618	rBV2	332	351	0.03%	0.003%
40	6.376	1641	1644	1646	rBV	237	170	0.01%	0.002%
41	6.563	1696	1702	1704	rBV2	193	222	0.02%	0.002%
42	6.605	1712	1715	1724	rVB2	224	268	0.02%	0.002%
43	6.650	1724	1729	1732	rBV2	316	284	0.02%	0.003%
44	6.730	1751	1754	1756	rBV2	185	137	0.01%	0.001%
45	6.881	1796	1801	1804	rBV2	249	292	0.02%	0.003%
46	6.987	1823	1834	1863	rBV	170595	312455	22.98%	2.886%
47	7.206	1898	1902	1904	rBV3	326	263	0.02%	0.002%
48	7.319	1922	1937	1961	rBV	651989	1136812	83.60%	10.499%
49	7.566	2011	2014	2018	rVB2	270	241	0.02%	0.002%
50	7.624	2021	2032	2058	rBV	117810	209517	15.41%	1.935%
51	7.862	2103	2106	2108	rBV	204	159	0.01%	0.001%
52	7.923	2119	2125	2130	rBV2	247	250	0.02%	0.002%
53	7.949	2130	2133	2138	rVB	256	173	0.01%	0.002%
54	7.984	2138	2144	2150	rBV2	850	1025	0.08%	0.009%
55	8.093	2168	2178	2214	rBV2	286350	561859	41.32%	5.189%
56	8.418	2276	2279	2281	rBV2	315	238	0.02%	0.002%
57	8.486	2298	2300	2304	rBV	305	246	0.02%	0.002%
58	8.650	2347	2351	2353	rBV	325	230	0.02%	0.002%
59	8.717	2369	2372	2377	rBV2	210	178	0.01%	0.002%
60	8.855	2403	2415	2443	rBV	694045	1111280	81.73%	10.263%
61	9.080	2484	2485	2490	rVB2	257	167	0.01%	0.002%
62	9.122	2495	2498	2503	rVB	457	276	0.02%	0.003%
63	9.151	2503	2507	2509	rBV2	570	441	0.03%	0.004%
64	9.199	2518	2522	2525	rBV	280	261	0.02%	0.002%
65	9.328	2558	2562	2565	rBV	314	330	0.02%	0.003%
66	9.357	2568	2571	2577	rVB	204	156	0.01%	0.001%
67	9.386	2577	2580	2582	rBV	180	147	0.01%	0.001%
68	9.521	2618	2622	2626	rBV2	243	230	0.02%	0.002%
69	9.759	2692	2696	2698	rBV	181	164	0.01%	0.002%
70	9.801	2706	2709	2714	rVB2	295	268	0.02%	0.002%
71	9.974	2760	2763	2765	rBV	223	157	0.01%	0.001%
72	10.164	2819	2822	2825	rBV2	261	190	0.01%	0.002%
73	10.222	2828	2840	2861	rVV	380853	591516	43.50%	5.463%
74	10.318	2868	2870	2875	rVB2	308	163	0.01%	0.002%
75	10.383	2888	2890	2894	rVB2	195	142	0.01%	0.001%
76	10.505	2925	2928	2936	rVB2	277	340	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020080.D
 Acq On : 20 Jan 2021 16:59
 Operator : SY/MD
 Sample : M1147-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

77	10.553	2939	2943	2945	rBV2	377	264	0.02%	0.002%
78	10.627	2963	2966	2970	rVB2	214	149	0.01%	0.001%
79	10.698	2982	2988	2990	rBV	247	288	0.02%	0.003%
80	10.830	3024	3029	3032	rBV2	283	219	0.02%	0.002%
81	10.923	3056	3058	3060	rBV2	342	194	0.01%	0.002%
82	11.000	3079	3082	3087	rBB2	215	162	0.01%	0.001%
83	11.026	3087	3090	3095	rBV2	277	285	0.02%	0.003%
84	11.164	3130	3133	3135	rBV2	377	207	0.02%	0.002%
85	11.196	3137	3143	3150	rVB5	1053	1250	0.09%	0.012%
86	11.257	3150	3162	3183	rBV	761901	1183481	87.04%	10.930%
87	11.630	3266	3278	3298	rBV	739850	1154272	84.89%	10.660%
88	11.817	3334	3336	3339	rBV2	332	224	0.02%	0.002%
89	11.833	3339	3341	3344	rVB	367	150	0.01%	0.001%
90	12.260	3471	3474	3479	rBV	326	318	0.02%	0.003%
91	12.469	3536	3539	3541	rBV2	249	175	0.01%	0.002%
92	12.518	3551	3554	3556	rBV	212	179	0.01%	0.002%
93	12.550	3562	3564	3567	rBV	313	197	0.01%	0.002%
94	12.649	3592	3595	3596	rBV2	483	301	0.02%	0.003%
95	12.759	3625	3629	3633	rBV2	383	339	0.02%	0.003%
96	12.785	3633	3637	3639	rBV2	231	187	0.01%	0.002%
97	13.280	3785	3791	3802	rVB5	1366	1948	0.14%	0.018%
98	13.791	3949	3950	3953	rBV	368	235	0.02%	0.002%
99	14.132	4054	4056	4058	rBV	259	141	0.01%	0.001%
100	14.598	4199	4201	4203	rBV	395	202	0.01%	0.002%




Sum of corrected areas: 10828067

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020080.D
Acq On : 20 Jan 2021 16:59
Operator : SY/MD
Sample : M1147-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

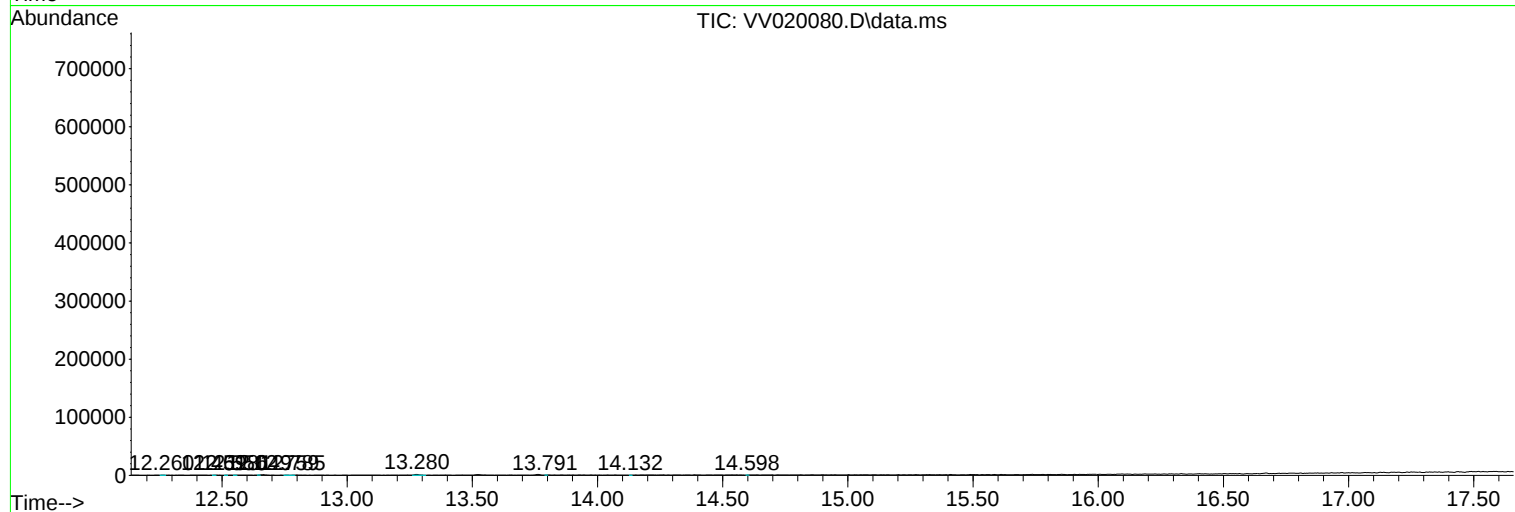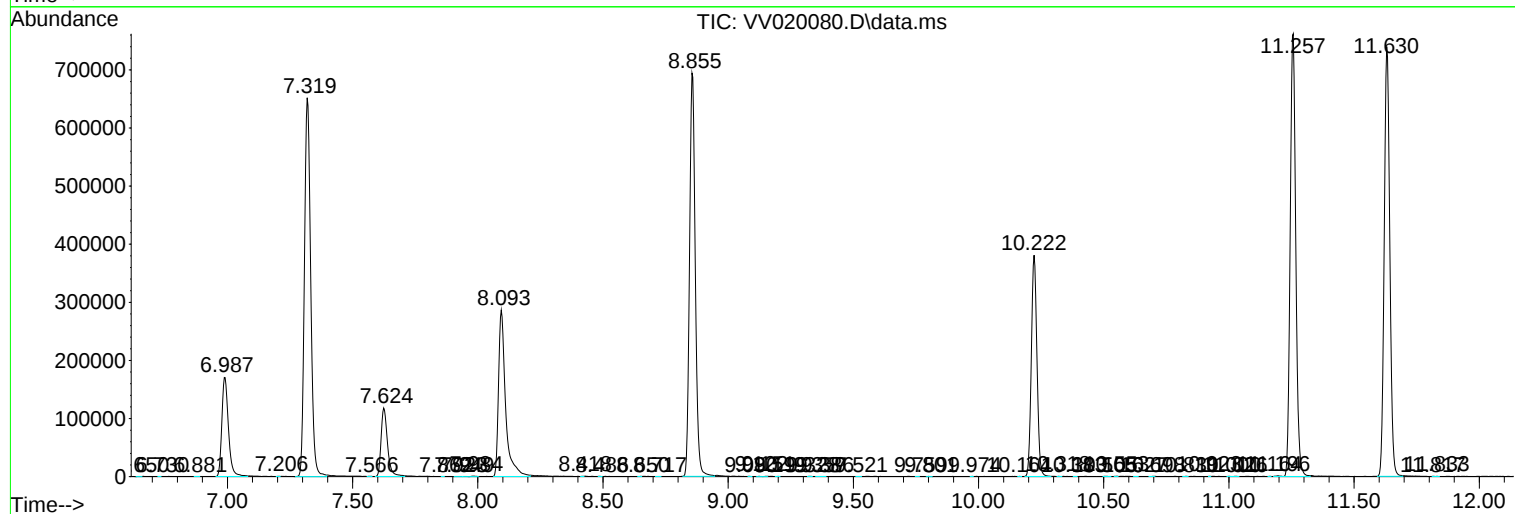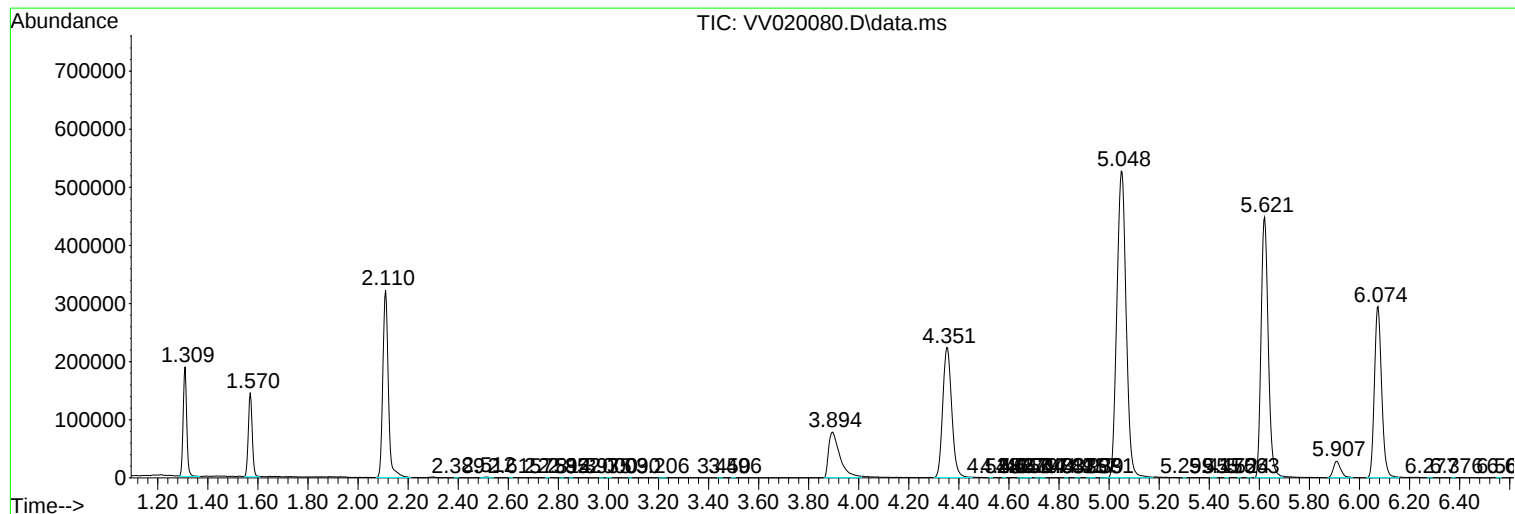

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020080.D
Acq On : 20 Jan 2021 16:59
Operator : SY/MD
Sample : M1147-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020080.D
Acq On : 20 Jan 2021 16:59
Operator : SY/MD
Sample : M1147-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
