

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020081.D
 Acq On : 20 Jan 2021 17:23
 Operator : SY/MD
 Sample : M1173-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

Signal : TIC: VV020081.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	83	rVB	182950	189489	3.85%	0.920%
2	1.569	141	149	163	rVB	145006	159267	3.24%	0.773%
3	1.859	236	239	241	rBV2	594	402	0.01%	0.002%
4	2.032	289	293	297	rBV3	559	522	0.01%	0.003%
5	2.068	302	304	306	rVV	410	235	0.00%	0.001%
6	2.110	306	317	345	rVV	323722	484614	9.85%	2.353%
7	2.248	356	360	365	rBV2	394	395	0.01%	0.002%
8	2.299	365	376	384	rVB3	1244	2188	0.04%	0.011%
9	2.512	436	442	443	rBV2	1321	1210	0.02%	0.006%
10	2.624	473	477	480	rBV2	712	611	0.01%	0.003%
11	2.685	490	496	502	rVB	324	483	0.01%	0.002%
12	2.769	517	522	526	rVV3	310	342	0.01%	0.002%
13	2.794	528	530	535	rVB2	326	239	0.00%	0.001%
14	3.039	601	606	611	rBV2	329	365	0.01%	0.002%
15	3.418	721	724	727	rVB2	293	218	0.00%	0.001%
16	3.479	740	743	752	rVB2	254	280	0.01%	0.001%
17	3.521	753	756	761	rVB2	242	200	0.00%	0.001%
18	3.563	762	769	770	rBV2	258	284	0.01%	0.001%
19	3.656	794	798	802	rBV2	187	195	0.00%	0.001%
20	3.724	816	819	823	rVB	289	237	0.00%	0.001%
21	3.769	826	833	835	rBV2	441	498	0.01%	0.002%
22	3.891	860	871	908	rBV	91496	272388	5.53%	1.323%
23	4.354	998	1015	1048	rBV	226889	564725	11.47%	2.742%
24	4.608	1089	1094	1095	rVV2	368	259	0.01%	0.001%
25	4.618	1095	1097	1100	rVV2	284	190	0.00%	0.001%
26	4.634	1100	1102	1105	rVB	360	202	0.00%	0.001%
27	4.656	1105	1109	1110	rBV	386	231	0.00%	0.001%
28	4.688	1115	1119	1123	rBV2	439	426	0.01%	0.002%
29	4.836	1155	1165	1177	rVB6	1994	4337	0.09%	0.021%
30	4.942	1191	1198	1201	rBV2	444	670	0.01%	0.003%
31	5.052	1214	1232	1242	rBV2	542488	1385482	28.15%	6.727%
32	5.380	1327	1334	1336	rBV3	446	493	0.01%	0.002%
33	5.405	1339	1342	1346	rBV2	456	400	0.01%	0.002%
34	5.479	1362	1365	1370	rVB3	409	328	0.01%	0.002%
35	5.621	1396	1409	1444	rBV	433868	856198	17.39%	4.157%
36	5.814	1467	1469	1473	rVB2	516	274	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012021\
 Data File : VW020081.D
 Acq On : 20 Jan 2021 17:23
 Operator : SY/MD
 Sample : M1173-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

37	5.910	1488	1499	1522	rVB2	18348	37790	0.77%	0.183%
38	6.074	1534	1550	1572	rBV	301403	607668	12.35%	2.950%
39	6.196	1584	1588	1590	rBV3	535	471	0.01%	0.002%
40	6.264	1607	1609	1614	rVB3	424	322	0.01%	0.002%
41	6.646	1725	1728	1732	rBV2	345	330	0.01%	0.002%
42	6.814	1778	1780	1785	rVB2	289	221	0.00%	0.001%
43	6.990	1823	1835	1861	rBV	175902	317252	6.45%	1.540%
44	7.251	1911	1916	1919	rBV3	278	261	0.01%	0.001%
45	7.322	1925	1938	1961	rBV	667014	1148871	23.34%	5.578%
46	7.495	1989	1992	1994	rBV2	365	267	0.01%	0.001%
47	7.624	2022	2032	2054	rBV	124971	214547	4.36%	1.042%
48	7.804	2085	2088	2092	rVB2	521	420	0.01%	0.002%
49	7.990	2139	2146	2152	rVB3	1102	1269	0.03%	0.006%
50	8.093	2167	2178	2213	rBV	324979	608230	12.36%	2.953%
51	8.344	2253	2256	2259	rBV3	473	256	0.01%	0.001%
52	8.884	2403	2424	2451	rBV2	2439397	4922110	100.00%	23.898%
53	9.125	2496	2499	2502	rBB3	287	195	0.00%	0.001%
54	9.325	2558	2561	2567	rBV2	308	300	0.01%	0.001%
55	9.350	2567	2569	2573	rVV2	283	191	0.00%	0.001%
56	9.373	2573	2576	2580	rVB	308	226	0.00%	0.001%
57	9.392	2580	2582	2586	rBV2	379	217	0.00%	0.001%
58	9.447	2595	2599	2601	rBV	288	279	0.01%	0.001%
59	9.553	2627	2632	2634	rBV2	428	420	0.01%	0.002%
60	9.604	2646	2648	2652	rVB	403	220	0.00%	0.001%
61	9.630	2652	2656	2658	rBV	219	193	0.00%	0.001%
62	9.672	2665	2669	2674	rBV2	225	263	0.01%	0.001%
63	9.788	2699	2705	2709	rBV	335	358	0.01%	0.002%
64	9.842	2719	2722	2728	rVV2	252	247	0.01%	0.001%
65	10.129	2807	2811	2813	rBV	281	227	0.00%	0.001%
66	10.222	2828	2840	2859	rBV	409127	637648	12.95%	3.096%
67	10.498	2918	2926	2928	rBV2	290	370	0.01%	0.002%
68	10.543	2938	2940	2945	rVB2	414	322	0.01%	0.002%
69	10.977	3070	3075	3078	rBV2	215	250	0.01%	0.001%
70	11.096	3109	3112	3116	rBV2	276	242	0.00%	0.001%
71	11.190	3128	3141	3151	rBV	185990	292789	5.95%	1.422%
72	11.276	3151	3168	3190	rVB2	1453483	3284789	66.74%	15.948%
73	11.492	3233	3235	3240	rVB2	323	227	0.00%	0.001%
74	11.550	3249	3253	3255	rBV2	325	325	0.01%	0.002%
75	11.649	3266	3284	3305	rBV2	1921036	3850806	78.23%	18.697%
76	11.804	3331	3332	3335	rVB2	609	279	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020081.D
 Acq On : 20 Jan 2021 17:23
 Operator : SY/MD
 Sample : M1173-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

77	11.820	3335	3337	3341	rVB2	444	320	0.01%	0.002%
78	11.852	3341	3347	3350	rBV2	454	524	0.01%	0.003%
79	12.157	3436	3442	3443	rBV2	319	293	0.01%	0.001%
80	12.241	3463	3468	3474	rBV2	299	249	0.01%	0.001%
81	12.328	3492	3495	3497	rVB2	355	214	0.00%	0.001%
82	12.405	3514	3519	3520	rBV2	1298	912	0.02%	0.004%
83	12.582	3572	3574	3577	rVB2	427	240	0.00%	0.001%
84	12.659	3591	3598	3606	rVB6	2044	2772	0.06%	0.013%
85	12.694	3606	3609	3613	rBV	257	281	0.01%	0.001%
86	12.765	3625	3631	3635	rBV3	893	1122	0.02%	0.005%
87	13.048	3717	3719	3722	rBV	274	199	0.00%	0.001%
88	13.202	3763	3767	3773	rVB2	278	302	0.01%	0.001%
89	13.270	3776	3788	3806	rBV	375898	567870	11.54%	2.757%
90	13.386	3822	3824	3829	rVB	379	209	0.00%	0.001%
91	13.518	3856	3865	3873	rBV4	1797	2769	0.06%	0.013%
92	13.752	3928	3938	3954	rVB	96728	146745	2.98%	0.712%
93	13.948	3996	3999	4003	rVB	560	423	0.01%	0.002%
94	14.119	4051	4052	4057	rBV2	317	240	0.00%	0.001%
95	14.736	4242	4244	4247	rBV	333	195	0.00%	0.001%
96	14.833	4270	4274	4281	rVB5	1513	1716	0.03%	0.008%
97	15.411	4445	4454	4462	rBV5	4604	6551	0.13%	0.032%
98	15.472	4470	4473	4476	rBV2	506	416	0.01%	0.002%
99	15.492	4477	4479	4482	rBV2	560	439	0.01%	0.002%
100	16.144	4678	4682	4684	rBV3	887	680	0.01%	0.003%




Sum of corrected areas: 20596226

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020081.D
Acq On : 20 Jan 2021 17:23
Operator : SY/MD
Sample : M1173-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

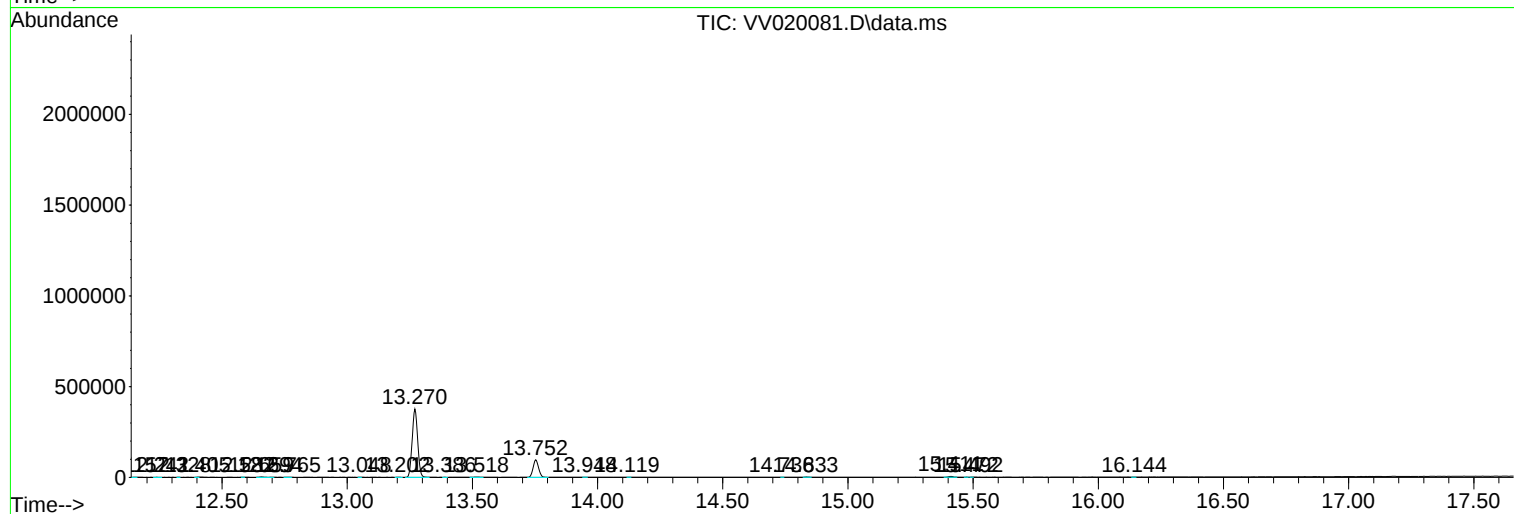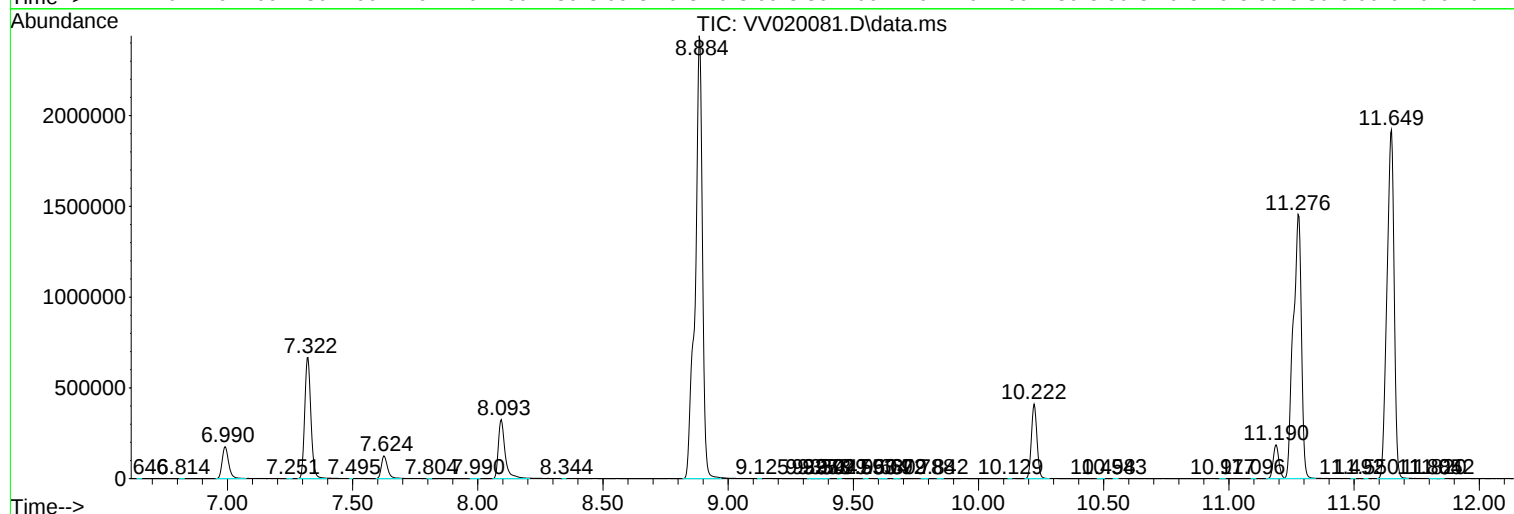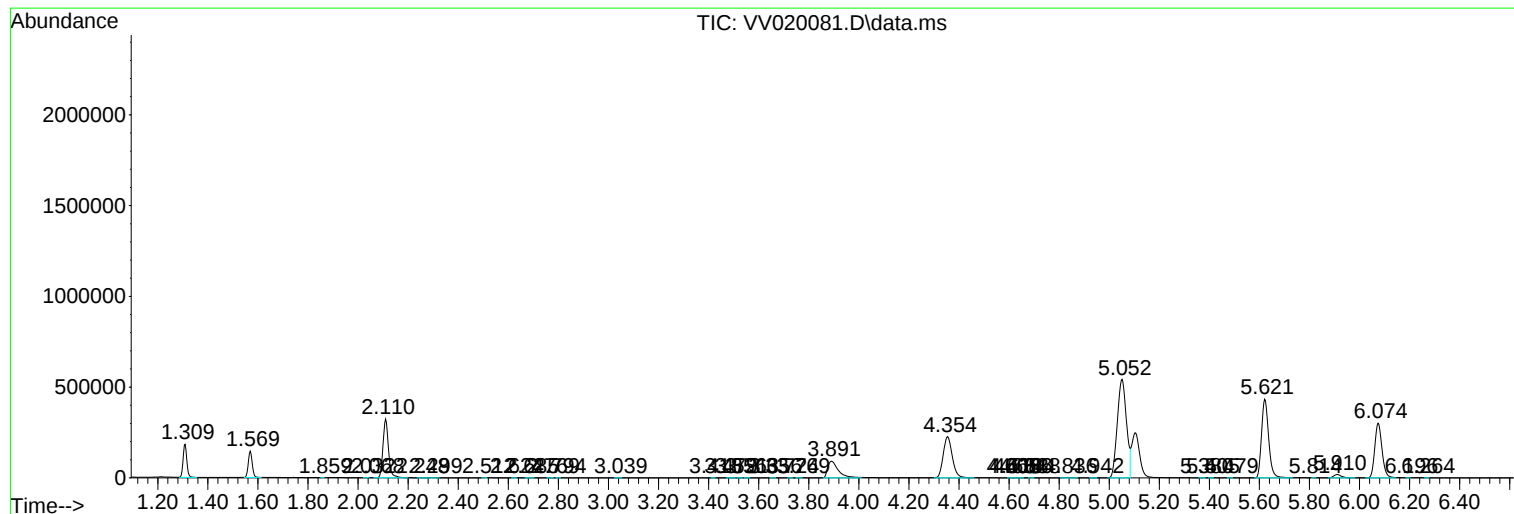

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020081.D
Acq On : 20 Jan 2021 17:23
Operator : SY/MD
Sample : M1173-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020081.D
Acq On : 20 Jan 2021 17:23
Operator : SY/MD
Sample : M1173-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
