

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020082.D
 Acq On : 20 Jan 2021 17:46
 Operator : SY/MD
 Sample : VIBLK61
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

Signal : TIC: VV020082.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	79	rVB	184951	183913	13.15%	1.677%
2	1.569	141	149	165	rVB	140556	157749	11.28%	1.438%
3	2.110	306	317	343	rVB	322050	484553	34.64%	4.418%
4	2.270	363	367	368	rBV	244	156	0.01%	0.001%
5	2.344	388	390	393	rBV2	227	140	0.01%	0.001%
6	2.360	393	395	397	rVB	319	137	0.01%	0.001%
7	2.515	436	443	451	rVB5	1493	2352	0.17%	0.021%
8	2.585	462	465	468	rBV3	384	303	0.02%	0.003%
9	2.621	471	476	477	rBV2	615	394	0.03%	0.004%
10	2.675	488	493	495	rVB2	223	189	0.01%	0.002%
11	2.756	515	518	521	rBV	243	168	0.01%	0.002%
12	2.801	530	532	533	rBV2	362	145	0.01%	0.001%
13	2.955	576	580	584	rVB2	235	226	0.02%	0.002%
14	2.984	584	589	594	rVB	195	120	0.01%	0.001%
15	3.036	600	605	611	rBV2	190	246	0.02%	0.002%
16	3.296	680	686	690	rVB2	249	281	0.02%	0.003%
17	3.328	690	696	700	rBV2	226	208	0.01%	0.002%
18	3.360	700	706	709	rBV2	260	239	0.02%	0.002%
19	3.383	709	713	715	rBV2	179	136	0.01%	0.001%
20	3.470	735	740	746	rVB2	162	198	0.01%	0.002%
21	3.518	749	755	757	rBV2	240	236	0.02%	0.002%
22	3.592	775	778	781	rVB2	165	119	0.01%	0.001%
23	3.634	787	791	796	rBV2	385	391	0.03%	0.004%
24	3.801	841	843	848	rBV2	151	149	0.01%	0.001%
25	3.849	854	858	861	rVB	279	176	0.01%	0.002%
26	3.891	861	871	905	rBV	90210	273392	19.54%	2.493%
27	4.354	998	1015	1049	rBV	228912	565457	40.42%	5.156%
28	4.605	1090	1093	1095	rBV2	269	151	0.01%	0.001%
29	4.659	1106	1110	1115	rBV2	415	403	0.03%	0.004%
30	4.682	1115	1117	1118	rBV	286	145	0.01%	0.001%
31	4.724	1128	1130	1132	rVB	274	126	0.01%	0.001%
32	4.753	1135	1139	1141	rBV	256	179	0.01%	0.002%
33	4.843	1163	1167	1170	rBV2	250	183	0.01%	0.002%
34	4.859	1170	1172	1176	rBV2	300	133	0.01%	0.001%
35	4.900	1182	1185	1188	rVB2	291	197	0.01%	0.002%
36	4.920	1188	1191	1194	rBV	248	189	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020082.D
 Acq On : 20 Jan 2021 17:46
 Operator : SY/MD
 Sample : VIBLK61
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

37	4.978	1206	1209	1210	rBV	267	169	0.01%	0.002%
38	5.052	1214	1232	1269	rBV2	546952	1398826	100.00%	12.754%
39	5.534	1379	1382	1386	rVB2	424	281	0.02%	0.003%
40	5.569	1390	1393	1396	rVB2	202	169	0.01%	0.002%
41	5.621	1396	1409	1439	rBV	438399	869271	62.14%	7.926%
42	5.910	1488	1499	1515	rBV3	29333	59971	4.29%	0.547%
43	6.074	1536	1550	1571	rBV	303144	609619	43.58%	5.558%
44	6.309	1620	1623	1627	rVB2	246	197	0.01%	0.002%
45	6.360	1635	1639	1643	rVB2	398	318	0.02%	0.003%
46	6.386	1644	1647	1651	rBV2	195	161	0.01%	0.001%
47	6.431	1657	1661	1664	rVB2	288	266	0.02%	0.002%
48	6.476	1670	1675	1681	rBV2	338	419	0.03%	0.004%
49	6.534	1689	1693	1697	rBV2	133	130	0.01%	0.001%
50	6.714	1746	1749	1752	rBV	274	202	0.01%	0.002%
51	6.772	1761	1767	1769	rBV2	171	135	0.01%	0.001%
52	6.868	1791	1797	1803	rVB2	259	386	0.03%	0.004%
53	6.900	1803	1807	1811	rBV	437	341	0.02%	0.003%
54	6.990	1824	1835	1859	rBV	176249	316364	22.62%	2.884%
55	7.322	1925	1938	1959	rBV	662308	1154394	82.53%	10.525%
56	7.627	2022	2033	2061	rVV	125263	217879	15.58%	1.987%
57	7.759	2072	2074	2076	rVB2	432	134	0.01%	0.001%
58	7.884	2111	2113	2117	rVB2	232	156	0.01%	0.001%
59	7.913	2117	2122	2125	rBV2	323	302	0.02%	0.003%
60	7.984	2138	2144	2145	rBV3	723	615	0.04%	0.006%
61	8.019	2153	2155	2160	rVB	261	177	0.01%	0.002%
62	8.048	2160	2164	2165	rBV	238	182	0.01%	0.002%
63	8.093	2168	2178	2218	rBV2	319169	619311	44.27%	5.647%
64	8.392	2267	2271	2272	rBV2	389	230	0.02%	0.002%
65	8.514	2306	2309	2314	rBV	250	212	0.02%	0.002%
66	8.788	2391	2394	2397	rBV2	215	159	0.01%	0.001%
67	8.858	2403	2416	2449	rBV	660542	1087846	77.77%	9.918%
68	9.267	2540	2543	2545	rBV2	255	169	0.01%	0.002%
69	9.363	2569	2573	2577	rBV2	249	281	0.02%	0.003%
70	9.428	2589	2593	2595	rBV2	308	229	0.02%	0.002%
71	9.566	2633	2636	2639	rBV	337	314	0.02%	0.003%
72	9.637	2655	2658	2661	rVB2	215	127	0.01%	0.001%
73	9.694	2673	2676	2681	rBV2	289	320	0.02%	0.003%
74	9.717	2681	2683	2686	rVV	360	203	0.01%	0.002%
75	9.756	2691	2695	2698	rBV2	287	214	0.02%	0.002%
76	9.852	2721	2725	2727	rBV2	215	185	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020082.D
 Acq On : 20 Jan 2021 17:46
 Operator : SY/MD
 Sample : VIBLK61
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

77	9.948	2748	2755	2760	rVB2	541	621	0.04%	0.006%
78	10.084	2794	2797	2798	rBV2	244	160	0.01%	0.001%
79	10.154	2816	2819	2822	rBV	274	223	0.02%	0.002%
80	10.222	2828	2840	2863	rBV	394581	619014	44.25%	5.644%
81	10.334	2872	2875	2876	rBV2	236	171	0.01%	0.002%
82	10.415	2897	2900	2904	rVB	279	163	0.01%	0.001%
83	10.434	2904	2906	2908	rBV	192	130	0.01%	0.001%
84	10.746	3000	3003	3005	rBV2	233	138	0.01%	0.001%
85	10.784	3013	3015	3017	rBV	268	182	0.01%	0.002%
86	10.842	3029	3033	3039	rVB2	319	357	0.03%	0.003%
87	10.871	3039	3042	3044	rBV	284	212	0.02%	0.002%
88	10.923	3056	3058	3061	rBV	372	292	0.02%	0.003%
89	11.257	3150	3162	3184	rBV	733243	1143902	81.78%	10.430%
90	11.540	3246	3250	3254	rBV2	352	333	0.02%	0.003%
91	11.630	3265	3278	3303	rBV	739566	1177853	84.20%	10.739%
92	11.804	3330	3332	3333	rBV	354	146	0.01%	0.001%
93	12.170	3444	3446	3449	rBV	246	158	0.01%	0.001%
94	12.501	3546	3549	3552	rBV	362	253	0.02%	0.002%
95	12.804	3641	3643	3651	rVB2	321	326	0.02%	0.003%
96	13.003	3702	3705	3707	rBV	258	194	0.01%	0.002%
97	13.093	3731	3733	3735	rBV	195	117	0.01%	0.001%
98	13.273	3783	3789	3799	rBV4	5355	7748	0.55%	0.071%
99	13.495	3855	3858	3860	rBV	445	334	0.02%	0.003%
100	14.019	4018	4021	4026	rBV3	531	522	0.04%	0.005%




Sum of corrected areas: 10967892

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020082.D
Acq On : 20 Jan 2021 17:46
Operator : SY/MD
Sample : VIBLK61
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

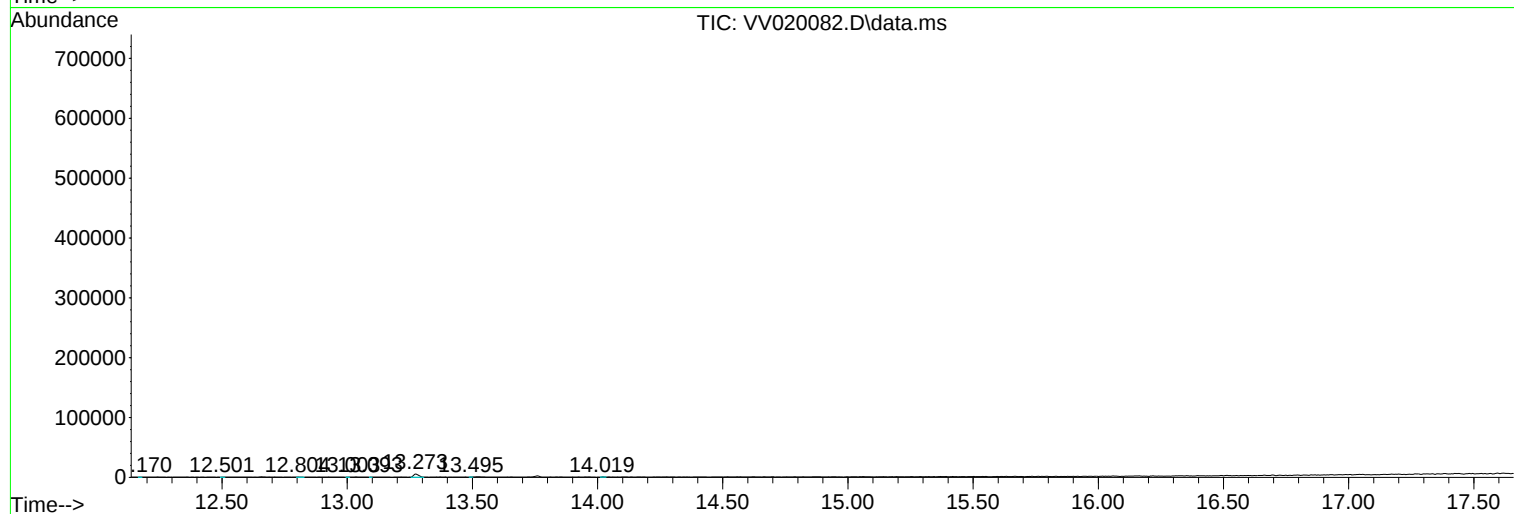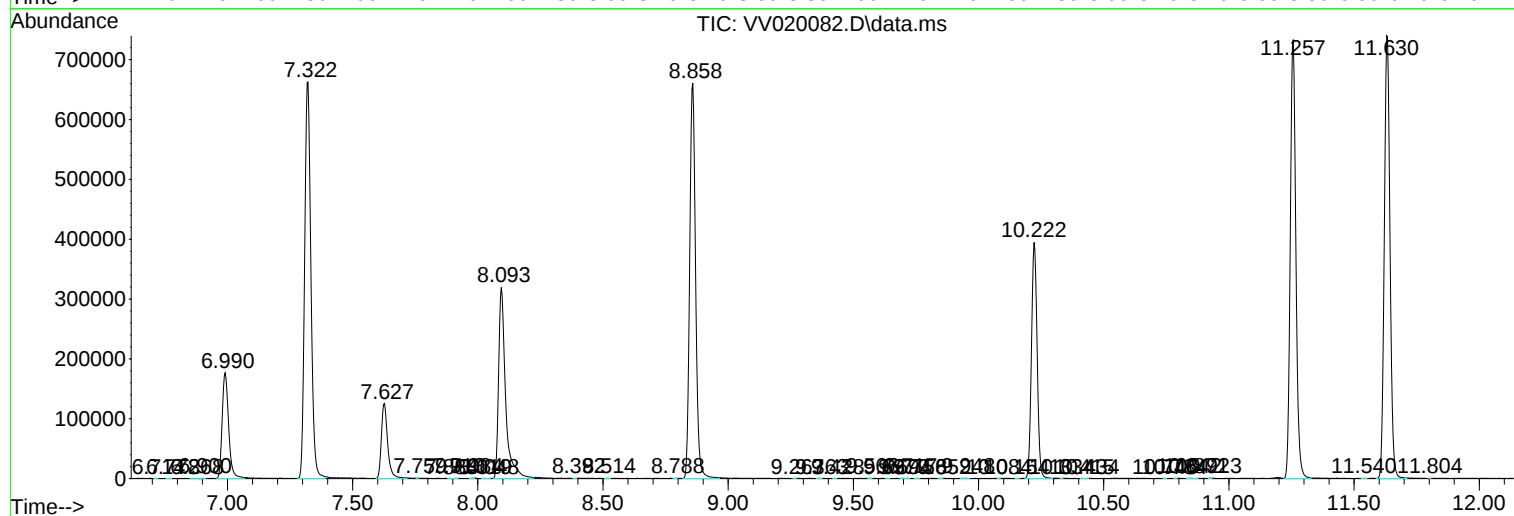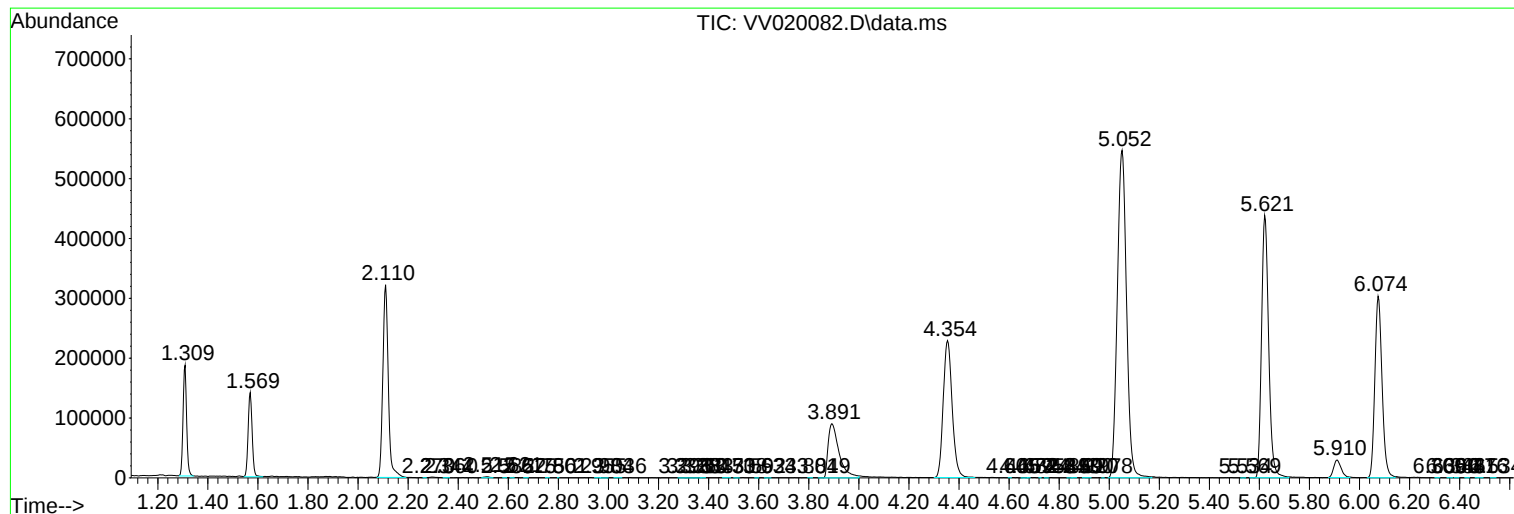

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020082.D
Acq On : 20 Jan 2021 17:46
Operator : SY/MD
Sample : VIBLK61
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020082.D
Acq On : 20 Jan 2021 17:46
Operator : SY/MD
Sample : VIBLK61
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
