

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020084.D
 Acq On : 20 Jan 2021 18:33
 Operator : SY/MD
 Sample : VIBLK62
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

Signal : TIC: VV020084.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	79	rVB	183706	187320	13.30%	1.678%
2	1.569	141	149	163	rBV	148638	164011	11.65%	1.469%
3	2.110	307	317	348	rVB	326319	491670	34.92%	4.404%
4	2.261	361	364	367	rBV2	235	168	0.01%	0.002%
5	2.360	393	395	399	rVB	321	188	0.01%	0.002%
6	2.383	399	402	406	rVB	348	253	0.02%	0.002%
7	2.511	437	442	448	rVV2	1320	1735	0.12%	0.016%
8	2.540	449	451	459	rVB2	458	373	0.03%	0.003%
9	2.765	516	521	522	rBV2	290	219	0.02%	0.002%
10	2.823	536	539	542	rVB	187	142	0.01%	0.001%
11	2.849	544	547	551	rVV	251	188	0.01%	0.002%
12	2.897	560	562	566	rBV2	181	136	0.01%	0.001%
13	2.978	581	587	592	rVB2	272	380	0.03%	0.003%
14	3.010	594	597	602	rBV	224	157	0.01%	0.001%
15	3.084	613	620	624	rBV2	167	201	0.01%	0.002%
16	3.177	642	649	652	rBV2	162	223	0.02%	0.002%
17	3.267	672	677	678	rBV	210	192	0.01%	0.002%
18	3.344	698	701	704	rBV	185	143	0.01%	0.001%
19	3.392	711	716	719	rBV2	280	291	0.02%	0.003%
20	3.463	735	738	743	rBV2	208	199	0.01%	0.002%
21	3.659	797	799	805	rBV2	291	254	0.02%	0.002%
22	3.688	805	808	813	rBV2	207	215	0.02%	0.002%
23	3.836	848	854	857	rBV2	220	200	0.01%	0.002%
24	3.891	860	871	905	rBV2	92647	279810	19.87%	2.506%
25	4.248	979	982	985	rBV2	347	251	0.02%	0.002%
26	4.354	999	1015	1044	rBV	228804	566415	40.23%	5.073%
27	4.637	1099	1103	1109	rBV2	308	324	0.02%	0.003%
28	4.672	1109	1114	1118	rBV3	355	390	0.03%	0.003%
29	4.688	1118	1119	1124	rVB2	238	144	0.01%	0.001%
30	4.714	1124	1127	1132	rVB	270	250	0.02%	0.002%
31	4.743	1132	1136	1139	rBV	294	278	0.02%	0.002%
32	4.897	1179	1184	1186	rBV	295	278	0.02%	0.002%
33	4.955	1195	1202	1208	rBV2	262	425	0.03%	0.004%
34	5.052	1215	1232	1260	rBV2	546998	1408071	100.00%	12.612%
35	5.338	1316	1321	1322	rBV2	392	324	0.02%	0.003%
36	5.543	1381	1385	1390	rBV	171	213	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020084.D
 Acq On : 20 Jan 2021 18:33
 Operator : SY/MD
 Sample : VIBLK62
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

37	5.621	1397	1409	1436	rBV	450613	894863	63.55%	8.015%
38	5.797	1461	1464	1469	rBV3	742	525	0.04%	0.005%
39	5.910	1488	1499	1521	rVB2	27957	57021	4.05%	0.511%
40	6.026	1530	1535	1537	rBV2	301	315	0.02%	0.003%
41	6.074	1537	1550	1579	rVV	304449	613832	43.59%	5.498%
42	6.302	1619	1621	1623	rBV	288	138	0.01%	0.001%
43	6.344	1630	1634	1639	rVB3	246	235	0.02%	0.002%
44	6.373	1639	1643	1647	rBV2	219	208	0.01%	0.002%
45	6.572	1702	1705	1709	rBV2	238	210	0.01%	0.002%
46	6.608	1713	1716	1719	rVB	242	177	0.01%	0.002%
47	6.730	1750	1754	1755	rBV	295	140	0.01%	0.001%
48	6.842	1786	1789	1792	rBV	301	270	0.02%	0.002%
49	6.894	1803	1805	1808	rBV2	194	143	0.01%	0.001%
50	6.939	1815	1819	1824	rVB2	269	275	0.02%	0.002%
51	6.990	1824	1835	1862	rBV	176957	323101	22.95%	2.894%
52	7.174	1888	1892	1896	rBV3	450	410	0.03%	0.004%
53	7.196	1896	1899	1902	rBV3	306	234	0.02%	0.002%
54	7.264	1918	1920	1922	rBV	277	140	0.01%	0.001%
55	7.322	1925	1938	1965	rBV	672637	1169566	83.06%	10.476%
56	7.627	2023	2033	2060	rBV	126696	217608	15.45%	1.949%
57	7.804	2083	2088	2094	rBV4	475	471	0.03%	0.004%
58	7.839	2097	2099	2102	rVB	318	159	0.01%	0.001%
59	7.907	2118	2120	2124	rBV	181	135	0.01%	0.001%
60	8.029	2154	2158	2161	rBV3	314	323	0.02%	0.003%
61	8.093	2168	2178	2214	rBV3	324362	625663	44.43%	5.604%
62	8.334	2251	2253	2258	rVB3	528	264	0.02%	0.002%
63	8.428	2280	2282	2285	rBV	315	200	0.01%	0.002%
64	8.585	2328	2331	2334	rBV2	341	224	0.02%	0.002%
65	8.688	2359	2363	2366	rBV2	149	138	0.01%	0.001%
66	8.858	2404	2416	2444	rBV	676967	1114348	79.14%	9.981%
67	9.135	2498	2502	2504	rBV	360	255	0.02%	0.002%
68	9.193	2517	2520	2522	rBV2	220	181	0.01%	0.002%
69	9.260	2537	2541	2542	rBV2	203	153	0.01%	0.001%
70	9.395	2579	2583	2586	rBV2	331	242	0.02%	0.002%
71	9.463	2601	2604	2608	rBV	213	232	0.02%	0.002%
72	9.537	2621	2627	2629	rBV	310	332	0.02%	0.003%
73	9.588	2641	2643	2645	rVB	292	152	0.01%	0.001%
74	9.611	2646	2650	2653	rBV2	244	252	0.02%	0.002%
75	9.682	2670	2672	2675	rBV	260	179	0.01%	0.002%
76	9.714	2679	2682	2685	rBV	216	205	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020084.D
 Acq On : 20 Jan 2021 18:33
 Operator : SY/MD
 Sample : VIBLK62
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

77	9.781	2700	2703	2705	rBV2	207	175	0.01%	0.002%
78	9.974	2761	2763	2769	rVB2	305	270	0.02%	0.002%
79	10.003	2769	2772	2777	rBV2	281	322	0.02%	0.003%
80	10.222	2826	2840	2860	rBV	406371	630953	44.81%	5.651%
81	10.315	2865	2869	2874	rVB2	504	369	0.03%	0.003%
82	10.347	2874	2879	2881	rBV2	214	209	0.01%	0.002%
83	10.492	2922	2924	2928	rBV	246	139	0.01%	0.001%
84	10.547	2938	2941	2947	rVB2	527	473	0.03%	0.004%
85	10.575	2947	2950	2954	rBV	266	194	0.01%	0.002%
86	10.640	2965	2970	2975	rBV2	202	268	0.02%	0.002%
87	11.202	3134	3145	3150	rBV3	1098	1944	0.14%	0.017%
88	11.257	3150	3162	3183	rBV	759263	1174947	83.44%	10.524%
89	11.630	3266	3278	3297	rBV	739939	1193679	84.77%	10.692%
90	11.791	3325	3328	3334	rVB2	655	534	0.04%	0.005%
91	11.826	3334	3339	3343	rBV2	349	429	0.03%	0.004%
92	11.936	3369	3373	3376	rBV2	281	284	0.02%	0.003%
93	12.505	3547	3550	3552	rBV2	217	179	0.01%	0.002%
94	12.743	3620	3624	3626	rBV2	295	262	0.02%	0.002%
95	12.948	3684	3688	3698	rBV2	333	527	0.04%	0.005%
96	13.009	3704	3707	3709	rBV2	265	190	0.01%	0.002%
97	13.273	3781	3789	3800	rVB3	10920	16668	1.18%	0.149%
98	13.344	3805	3811	3813	rBV	455	449	0.03%	0.004%
99	13.607	3890	3893	3895	rBV	369	220	0.02%	0.002%
100	13.755	3931	3939	3950	rVB5	7222	11173	0.79%	0.100%




Sum of corrected areas: 11164407

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020084.D
Acq On : 20 Jan 2021 18:33
Operator : SY/MD
Sample : VIBLK62
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

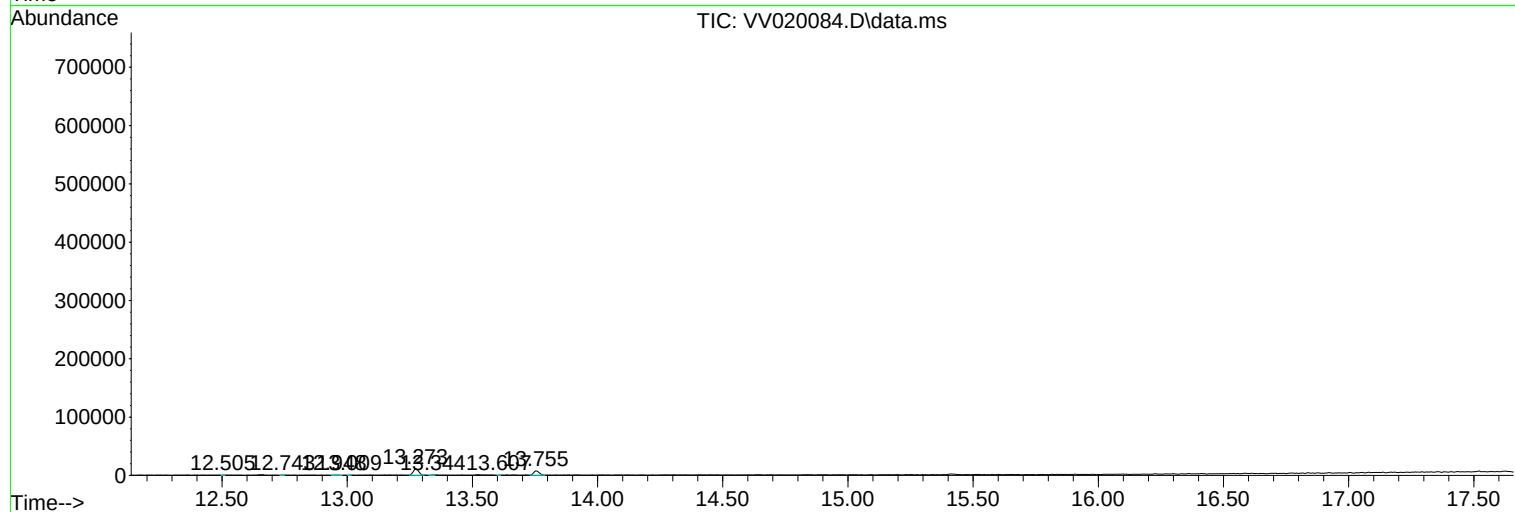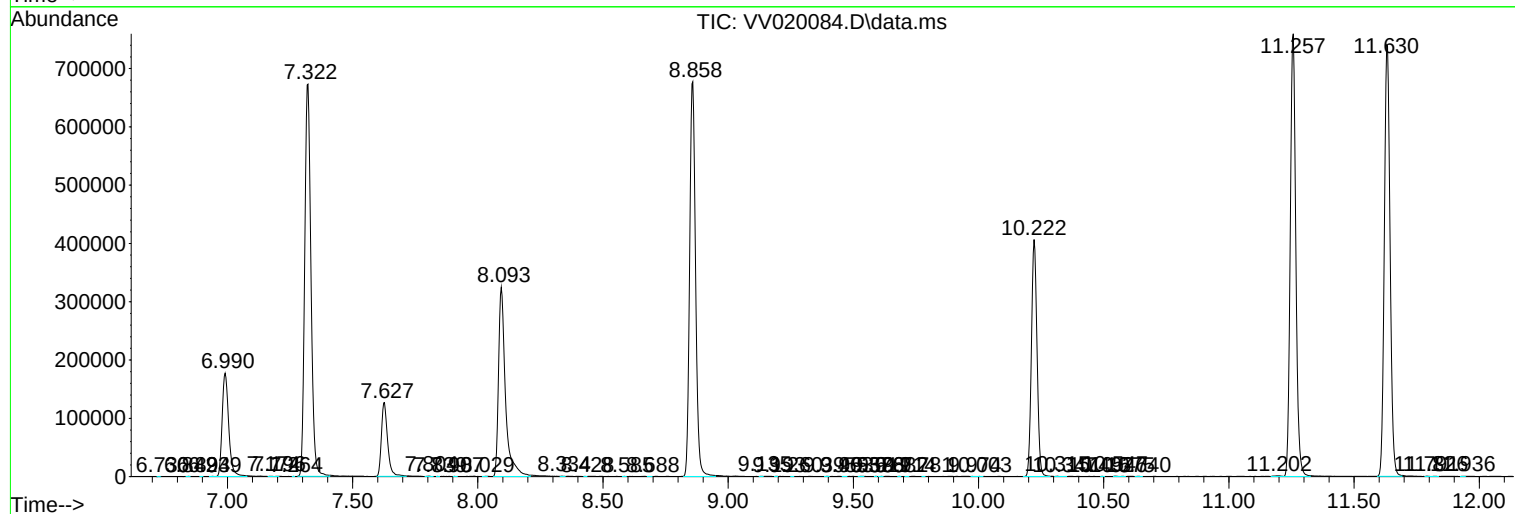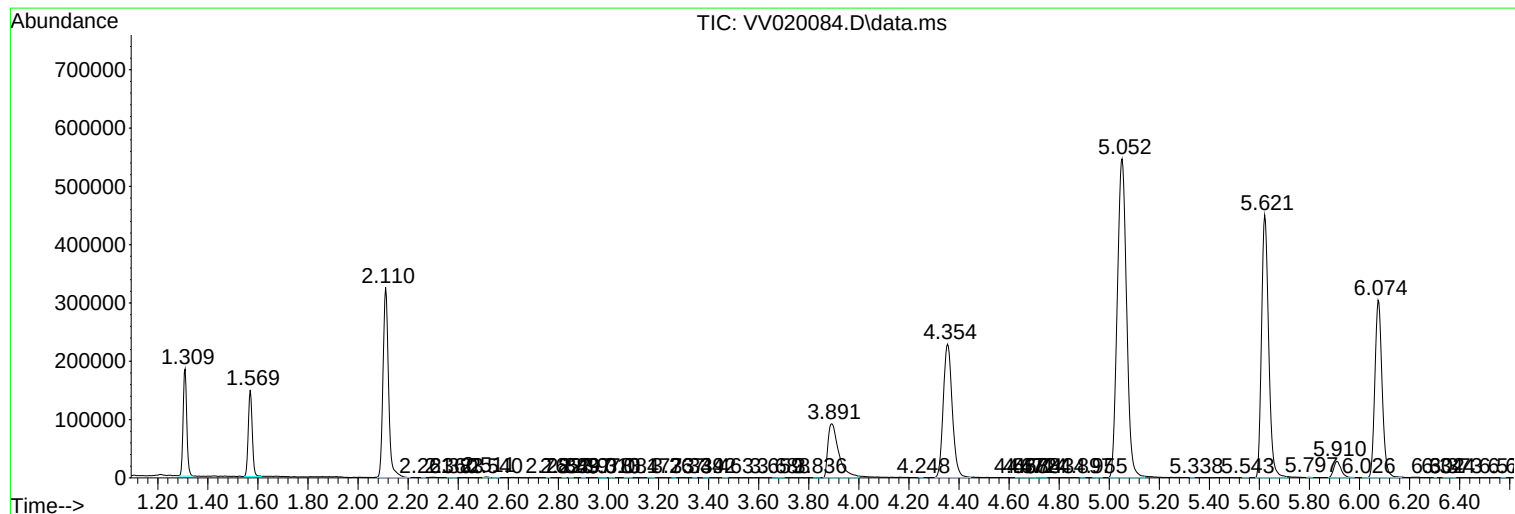

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020084.D
Acq On : 20 Jan 2021 18:33
Operator : SY/MD
Sample : VIBLK62
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020084.D
Acq On : 20 Jan 2021 18:33
Operator : SY/MD
Sample : VIBLK62
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
