

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020086.D
 Acq On : 20 Jan 2021 19:20
 Operator : SY/MD
 Sample : M1181-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

Signal : TIC: VV020086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	85	rVB	181517	184806	13.31%	1.724%
2	1.569	141	149	161	rBV	134721	153926	11.09%	1.436%
3	2.110	306	317	340	rBV	323892	485571	34.98%	4.529%
4	2.338	385	388	391	rBB3	315	192	0.01%	0.002%
5	2.370	395	398	401	rBV2	296	205	0.01%	0.002%
6	2.399	405	407	409	rBV2	190	110	0.01%	0.001%
7	2.447	419	422	426	rBV3	330	263	0.02%	0.002%
8	2.482	430	433	438	rBV2	381	291	0.02%	0.003%
9	2.515	438	443	449	rBV2	598	767	0.06%	0.007%
10	2.872	547	554	555	rBV	266	221	0.02%	0.002%
11	3.068	612	615	617	rBV	192	141	0.01%	0.001%
12	3.100	622	625	630	rVV2	226	232	0.02%	0.002%
13	3.193	649	654	657	rBV	177	177	0.01%	0.002%
14	3.216	657	661	664	rVV2	197	155	0.01%	0.001%
15	3.335	694	698	701	rBV	313	310	0.02%	0.003%
16	3.380	707	712	715	rBV2	170	220	0.02%	0.002%
17	3.425	723	726	728	rBV	167	125	0.01%	0.001%
18	3.450	731	734	738	rVB	322	252	0.02%	0.002%
19	3.544	757	763	766	rBV2	197	230	0.02%	0.002%
20	3.624	785	788	791	rBV	333	295	0.02%	0.003%
21	3.659	795	799	802	rBV2	292	275	0.02%	0.003%
22	3.724	816	819	823	rBV2	163	147	0.01%	0.001%
23	3.814	842	847	850	rBV	182	216	0.02%	0.002%
24	3.888	859	870	903	rBV	89292	251625	18.12%	2.347%
25	4.283	990	993	994	rBV	306	206	0.01%	0.002%
26	4.354	998	1015	1041	rVV	227372	555768	40.03%	5.183%
27	4.566	1078	1081	1085	rBV2	388	361	0.03%	0.003%
28	4.611	1092	1095	1100	rVB2	386	265	0.02%	0.002%
29	4.634	1100	1102	1106	rVV	215	115	0.01%	0.001%
30	4.656	1106	1109	1111	rVV	238	146	0.01%	0.001%
31	4.669	1111	1113	1116	rVB2	218	108	0.01%	0.001%
32	4.717	1124	1128	1134	rBV3	399	409	0.03%	0.004%
33	4.749	1134	1138	1141	rBV	238	203	0.01%	0.002%
34	4.888	1177	1181	1183	rBV2	302	217	0.02%	0.002%
35	4.942	1194	1198	1201	rBV	213	197	0.01%	0.002%
36	5.052	1214	1232	1259	rBV2	541836	1388327	100.00%	12.948%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020086.D
 Acq On : 20 Jan 2021 19:20
 Operator : SY/MD
 Sample : M1181-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

37	5.293	1305	1307	1308	rBV	338	159	0.01%	0.001%
38	5.402	1338	1341	1344	rBV2	414	253	0.02%	0.002%
39	5.418	1344	1346	1351	rVB2	252	208	0.01%	0.002%
40	5.444	1351	1354	1356	rBV	137	97	0.01%	0.001%
41	5.482	1363	1366	1367	rBV	157	107	0.01%	0.001%
42	5.621	1395	1409	1433	rBV	432685	861987	62.09%	8.039%
43	5.910	1487	1499	1515	rBV3	37863	77048	5.55%	0.719%
44	6.074	1537	1550	1574	rBV	299337	607977	43.79%	5.670%
45	6.206	1588	1591	1594	rBV2	696	552	0.04%	0.005%
46	6.251	1603	1605	1612	rVB3	391	448	0.03%	0.004%
47	6.296	1615	1619	1624	rVB3	282	289	0.02%	0.003%
48	6.322	1624	1627	1630	rBV2	244	224	0.02%	0.002%
49	6.376	1641	1644	1647	rVB2	290	160	0.01%	0.001%
50	6.392	1647	1649	1652	rVB	252	131	0.01%	0.001%
51	6.412	1652	1655	1659	rBV2	215	215	0.02%	0.002%
52	6.431	1659	1661	1664	rBV2	243	171	0.01%	0.002%
53	6.640	1723	1726	1728	rBV	237	184	0.01%	0.002%
54	6.672	1734	1736	1741	rBV	340	262	0.02%	0.002%
55	6.830	1780	1785	1786	rBV2	201	147	0.01%	0.001%
56	6.842	1786	1789	1792	rVV	335	194	0.01%	0.002%
57	6.868	1794	1797	1798	rBV	273	130	0.01%	0.001%
58	6.923	1811	1814	1819	rBV2	225	238	0.02%	0.002%
59	6.990	1824	1835	1857	rBV	172716	312578	22.51%	2.915%
60	7.322	1925	1938	1961	rBV	658415	1137201	81.91%	10.606%
61	7.627	2022	2033	2061	rBV	120055	209905	15.12%	1.958%
62	7.826	2093	2095	2098	rBV	285	207	0.01%	0.002%
63	7.855	2102	2104	2111	rBV2	220	177	0.01%	0.002%
64	7.920	2118	2124	2127	rBV2	329	363	0.03%	0.003%
65	7.984	2140	2144	2150	rBV3	696	753	0.05%	0.007%
66	8.093	2168	2178	2211	rBV2	289076	586722	42.26%	5.472%
67	8.440	2283	2286	2287	rBV2	207	106	0.01%	0.001%
68	8.550	2317	2320	2323	rBV2	302	264	0.02%	0.002%
69	8.678	2357	2360	2362	rBV2	225	176	0.01%	0.002%
70	8.723	2371	2374	2378	rVB2	205	172	0.01%	0.002%
71	8.858	2404	2416	2447	rBV	660425	1066044	76.79%	9.943%
72	9.241	2532	2535	2538	rBV	270	217	0.02%	0.002%
73	9.260	2538	2541	2546	rVV	258	236	0.02%	0.002%
74	9.473	2601	2607	2608	rBV	257	255	0.02%	0.002%
75	9.598	2643	2646	2649	rBV2	332	286	0.02%	0.003%
76	9.711	2678	2681	2682	rBV	220	109	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020086.D
 Acq On : 20 Jan 2021 19:20
 Operator : SY/MD
 Sample : M1181-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

77	9.762	2695	2697	2700	rBV2	161	118	0.01%	0.001%
78	9.990	2764	2768	2772	rVV2	191	181	0.01%	0.002%
79	10.045	2780	2785	2789	rBV2	236	238	0.02%	0.002%
80	10.145	2814	2816	2819	rBV	233	147	0.01%	0.001%
81	10.222	2828	2840	2860	rBV	372817	580580	41.82%	5.415%
82	10.338	2872	2876	2880	rBV2	333	319	0.02%	0.003%
83	10.376	2885	2888	2890	rBV2	356	183	0.01%	0.002%
84	10.437	2903	2907	2909	rVV2	309	238	0.02%	0.002%
85	10.604	2956	2959	2960	rBV	251	142	0.01%	0.001%
86	10.755	3004	3006	3009	rVB	205	100	0.01%	0.001%
87	10.936	3056	3062	3065	rBV	381	367	0.03%	0.003%
88	11.103	3110	3114	3121	rBV	256	347	0.02%	0.003%
89	11.202	3139	3145	3148	rVB4	686	757	0.05%	0.007%
90	11.257	3148	3162	3182	rBV	705440	1099278	79.18%	10.253%
91	11.514	3239	3242	3244	rBV2	230	178	0.01%	0.002%
92	11.630	3267	3278	3298	rBV	715943	1140239	82.13%	10.635%
93	11.890	3357	3359	3362	rBV	265	115	0.01%	0.001%
94	12.090	3419	3421	3424	rBV2	175	103	0.01%	0.001%
95	12.379	3508	3511	3513	rBV	288	210	0.02%	0.002%
96	12.611	3579	3583	3586	rBV	331	263	0.02%	0.002%
97	13.177	3754	3759	3761	rBV	329	317	0.02%	0.003%
98	13.273	3783	3789	3796	rBV5	1714	2523	0.18%	0.024%
99	13.437	3838	3840	3847	rVB3	526	482	0.03%	0.004%
100	13.752	3934	3938	3939	rBV2	790	542	0.04%	0.005%




Sum of corrected areas: 10721993

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020086.D
Acq On : 20 Jan 2021 19:20
Operator : SY/MD
Sample : M1181-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

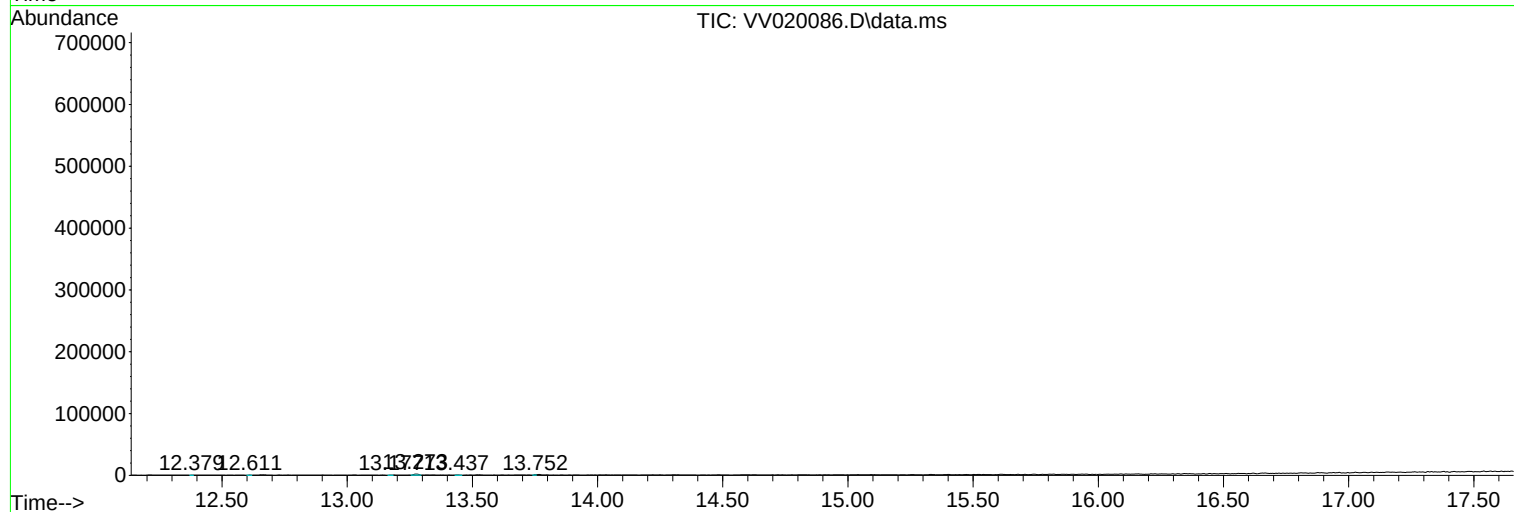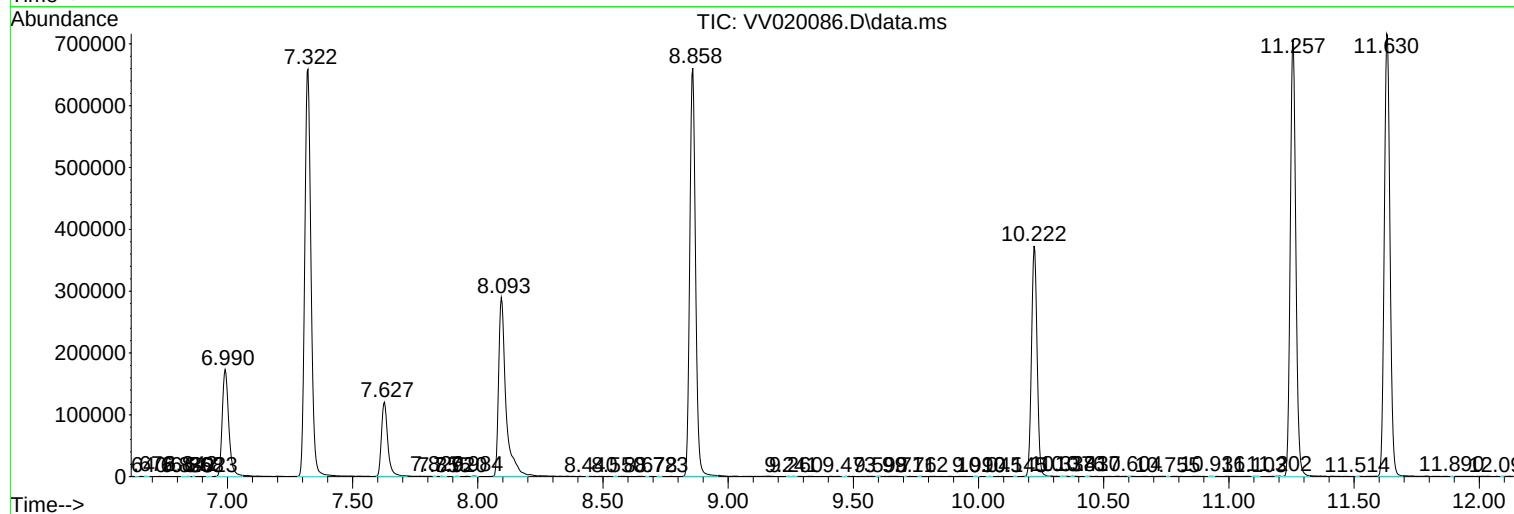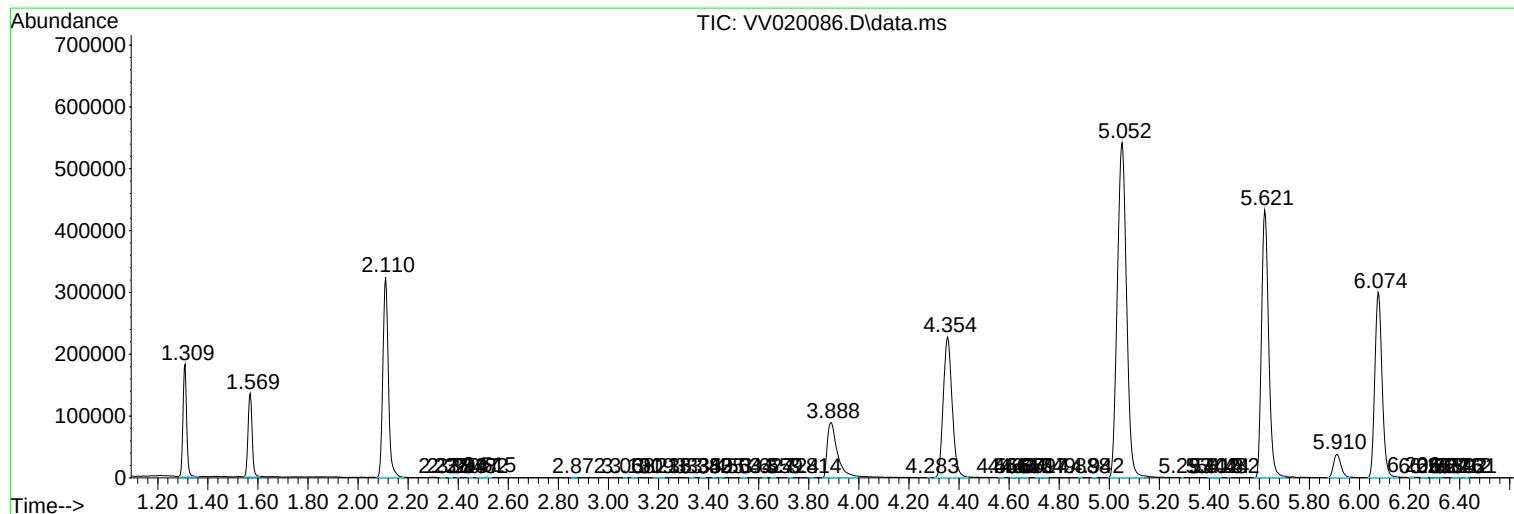

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020086.D
Acq On : 20 Jan 2021 19:20
Operator : SY/MD
Sample : M1181-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020086.D
Acq On : 20 Jan 2021 19:20
Operator : SY/MD
Sample : M1181-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
