

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020087.D
 Acq On : 20 Jan 2021 19:44
 Operator : SY/MD
 Sample : M1181-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

Signal : TIC: VV020087.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	61	69	89	rVB	2833496	2883874	27.22%	12.005%
2	1.569	143	149	166	rVB	141405	172089	1.62%	0.716%
3	2.110	308	317	339	rVB	317018	474881	4.48%	1.977%
4	2.299	370	376	387	rBV2	6129	10486	0.10%	0.044%
5	2.762	508	520	543	rBV	122716	215791	2.04%	0.898%
6	2.901	559	563	568	rBV3	425	473	0.00%	0.002%
7	2.952	576	579	585	rBV3	320	335	0.00%	0.001%
8	3.065	609	614	616	rBV2	346	275	0.00%	0.001%
9	3.081	617	619	622	rVV2	406	260	0.00%	0.001%
10	3.103	622	626	630	rVB	202	217	0.00%	0.001%
11	3.190	645	653	655	rBV2	1099	1115	0.01%	0.005%
12	3.264	674	676	679	rBV	220	142	0.00%	0.001%
13	3.331	694	697	698	rBV2	205	127	0.00%	0.001%
14	3.351	701	703	706	rVB2	182	94	0.00%	0.000%
15	3.399	713	718	722	rVB2	259	274	0.00%	0.001%
16	3.425	724	726	730	rBV	122	108	0.00%	0.000%
17	3.579	771	774	777	rBV	156	116	0.00%	0.000%
18	3.640	787	793	794	rBV2	239	238	0.00%	0.001%
19	3.730	818	821	822	rBV	204	98	0.00%	0.000%
20	3.814	836	847	848	rBV2	5190	5360	0.05%	0.022%
21	3.913	859	878	915	rBV	4357641	10596349	100.00%	44.111%
22	4.354	1000	1015	1043	rVB2	237668	582669	5.50%	2.426%
23	4.708	1122	1125	1128	rBV2	283	149	0.00%	0.001%
24	4.724	1128	1130	1133	rBV	184	126	0.00%	0.001%
25	4.749	1133	1138	1141	rBV3	281	281	0.00%	0.001%
26	4.827	1159	1162	1165	rVB2	204	134	0.00%	0.001%
27	4.862	1170	1173	1178	rVB3	390	363	0.00%	0.002%
28	4.949	1197	1200	1202	rBV	174	109	0.00%	0.000%
29	5.052	1214	1232	1276	rBV2	531221	1382522	13.05%	5.755%
30	5.351	1322	1325	1327	rVB	370	197	0.00%	0.001%
31	5.370	1328	1331	1334	rBV	368	293	0.00%	0.001%
32	5.495	1367	1370	1373	rVB2	632	419	0.00%	0.002%
33	5.511	1373	1375	1376	rBV	282	118	0.00%	0.000%
34	5.621	1396	1409	1444	rBV	422286	840174	7.93%	3.497%
35	5.913	1488	1500	1513	rBV5	20111	46217	0.44%	0.192%
36	6.023	1532	1534	1537	rBV	348	175	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020087.D
 Acq On : 20 Jan 2021 19:44
 Operator : SY/MD
 Sample : M1181-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

37	6.074	1537	1550	1576	rBV2	298168	599693	5.66%	2.496%
38	6.286	1612	1616	1619	rBV	265	228	0.00%	0.001%
39	6.344	1629	1634	1636	rBV2	159	153	0.00%	0.001%
40	6.383	1642	1646	1648	rBV	294	272	0.00%	0.001%
41	6.627	1720	1722	1725	rBV2	194	156	0.00%	0.001%
42	6.714	1744	1749	1750	rBV	215	189	0.00%	0.001%
43	6.743	1755	1758	1760	rBV2	236	94	0.00%	0.000%
44	6.810	1776	1779	1782	rBV2	324	213	0.00%	0.001%
45	6.852	1788	1792	1796	rVB2	206	194	0.00%	0.001%
46	6.884	1799	1802	1804	rBV2	240	161	0.00%	0.001%
47	6.942	1818	1820	1822	rVB	318	112	0.00%	0.000%
48	6.990	1823	1835	1859	rBV	172392	308244	2.91%	1.283%
49	7.219	1903	1906	1908	rBV2	419	225	0.00%	0.001%
50	7.248	1912	1915	1918	rBV3	475	328	0.00%	0.001%
51	7.322	1924	1938	1953	rBV	653071	1124402	10.61%	4.681%
52	7.576	2015	2017	2020	rBV	310	201	0.00%	0.001%
53	7.624	2022	2032	2063	rVV	119089	207697	1.96%	0.865%
54	7.826	2093	2095	2097	rBV2	199	96	0.00%	0.000%
55	7.984	2141	2144	2152	rVB3	822	792	0.01%	0.003%
56	8.016	2152	2154	2156	rBV2	200	117	0.00%	0.000%
57	8.093	2168	2178	2219	rBV3	286242	565131	5.33%	2.353%
58	8.415	2276	2278	2281	rVB3	371	178	0.00%	0.001%
59	8.434	2283	2284	2287	rBV	180	93	0.00%	0.000%
60	8.524	2308	2312	2314	rBV2	353	232	0.00%	0.001%
61	8.669	2355	2357	2359	rBV2	197	134	0.00%	0.001%
62	8.723	2364	2374	2387	rVV3	5925	10520	0.10%	0.044%
63	8.859	2404	2416	2446	rBV	647020	1057521	9.98%	4.402%
64	9.100	2488	2491	2493	rBV	276	156	0.00%	0.001%
65	9.151	2497	2507	2521	rVV2	11923	20443	0.19%	0.085%
66	9.251	2536	2538	2539	rBV2	282	107	0.00%	0.000%
67	9.553	2621	2632	2641	rBV4	6191	9385	0.09%	0.039%
68	9.662	2664	2666	2669	rBV2	226	143	0.00%	0.001%
69	9.698	2674	2677	2678	rBV2	239	144	0.00%	0.001%
70	9.820	2712	2715	2717	rBV	187	106	0.00%	0.000%
71	9.894	2735	2738	2739	rBV	220	136	0.00%	0.001%
72	10.026	2770	2779	2799	rVB2	12600	24135	0.23%	0.100%
73	10.100	2799	2802	2803	rBV	320	170	0.00%	0.001%
74	10.222	2829	2840	2859	rBV	408042	627296	5.92%	2.611%
75	10.309	2865	2867	2868	rBV2	310	113	0.00%	0.000%
76	10.386	2881	2891	2892	rBV4	1952	1934	0.02%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020087.D
 Acq On : 20 Jan 2021 19:44
 Operator : SY/MD
 Sample : M1181-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

77	10.457	2906	2913	2914	rBV3	720	570	0.01%	0.002%
78	10.682	2980	2983	2987	rBV	301	236	0.00%	0.001%
79	10.887	3044	3047	3048	rBV	317	168	0.00%	0.001%
80	10.926	3052	3059	3069	rVV3	1638	2668	0.03%	0.011%
81	11.010	3081	3085	3093	rVB2	362	382	0.00%	0.002%
82	11.055	3093	3099	3100	rBV2	239	203	0.00%	0.001%
83	11.093	3105	3111	3115	rVB3	1114	929	0.01%	0.004%
84	11.186	3133	3140	3141	rBV2	944	890	0.01%	0.004%
85	11.257	3150	3162	3179	rBV	695606	1088167	10.27%	4.530%
86	11.408	3205	3209	3210	rBV	540	359	0.00%	0.001%
87	11.501	3235	3238	3241	rVB	291	129	0.00%	0.001%
88	11.527	3241	3246	3247	rBV	612	443	0.00%	0.002%
89	11.630	3266	3278	3295	rBV	716659	1140943	10.77%	4.750%
90	11.752	3315	3316	3318	rBV2	314	127	0.00%	0.001%
91	12.190	3449	3452	3458	rBV2	258	258	0.00%	0.001%
92	12.842	3647	3655	3661	rBV3	2524	3486	0.03%	0.015%
93	13.083	3726	3730	3732	rBV	338	258	0.00%	0.001%
94	13.100	3732	3735	3739	rBV	263	222	0.00%	0.001%
95	13.122	3739	3742	3743	rBV	287	143	0.00%	0.001%
96	13.276	3785	3790	3798	rVB6	1971	2141	0.02%	0.009%
97	13.569	3877	3881	3885	rBV2	469	538	0.01%	0.002%
98	13.704	3920	3923	3924	rBV2	401	262	0.00%	0.001%
99	13.839	3963	3965	3967	rBV2	525	273	0.00%	0.001%
100	14.045	4027	4029	4031	rBV	308	163	0.00%	0.001%




Sum of corrected areas: 24022250

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020087.D
Acq On : 20 Jan 2021 19:44
Operator : SY/MD
Sample : M1181-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

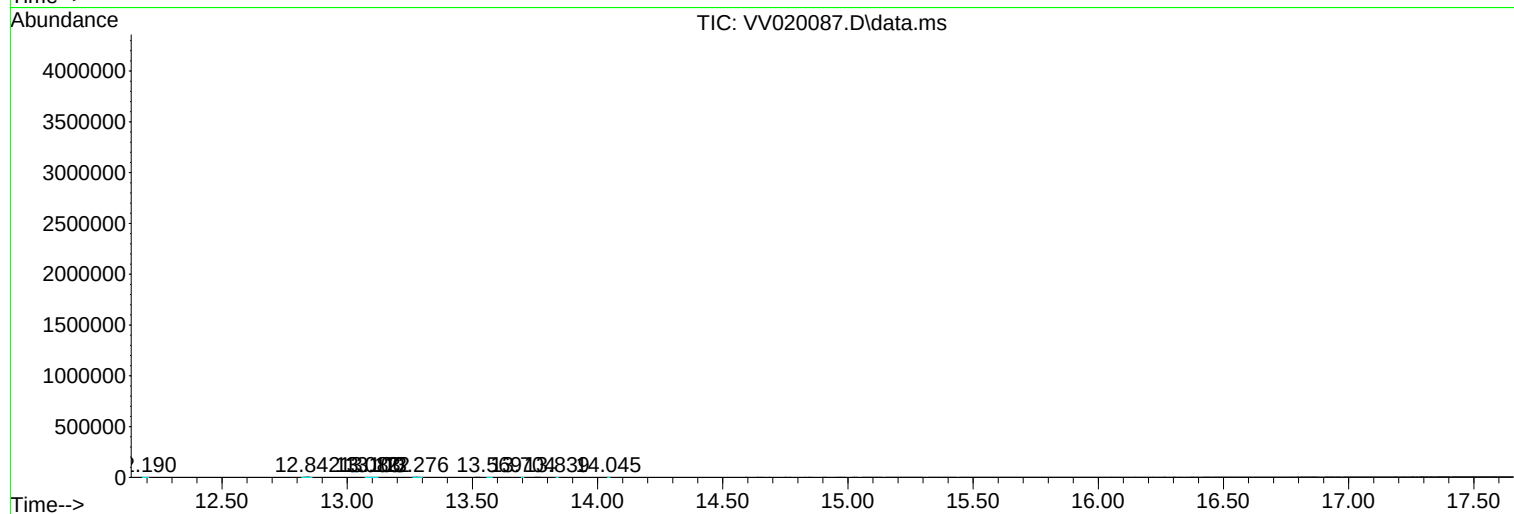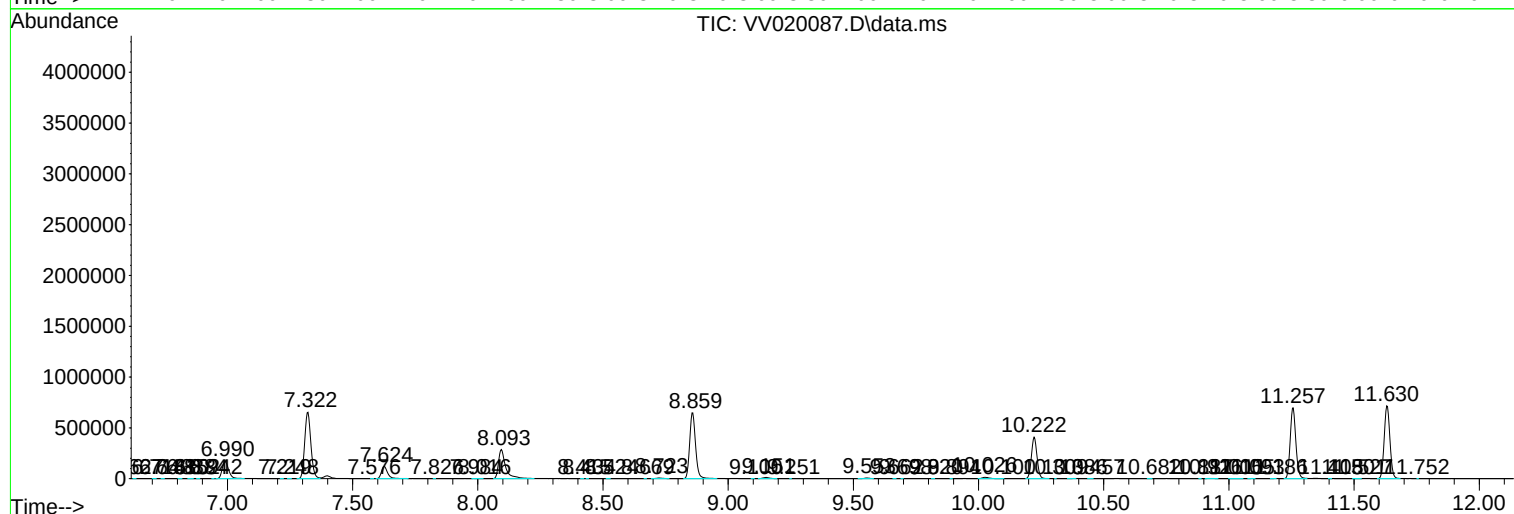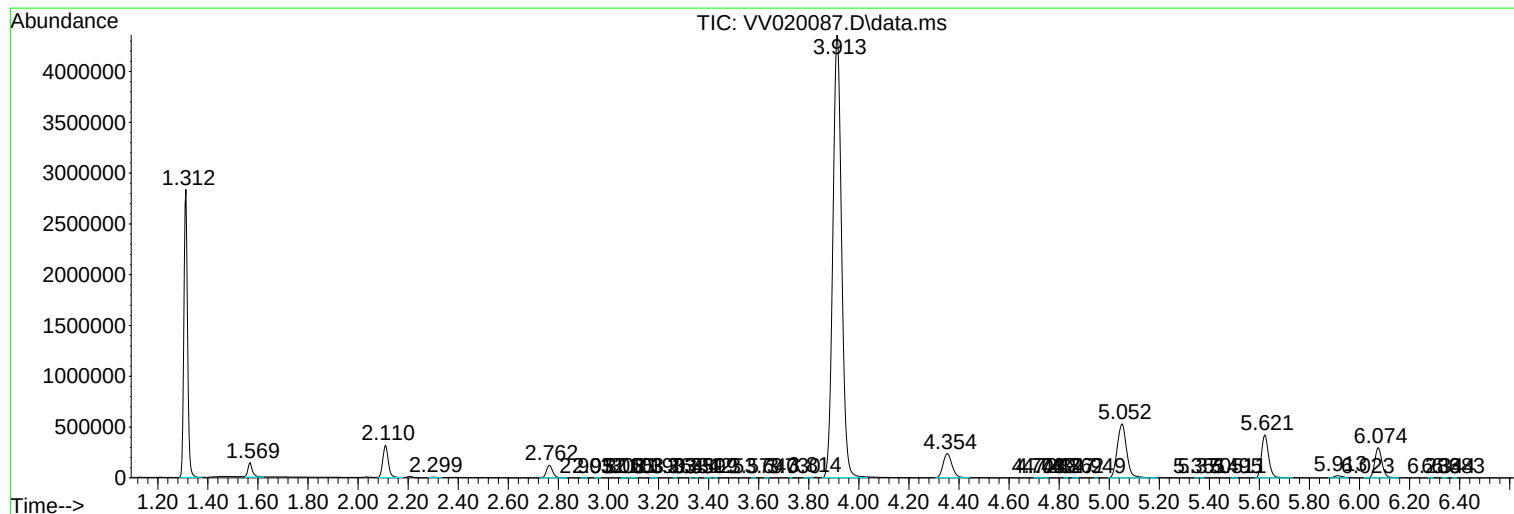

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020087.D
Acq On : 20 Jan 2021 19:44
Operator : SY/MD
Sample : M1181-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020087.D
Acq On : 20 Jan 2021 19:44
Operator : SY/MD
Sample : M1181-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
