

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020088.D
 Acq On : 20 Jan 2021 20:07
 Operator : SY/MD
 Sample : M1181-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

Signal : TIC: VV020088.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	61	69	88	rVB	3346816	3423520	22.52%	11.604%
2	1.569	143	149	166	rVB2	147610	190546	1.25%	0.646%
3	2.110	308	317	339	rVB	332471	496518	3.27%	1.683%
4	2.302	368	377	385	rBV2	4193	7694	0.05%	0.026%
5	2.765	510	521	541	rBV	119697	211537	1.39%	0.717%
6	2.888	554	559	561	rBV2	434	362	0.00%	0.001%
7	3.019	595	600	603	rBV4	411	464	0.00%	0.002%
8	3.135	630	636	645	rBV2	334	578	0.00%	0.002%
9	3.177	646	649	650	rBV2	460	315	0.00%	0.001%
10	3.248	668	671	674	rBV	172	128	0.00%	0.000%
11	3.386	709	714	717	rBV2	279	229	0.00%	0.001%
12	3.470	737	740	743	rBV	239	141	0.00%	0.000%
13	3.502	743	750	752	rBV2	308	325	0.00%	0.001%
14	3.563	764	769	771	rBV2	288	224	0.00%	0.001%
15	3.579	771	774	777	rVB2	228	141	0.00%	0.000%
16	3.601	777	781	783	rBV2	274	255	0.00%	0.001%
17	3.637	790	792	796	rBV2	171	164	0.00%	0.001%
18	3.688	805	808	816	rVB2	267	280	0.00%	0.001%
19	3.727	816	820	827	rBV2	301	340	0.00%	0.001%
20	3.769	831	833	835	rBV	211	116	0.00%	0.000%
21	3.823	839	850	859	rBV4	5125	10963	0.07%	0.037%
22	3.913	860	878	931	rBV	6307208	15201422	100.00%	51.524%
23	4.354	1001	1015	1048	rVB	243251	596071	3.92%	2.020%
24	4.759	1139	1141	1142	rBV2	490	224	0.00%	0.001%
25	4.820	1155	1160	1162	rVB4	273	177	0.00%	0.001%
26	4.836	1164	1165	1168	rVB	326	100	0.00%	0.000%
27	4.913	1187	1189	1194	rVB	323	219	0.00%	0.001%
28	4.987	1208	1212	1214	rBV	169	110	0.00%	0.000%
29	5.051	1214	1232	1264	rBV2	555354	1436156	9.45%	4.868%
30	5.399	1334	1340	1341	rBV	339	351	0.00%	0.001%
31	5.486	1365	1367	1368	rBV	271	129	0.00%	0.000%
32	5.527	1377	1380	1383	rVB2	251	137	0.00%	0.000%
33	5.543	1383	1385	1387	rVB	232	94	0.00%	0.000%
34	5.621	1397	1409	1434	rBV	431211	856802	5.64%	2.904%
35	5.871	1486	1487	1489	rBV2	281	113	0.00%	0.000%
36	5.913	1489	1500	1520	rVB6	18129	41664	0.27%	0.141%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020088.D
 Acq On : 20 Jan 2021 20:07
 Operator : SY/MD
 Sample : M1181-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

37	5.994	1520	1525	1526	rBV	494	294	0.00%	0.001%
38	6.074	1537	1550	1584	rBV	304823	625617	4.12%	2.120%
39	6.277	1612	1613	1615	rBV	246	117	0.00%	0.000%
40	6.350	1633	1636	1638	rBV	219	95	0.00%	0.000%
41	6.604	1712	1715	1720	rVB	313	171	0.00%	0.001%
42	6.643	1723	1727	1731	rBV3	263	238	0.00%	0.001%
43	6.695	1740	1743	1746	rBV	255	177	0.00%	0.001%
44	6.817	1778	1781	1784	rVB2	184	136	0.00%	0.000%
45	6.846	1784	1790	1791	rBV2	284	226	0.00%	0.001%
46	6.990	1823	1835	1861	rBV	177100	319694	2.10%	1.084%
47	7.225	1904	1908	1913	rBV3	288	272	0.00%	0.001%
48	7.254	1915	1917	1921	rVB3	281	189	0.00%	0.001%
49	7.322	1925	1938	1954	rBV	673933	1165145	7.66%	3.949%
50	7.576	2014	2017	2020	rBV2	290	205	0.00%	0.001%
51	7.627	2022	2033	2062	rVV	122990	214114	1.41%	0.726%
52	7.801	2083	2087	2088	rBV	511	311	0.00%	0.001%
53	7.891	2112	2115	2117	rBV	275	184	0.00%	0.001%
54	7.939	2123	2130	2132	rBV3	730	779	0.01%	0.003%
55	8.093	2167	2178	2216	rBV2	308626	602157	3.96%	2.041%
56	8.338	2251	2254	2255	rBV	411	188	0.00%	0.001%
57	8.569	2322	2326	2330	rBV	335	293	0.00%	0.001%
58	8.643	2346	2349	2352	rBV2	348	192	0.00%	0.001%
59	8.730	2365	2376	2384	rBV4	3866	6950	0.05%	0.024%
60	8.858	2404	2416	2444	rBV	658392	1076848	7.08%	3.650%
61	9.083	2483	2486	2489	rBV	575	387	0.00%	0.001%
62	9.151	2492	2507	2519	rBV3	13014	20604	0.14%	0.070%
63	9.251	2533	2538	2540	rBV2	172	187	0.00%	0.001%
64	9.440	2594	2597	2599	rVV2	471	344	0.00%	0.001%
65	9.473	2602	2607	2609	rBV2	332	291	0.00%	0.001%
66	9.553	2624	2632	2643	rBV3	5549	9171	0.06%	0.031%
67	9.611	2648	2650	2652	rBV	351	160	0.00%	0.001%
68	9.694	2674	2676	2680	rVB2	293	227	0.00%	0.001%
69	9.727	2683	2686	2689	rBV	337	255	0.00%	0.001%
70	9.887	2733	2736	2738	rBV2	175	130	0.00%	0.000%
71	9.919	2743	2746	2748	rBV2	225	163	0.00%	0.001%
72	9.942	2749	2753	2760	rVB2	1055	1150	0.01%	0.004%
73	10.026	2770	2779	2796	rVB3	10988	19080	0.13%	0.065%
74	10.112	2801	2806	2809	rVB2	415	342	0.00%	0.001%
75	10.128	2809	2811	2814	rBV2	245	170	0.00%	0.001%
76	10.148	2814	2817	2822	rBV2	210	210	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020088.D
 Acq On : 20 Jan 2021 20:07
 Operator : SY/MD
 Sample : M1181-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

77	10.222	2828	2840	2862	rBV	426559	660553	4.35%	2.239%
78	10.350	2878	2880	2883	rBV2	231	178	0.00%	0.001%
79	10.453	2907	2912	2919	rBV4	1073	1408	0.01%	0.005%
80	10.550	2931	2942	2946	rBV3	1131	1838	0.01%	0.006%
81	10.640	2967	2970	2979	rVB2	242	320	0.00%	0.001%
82	10.714	2990	2993	2996	rBV	196	112	0.00%	0.000%
83	10.736	2997	3000	3001	rBV2	307	170	0.00%	0.001%
84	10.788	3013	3016	3018	rBV	416	258	0.00%	0.001%
85	10.916	3053	3056	3058	rBV2	1146	860	0.01%	0.003%
86	11.090	3107	3110	3113	rBV2	674	484	0.00%	0.002%
87	11.193	3137	3142	3145	rBV3	1013	931	0.01%	0.003%
88	11.254	3149	3161	3182	rBV	715480	1105267	7.27%	3.746%
89	11.476	3228	3230	3231	rBV	302	121	0.00%	0.000%
90	11.546	3247	3252	3257	rBV3	1225	1235	0.01%	0.004%
91	11.572	3257	3260	3265	rBV2	339	283	0.00%	0.001%
92	11.630	3266	3278	3298	rBV	757000	1175557	7.73%	3.984%
93	11.775	3320	3323	3327	rBV3	501	468	0.00%	0.002%
94	11.813	3333	3335	3338	rBV	447	255	0.00%	0.001%
95	12.061	3408	3412	3416	rBV2	281	242	0.00%	0.001%
96	12.251	3466	3471	3473	rBV2	595	496	0.00%	0.002%
97	12.649	3593	3595	3599	rBV3	459	400	0.00%	0.001%
98	12.839	3647	3654	3663	rBV5	3280	4435	0.03%	0.015%
99	13.148	3747	3750	3754	rBV2	413	348	0.00%	0.001%
100	13.276	3784	3790	3792	rBV3	1049	1147	0.01%	0.004%




Sum of corrected areas: 29503438

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020088.D
Acq On : 20 Jan 2021 20:07
Operator : SY/MD
Sample : M1181-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

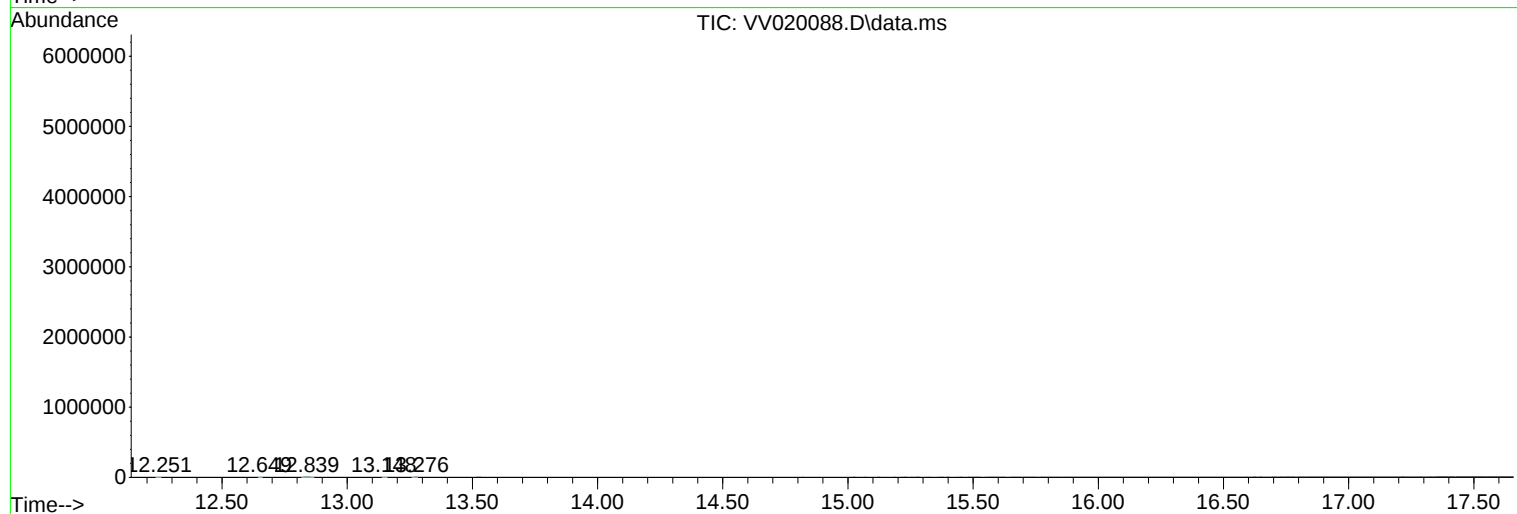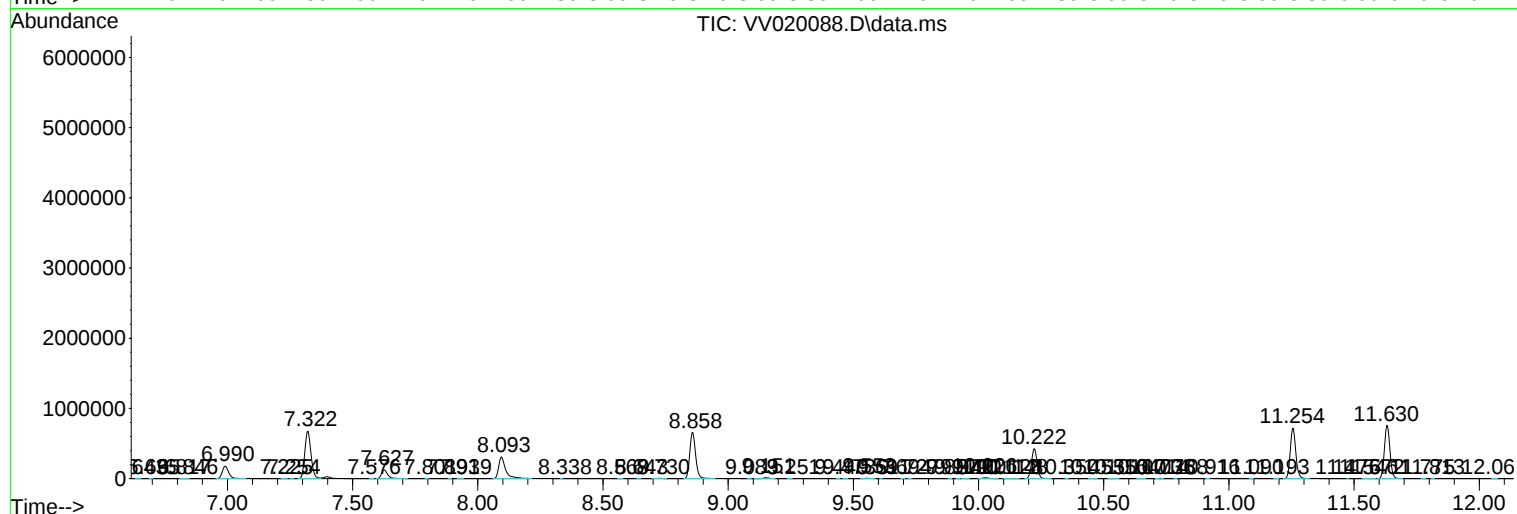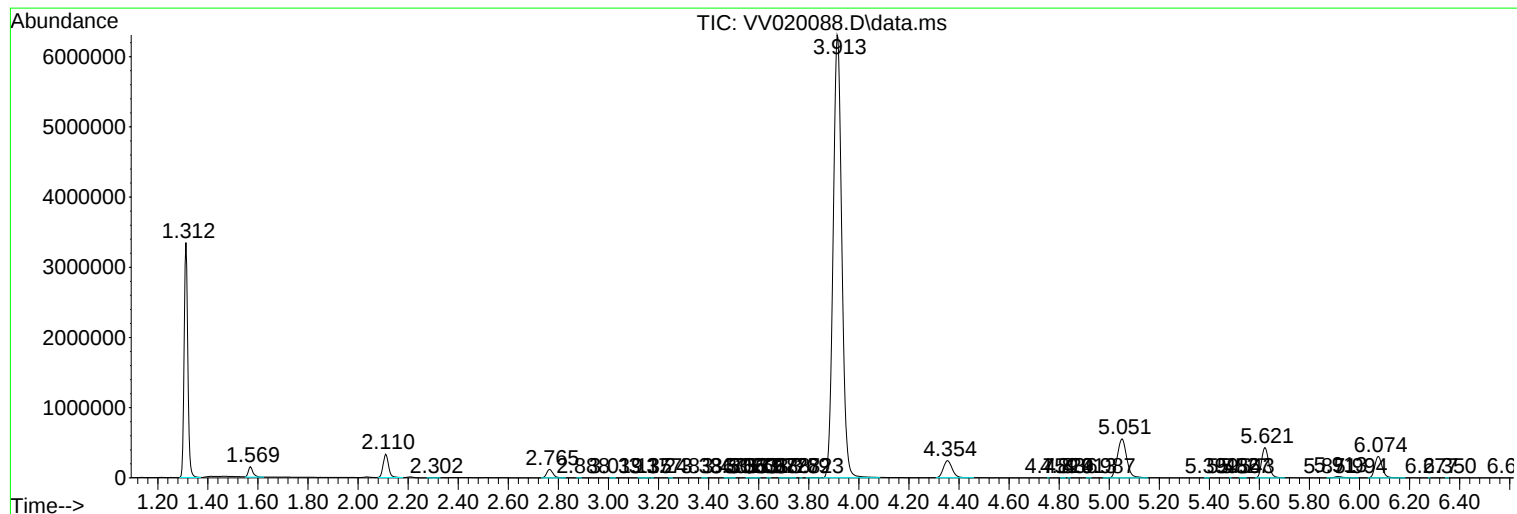

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020088.D
Acq On : 20 Jan 2021 20:07
Operator : SY/MD
Sample : M1181-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020088.D
Acq On : 20 Jan 2021 20:07
Operator : SY/MD
Sample : M1181-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------