

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020090.D
 Acq On : 20 Jan 2021 20:54
 Operator : SY/MD
 Sample : M1181-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

Signal : TIC: VV020090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	85	rVB2	234805	247998	16.53%	2.077%
2	1.569	143	149	161	rVB	154420	168778	11.25%	1.414%
3	2.110	308	317	339	rVB	335661	497150	33.15%	4.164%
4	2.296	368	375	384	rBV	2567	4050	0.27%	0.034%
5	2.772	510	523	542	rVB3	29736	60995	4.07%	0.511%
6	2.885	557	558	561	rVB2	175	90	0.01%	0.001%
7	2.962	577	582	584	rBV2	250	247	0.02%	0.002%
8	2.994	588	592	594	rBV	130	107	0.01%	0.001%
9	3.090	617	622	625	rVB2	292	260	0.02%	0.002%
10	3.200	653	656	659	rBV2	210	141	0.01%	0.001%
11	3.241	667	669	672	rBV2	285	153	0.01%	0.001%
12	3.299	683	687	691	rVB	405	217	0.01%	0.002%
13	3.354	700	704	707	rBV2	261	197	0.01%	0.002%
14	3.383	707	713	717	rBV2	300	307	0.02%	0.003%
15	3.441	729	731	734	rBV	143	118	0.01%	0.001%
16	3.463	734	738	741	rBV	249	163	0.01%	0.001%
17	3.585	772	776	779	rBV2	285	214	0.01%	0.002%
18	3.663	798	800	801	rBV2	127	73	0.00%	0.001%
19	3.688	805	808	811	rBV	215	187	0.01%	0.002%
20	3.730	818	821	823	rVB2	233	125	0.01%	0.001%
21	3.778	832	836	838	rBV2	210	153	0.01%	0.001%
22	3.823	846	850	853	rBV2	164	155	0.01%	0.001%
23	3.913	860	878	900	rBV2	235435	723669	48.25%	6.062%
24	4.251	979	983	984	rBV	339	227	0.02%	0.002%
25	4.354	998	1015	1043	rBV	241650	592067	39.47%	4.959%
26	4.576	1081	1084	1086	rBV2	283	181	0.01%	0.002%
27	4.624	1097	1099	1102	rVB2	295	170	0.01%	0.001%
28	4.640	1102	1104	1105	rBV2	216	77	0.01%	0.001%
29	4.666	1110	1112	1115	rVV2	167	118	0.01%	0.001%
30	4.682	1115	1117	1119	rVV	208	75	0.01%	0.001%
31	4.704	1121	1124	1127	rBV	174	140	0.01%	0.001%
32	4.720	1127	1129	1132	rVB2	201	115	0.01%	0.001%
33	4.782	1146	1148	1152	rBV	183	169	0.01%	0.001%
34	4.852	1166	1170	1172	rBV2	221	210	0.01%	0.002%
35	4.888	1178	1181	1183	rBV2	219	147	0.01%	0.001%
36	4.907	1183	1187	1190	rBV	284	273	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020090.D
 Acq On : 20 Jan 2021 20:54
 Operator : SY/MD
 Sample : M1181-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

37	5.052	1214	1232	1273	rBV2	577421	1499869	100.00%	12.563%
38	5.254	1293	1295	1297	rBV2	301	126	0.01%	0.001%
39	5.302	1308	1310	1313	rBV3	249	193	0.01%	0.002%
40	5.489	1365	1368	1371	rBV3	328	275	0.02%	0.002%
41	5.540	1382	1384	1388	rBV	364	260	0.02%	0.002%
42	5.569	1390	1393	1396	rVB2	225	101	0.01%	0.001%
43	5.621	1397	1409	1435	rBV	460064	901191	60.08%	7.549%
44	5.917	1489	1501	1518	rBV6	20035	47328	3.16%	0.396%
45	6.026	1533	1535	1537	rBV	254	142	0.01%	0.001%
46	6.074	1537	1550	1573	rBV	321311	643880	42.93%	5.393%
47	6.309	1619	1623	1627	rBV3	392	444	0.03%	0.004%
48	6.418	1654	1657	1661	rBV2	330	251	0.02%	0.002%
49	6.441	1661	1664	1665	rBV	173	94	0.01%	0.001%
50	6.524	1684	1690	1693	rBV2	213	301	0.02%	0.003%
51	6.634	1721	1724	1725	rBV	174	119	0.01%	0.001%
52	6.740	1753	1757	1762	rBV	303	293	0.02%	0.002%
53	6.804	1773	1777	1778	rBV	314	171	0.01%	0.001%
54	6.990	1824	1835	1856	rBV	181929	327917	21.86%	2.747%
55	7.190	1894	1897	1901	rBV4	473	339	0.02%	0.003%
56	7.322	1925	1938	1958	rBV	696833	1206759	80.46%	10.108%
57	7.540	2004	2006	2008	rBV2	476	201	0.01%	0.002%
58	7.627	2022	2033	2053	rBV	124666	219258	14.62%	1.837%
59	7.952	2133	2134	2136	rVB	304	96	0.01%	0.001%
60	7.984	2136	2144	2155	rBV5	6461	11242	0.75%	0.094%
61	8.093	2168	2178	2210	rBV2	310442	608987	40.60%	5.101%
62	8.521	2309	2311	2315	rVB2	367	187	0.01%	0.002%
63	8.556	2318	2322	2326	rBV3	399	324	0.02%	0.003%
64	8.592	2330	2333	2335	rBV2	208	133	0.01%	0.001%
65	8.624	2341	2343	2349	rBV2	307	234	0.02%	0.002%
66	8.707	2367	2369	2371	rBV	182	119	0.01%	0.001%
67	8.775	2386	2390	2392	rBV2	228	171	0.01%	0.001%
68	8.859	2404	2416	2440	rBV	686559	1120603	74.71%	9.386%
69	9.151	2500	2507	2522	rVB4	3732	5562	0.37%	0.047%
70	9.228	2528	2531	2542	rVB4	469	447	0.03%	0.004%
71	9.379	2572	2578	2582	rBV2	346	340	0.02%	0.003%
72	9.428	2587	2593	2597	rBV2	279	364	0.02%	0.003%
73	9.473	2604	2607	2613	rVB	318	347	0.02%	0.003%
74	9.502	2613	2616	2618	rBV	207	125	0.01%	0.001%
75	9.521	2619	2622	2624	rVV	212	120	0.01%	0.001%
76	9.559	2624	2634	2645	rVV2	917	1664	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020090.D
 Acq On : 20 Jan 2021 20:54
 Operator : SY/MD
 Sample : M1181-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

77	9.695	2667	2676	2679	rBV2	304	501	0.03%	0.004%
78	9.939	2749	2752	2757	rBV3	300	318	0.02%	0.003%
79	10.055	2785	2788	2790	rBV2	225	116	0.01%	0.001%
80	10.132	2809	2812	2814	rBV	238	144	0.01%	0.001%
81	10.222	2829	2840	2859	rBV	433526	671069	44.74%	5.621%
82	10.389	2889	2892	2893	rBV2	601	338	0.02%	0.003%
83	10.543	2935	2940	2941	rBV	738	503	0.03%	0.004%
84	10.576	2948	2950	2951	rBV	132	72	0.00%	0.001%
85	10.637	2966	2969	2972	rBV2	272	205	0.01%	0.002%
86	10.752	3000	3005	3009	rBV3	407	441	0.03%	0.004%
87	10.990	3077	3079	3081	rBV	208	137	0.01%	0.001%
88	11.096	3110	3112	3117	rVB	534	320	0.02%	0.003%
89	11.157	3129	3131	3136	rBV3	765	765	0.05%	0.006%
90	11.254	3150	3161	3184	rBV	742894	1151971	76.80%	9.649%
91	11.630	3266	3278	3298	rBV	771157	1205303	80.36%	10.096%
92	11.977	3383	3386	3389	rBV2	286	200	0.01%	0.002%
93	12.042	3404	3406	3408	rBV	134	75	0.01%	0.001%
94	12.267	3471	3476	3482	rVB3	662	705	0.05%	0.006%
95	12.357	3501	3504	3511	rVB5	3536	3726	0.25%	0.031%
96	12.646	3592	3594	3595	rBV	316	107	0.01%	0.001%
97	13.090	3724	3732	3736	rBV2	430	552	0.04%	0.005%
98	13.379	3819	3822	3827	rBV2	383	334	0.02%	0.003%
99	13.601	3889	3891	3893	rBV2	351	121	0.01%	0.001%
100	13.688	3913	3918	3921	rBV	463	486	0.03%	0.004%




Sum of corrected areas: 11938602

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020090.D
Acq On : 20 Jan 2021 20:54
Operator : SY/MD
Sample : M1181-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

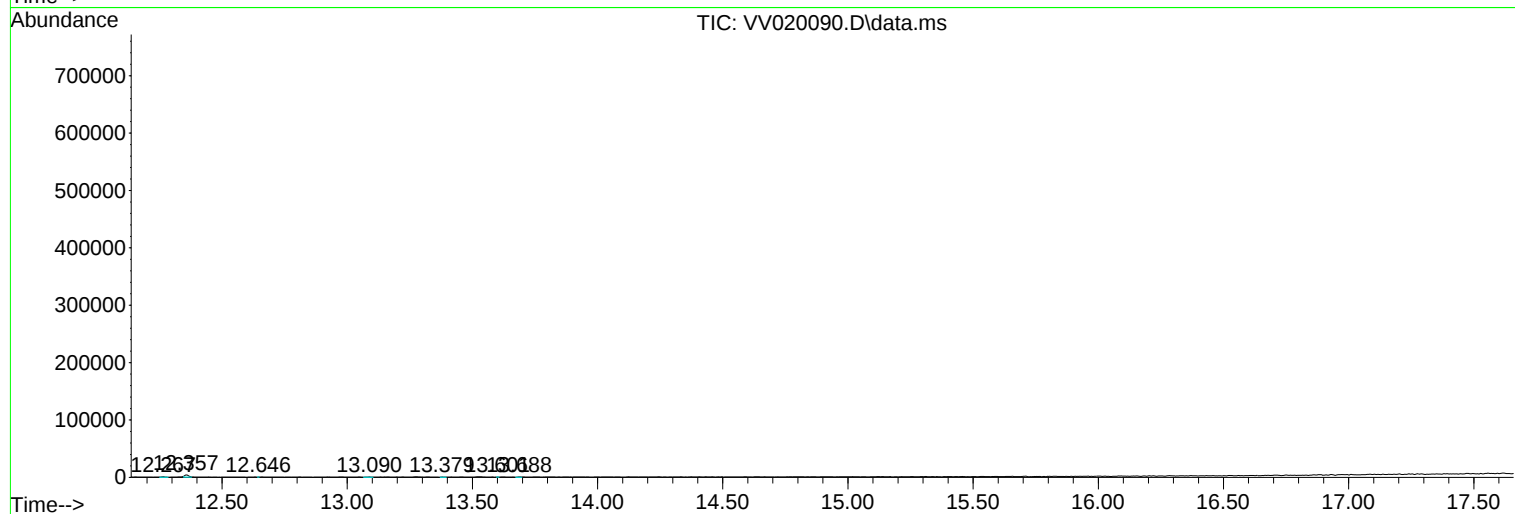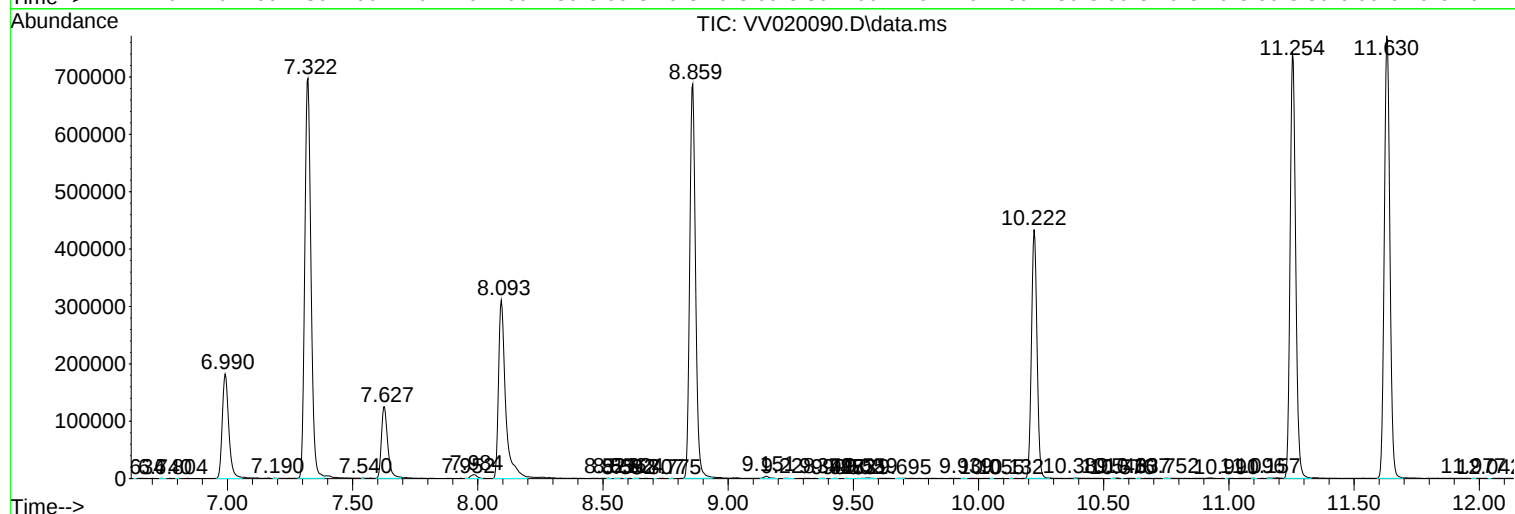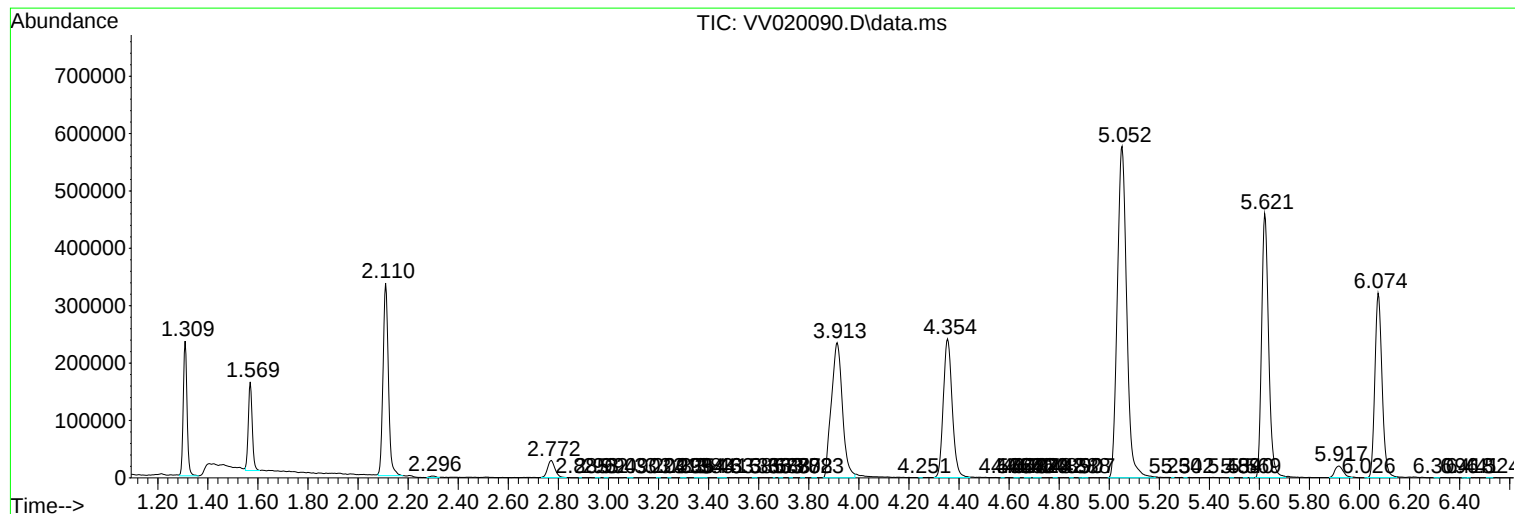

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020090.D
Acq On : 20 Jan 2021 20:54
Operator : SY/MD
Sample : M1181-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020090.D
Acq On : 20 Jan 2021 20:54
Operator : SY/MD
Sample : M1181-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
