

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020091.D
 Acq On : 20 Jan 2021 21:17
 Operator : SY/MD
 Sample : M1181-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

Signal : TIC: VV020091.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	78	rVB	188423	190095	13.18%	1.539%
2	1.569	142	149	166	rVB	147981	169354	11.74%	1.371%
3	2.109	307	317	338	rBV	315918	472186	32.73%	3.824%
4	2.351	390	392	395	rBV	251	138	0.01%	0.001%
5	2.447	416	422	425	rBV3	557	542	0.04%	0.004%
6	2.595	465	468	470	rBV2	336	200	0.01%	0.002%
7	2.643	477	483	487	rBV2	254	355	0.02%	0.003%
8	2.759	516	519	521	rBV	306	149	0.01%	0.001%
9	2.965	579	583	584	rBV	174	129	0.01%	0.001%
10	2.997	590	593	598	rBV2	235	281	0.02%	0.002%
11	3.074	614	617	621	rVB2	208	185	0.01%	0.001%
12	3.177	644	649	653	rBV2	152	171	0.01%	0.001%
13	3.277	678	680	684	rBV2	159	143	0.01%	0.001%
14	3.412	718	722	725	rBV	210	184	0.01%	0.001%
15	3.457	729	736	742	rBV2	239	362	0.03%	0.003%
16	3.505	748	751	753	rBV	182	141	0.01%	0.001%
17	3.576	764	773	778	rVB2	281	396	0.03%	0.003%
18	3.614	782	785	787	rBV	198	142	0.01%	0.001%
19	3.653	794	797	801	rVB2	203	135	0.01%	0.001%
20	3.685	801	807	809	rBV	167	163	0.01%	0.001%
21	3.714	810	816	821	rBV2	236	347	0.02%	0.003%
22	3.759	826	830	833	rBV2	206	212	0.01%	0.002%
23	3.894	861	872	922	rBV	85967	269920	18.71%	2.186%
24	4.354	998	1015	1049	rBV2	234076	580035	40.20%	4.697%
25	4.717	1126	1128	1134	rVB	488	367	0.03%	0.003%
26	4.814	1152	1158	1161	rBV2	256	319	0.02%	0.003%
27	4.830	1161	1163	1168	rVB2	299	194	0.01%	0.002%
28	4.916	1184	1190	1194	rBV2	256	290	0.02%	0.002%
29	4.968	1201	1206	1207	rBV2	196	151	0.01%	0.001%
30	5.051	1213	1232	1259	rBV2	562738	1442827	100.00%	11.685%
31	5.376	1329	1333	1334	rBV2	399	210	0.01%	0.002%
32	5.441	1350	1353	1355	rVB2	328	169	0.01%	0.001%
33	5.457	1355	1358	1360	rBV	296	143	0.01%	0.001%
34	5.492	1365	1369	1372	rBV2	210	217	0.02%	0.002%
35	5.543	1383	1385	1389	rBV2	181	174	0.01%	0.001%
36	5.566	1389	1392	1396	rBV2	204	159	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020091.D
 Acq On : 20 Jan 2021 21:17
 Operator : SY/MD
 Sample : M1181-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

37	5.621	1396	1409	1437	rBV	438287	873751	60.56%	7.076%
38	5.913	1489	1500	1521	rBV6	32410	76936	5.33%	0.623%
39	6.029	1531	1536	1537	rBV2	252	225	0.02%	0.002%
40	6.074	1537	1550	1580	rVV2	315148	635538	44.05%	5.147%
41	6.270	1609	1611	1614	rBV	245	148	0.01%	0.001%
42	6.296	1617	1619	1624	rVB	425	301	0.02%	0.002%
43	6.322	1624	1627	1628	rBV2	206	132	0.01%	0.001%
44	6.360	1633	1639	1642	rBV3	409	406	0.03%	0.003%
45	6.389	1642	1648	1654	rBV2	410	464	0.03%	0.004%
46	6.482	1672	1677	1680	rBV	240	268	0.02%	0.002%
47	6.614	1716	1718	1722	rVB	389	204	0.01%	0.002%
48	6.643	1722	1727	1729	rBV	318	346	0.02%	0.003%
49	6.704	1743	1746	1749	rBV2	383	258	0.02%	0.002%
50	6.723	1749	1752	1754	rBV	258	143	0.01%	0.001%
51	6.752	1758	1761	1765	rBV2	304	316	0.02%	0.003%
52	6.826	1781	1784	1786	rVB	218	134	0.01%	0.001%
53	6.990	1823	1835	1854	rBV	174516	315512	21.87%	2.555%
54	7.321	1924	1938	1963	rBV	697100	1193374	82.71%	9.664%
55	7.627	2022	2033	2051	rBV	125669	213366	14.79%	1.728%
56	7.932	2126	2128	2130	rBV2	324	144	0.01%	0.001%
57	7.981	2130	2143	2168	rBV	754236	1258230	87.21%	10.190%
58	8.093	2168	2178	2209	rBV2	313084	603552	41.83%	4.888%
59	8.325	2247	2250	2252	rBV2	344	231	0.02%	0.002%
60	8.408	2274	2276	2280	rBV2	368	218	0.02%	0.002%
61	8.428	2280	2282	2286	rBV3	353	304	0.02%	0.002%
62	8.482	2296	2299	2303	rBV	284	266	0.02%	0.002%
63	8.518	2307	2310	2312	rBV2	346	222	0.02%	0.002%
64	8.765	2383	2387	2389	rBV2	388	321	0.02%	0.003%
65	8.858	2404	2416	2440	rBV	669299	1089685	75.52%	8.825%
66	9.083	2483	2486	2488	rVV2	422	263	0.02%	0.002%
67	9.231	2528	2532	2534	rBV	354	253	0.02%	0.002%
68	9.296	2546	2552	2554	rBV	387	374	0.03%	0.003%
69	9.363	2571	2573	2575	rBV2	234	132	0.01%	0.001%
70	9.415	2583	2589	2591	rBV2	215	244	0.02%	0.002%
71	9.685	2670	2673	2678	rVB	250	255	0.02%	0.002%
72	9.710	2678	2681	2683	rBV2	162	130	0.01%	0.001%
73	9.829	2714	2718	2723	rVB2	377	314	0.02%	0.003%
74	9.858	2723	2727	2731	rVB	309	285	0.02%	0.002%
75	9.881	2731	2734	2735	rBV	181	129	0.01%	0.001%
76	9.916	2742	2745	2748	rBV2	310	258	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020091.D
 Acq On : 20 Jan 2021 21:17
 Operator : SY/MD
 Sample : M1181-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

77	10.051	2783	2787	2790	rBV2	289	227	0.02%	0.002%
78	10.222	2828	2840	2863	rBV	419901	652482	45.22%	5.284%
79	10.360	2880	2883	2886	rBV3	311	254	0.02%	0.002%
80	10.501	2924	2927	2930	rBV2	353	295	0.02%	0.002%
81	10.543	2937	2940	2941	rBV	327	198	0.01%	0.002%
82	10.640	2967	2970	2973	rBV2	276	190	0.01%	0.002%
83	10.762	3005	3008	3012	rBV2	215	187	0.01%	0.002%
84	10.862	3037	3039	3044	rBV2	294	212	0.01%	0.002%
85	10.948	3063	3066	3070	rVB2	286	219	0.02%	0.002%
86	10.977	3072	3075	3079	rBV2	208	200	0.01%	0.002%
87	11.042	3093	3095	3098	rBV2	299	196	0.01%	0.002%
88	11.083	3105	3108	3112	rVB	306	214	0.01%	0.002%
89	11.173	3134	3136	3140	rBV2	324	291	0.02%	0.002%
90	11.196	3140	3143	3145	rVV2	436	270	0.02%	0.002%
91	11.257	3150	3162	3186	rBV	708174	1115784	77.33%	9.036%
92	11.585	3261	3264	3266	rBV	260	177	0.01%	0.001%
93	11.630	3266	3278	3300	rVV	755256	1175999	81.51%	9.524%
94	11.816	3333	3336	3340	rBV3	430	359	0.02%	0.003%
95	12.029	3399	3402	3405	rBV	294	190	0.01%	0.002%
96	12.064	3405	3413	3415	rBV2	291	378	0.03%	0.003%
97	12.923	3677	3680	3681	rBV	297	181	0.01%	0.001%
98	13.061	3720	3723	3725	rBV	428	270	0.02%	0.002%
99	13.186	3760	3762	3765	rBV	380	181	0.01%	0.001%
100	13.675	3911	3914	3917	rBV2	418	318	0.02%	0.003%




Sum of corrected areas: 12348089

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020091.D
Acq On : 20 Jan 2021 21:17
Operator : SY/MD
Sample : M1181-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

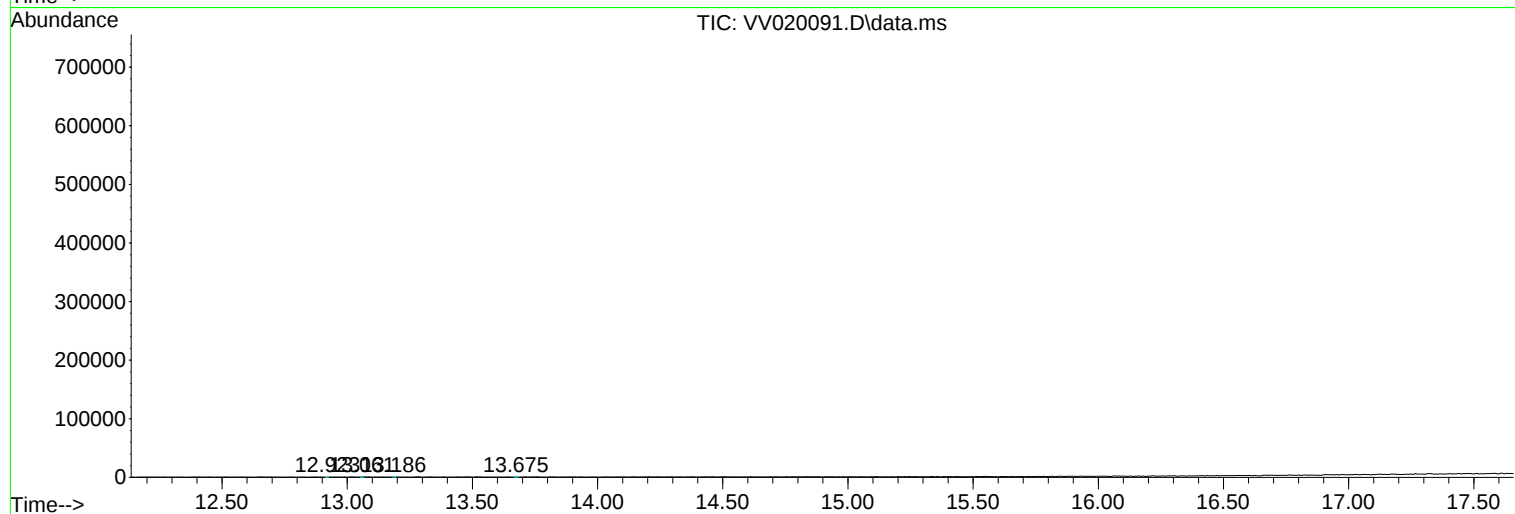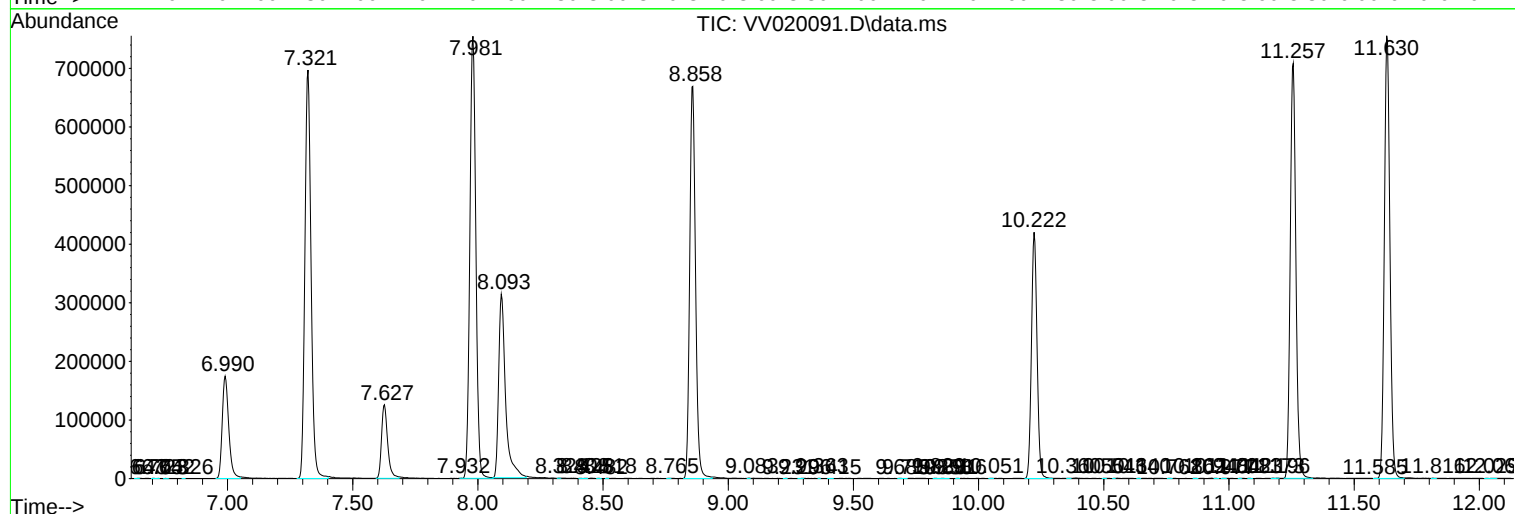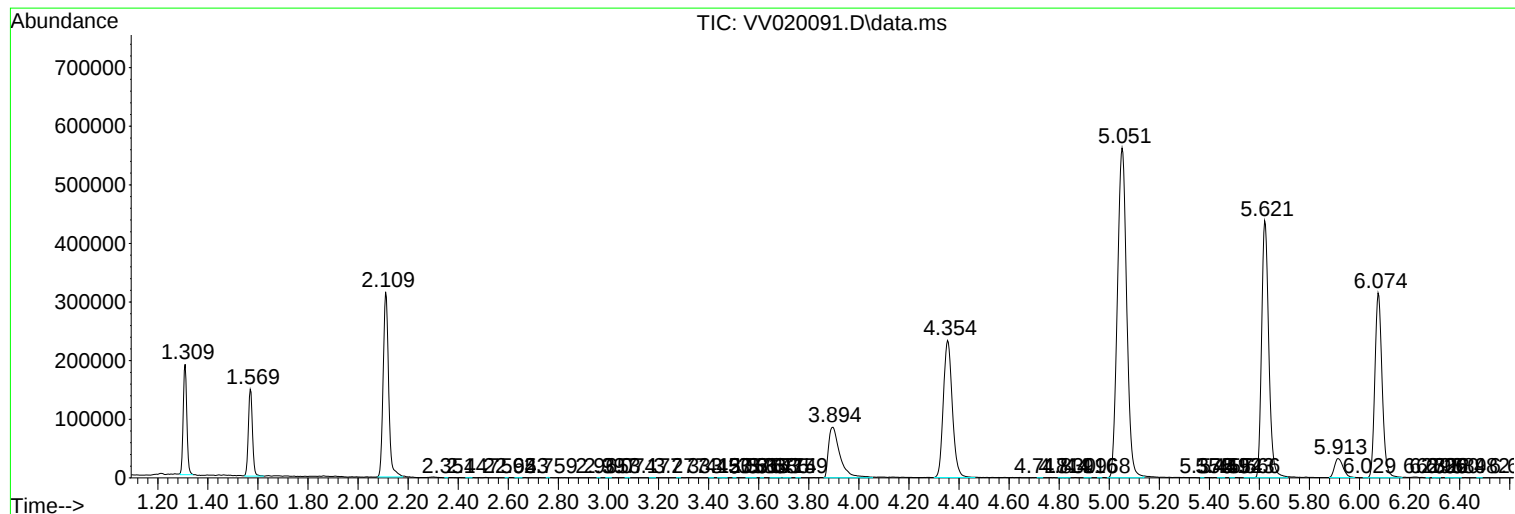

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020091.D
Acq On : 20 Jan 2021 21:17
Operator : SY/MD
Sample : M1181-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020091.D
Acq On : 20 Jan 2021 21:17
Operator : SY/MD
Sample : M1181-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
