

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020093.D
 Acq On : 20 Jan 2021 22:04
 Operator : SY/MD
 Sample : M1181-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

Signal : TIC: VV020093.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	86	rVB	206042	207041	13.38%	1.668%
2	1.569	141	149	163	rVB	164919	181390	11.72%	1.462%
3	2.045	295	297	299	rVB	700	262	0.02%	0.002%
4	2.110	306	317	342	rBV	340549	514925	33.27%	4.150%
5	2.299	369	376	384	rVB3	1475	2382	0.15%	0.019%
6	2.367	394	397	400	rBV2	412	309	0.02%	0.002%
7	2.438	416	419	421	rBV2	333	202	0.01%	0.002%
8	2.512	439	442	452	rVB4	801	859	0.06%	0.007%
9	2.569	456	460	464	rVB2	401	360	0.02%	0.003%
10	2.592	464	467	470	rBV2	308	274	0.02%	0.002%
11	2.688	492	497	502	rVB3	254	283	0.02%	0.002%
12	2.766	511	521	535	rBV8	2112	4046	0.26%	0.033%
13	2.820	535	538	542	rVB	306	265	0.02%	0.002%
14	2.849	542	547	550	rBV	224	257	0.02%	0.002%
15	2.901	559	563	567	rBV2	270	308	0.02%	0.002%
16	2.981	585	588	595	rVB2	252	347	0.02%	0.003%
17	3.055	604	611	613	rBV2	316	352	0.02%	0.003%
18	3.110	624	628	631	rBV2	260	251	0.02%	0.002%
19	3.409	715	721	724	rVB2	284	253	0.02%	0.002%
20	3.602	778	781	787	rVB	273	275	0.02%	0.002%
21	3.679	801	805	811	rVB	311	390	0.03%	0.003%
22	3.907	862	876	907	rBV3	131441	443979	28.69%	3.578%
23	4.155	950	953	956	rBV2	353	249	0.02%	0.002%
24	4.354	998	1015	1046	rBV2	248016	617344	39.89%	4.975%
25	4.466	1046	1050	1053	rBV2	704	508	0.03%	0.004%
26	4.556	1074	1078	1083	rBV3	458	453	0.03%	0.004%
27	4.775	1143	1146	1152	rVB2	407	482	0.03%	0.004%
28	4.814	1155	1158	1160	rBV3	356	256	0.02%	0.002%
29	5.052	1211	1232	1260	rBV2	613074	1547589	100.00%	12.472%
30	5.248	1290	1293	1295	rBV3	377	228	0.01%	0.002%
31	5.302	1306	1310	1313	rBV3	309	328	0.02%	0.003%
32	5.409	1339	1343	1345	rBV2	586	450	0.03%	0.004%
33	5.418	1345	1346	1349	rVV	583	260	0.02%	0.002%
34	5.482	1364	1366	1370	rBV2	412	252	0.02%	0.002%
35	5.566	1389	1392	1395	rBV	240	216	0.01%	0.002%
36	5.621	1395	1409	1438	rBV	470212	938760	60.66%	7.565%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020093.D
 Acq On : 20 Jan 2021 22:04
 Operator : SY/MD
 Sample : M1181-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

37	5.917	1488	1501	1521	rVB8	34489	81009	5.23%	0.653%
38	6.074	1536	1550	1581	rBV	341008	686368	44.35%	5.531%
39	6.212	1589	1593	1594	rBV2	967	589	0.04%	0.005%
40	6.315	1620	1625	1628	rBV4	404	358	0.02%	0.003%
41	6.347	1628	1635	1640	rVB2	293	376	0.02%	0.003%
42	6.460	1667	1670	1673	rBV	313	244	0.02%	0.002%
43	6.495	1678	1681	1687	rVB2	250	271	0.02%	0.002%
44	6.534	1690	1693	1695	rBV2	411	197	0.01%	0.002%
45	6.990	1824	1835	1860	rBV	187832	338398	21.87%	2.727%
46	7.135	1877	1880	1884	rVB2	426	337	0.02%	0.003%
47	7.154	1885	1886	1891	rVB4	531	328	0.02%	0.003%
48	7.180	1891	1894	1896	rBV2	390	262	0.02%	0.002%
49	7.322	1925	1938	1971	rBV	737236	1268047	81.94%	10.219%
50	7.627	2020	2033	2053	rBV	127989	222997	14.41%	1.797%
51	7.891	2113	2115	2119	rVB2	376	202	0.01%	0.002%
52	7.916	2119	2123	2125	rBV2	285	227	0.01%	0.002%
53	7.981	2130	2143	2166	rVB	224976	378564	24.46%	3.051%
54	8.093	2167	2178	2209	rBV2	338107	649606	41.98%	5.235%
55	8.441	2281	2286	2291	rBV3	389	432	0.03%	0.003%
56	8.508	2303	2307	2310	rBV2	230	198	0.01%	0.002%
57	8.524	2310	2312	2316	rVB2	356	256	0.02%	0.002%
58	8.572	2323	2327	2330	rBV2	346	245	0.02%	0.002%
59	8.662	2352	2355	2358	rBV2	349	205	0.01%	0.002%
60	8.794	2392	2396	2399	rVB2	286	216	0.01%	0.002%
61	8.859	2403	2416	2436	rBV	722783	1164751	75.26%	9.386%
62	9.023	2464	2467	2477	rVB6	769	944	0.06%	0.008%
63	9.113	2488	2495	2497	rBV2	314	275	0.02%	0.002%
64	9.125	2497	2499	2502	rVB	443	292	0.02%	0.002%
65	9.270	2539	2544	2548	rBV	218	196	0.01%	0.002%
66	9.518	2618	2621	2623	rBV	429	255	0.02%	0.002%
67	9.778	2697	2702	2706	rBV2	281	307	0.02%	0.002%
68	10.003	2769	2772	2775	rBV2	271	199	0.01%	0.002%
69	10.071	2790	2793	2796	rBV	396	212	0.01%	0.002%
70	10.090	2796	2799	2806	rBV2	364	396	0.03%	0.003%
71	10.222	2828	2840	2865	rVV	445847	697810	45.09%	5.623%
72	10.386	2887	2891	2895	rBV2	623	734	0.05%	0.006%
73	10.765	3004	3009	3013	rBV2	203	267	0.02%	0.002%
74	10.839	3027	3032	3036	rBV2	242	279	0.02%	0.002%
75	11.257	3150	3162	3182	rBV	762253	1187691	76.74%	9.571%
76	11.485	3230	3233	3235	rVB	412	239	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020093.D
 Acq On : 20 Jan 2021 22:04
 Operator : SY/MD
 Sample : M1181-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

77	11.630	3266	3278	3296	rBV	804897	1250109	80.78%	10.074%
78	11.784	3322	3326	3328	rBV3	545	443	0.03%	0.004%
79	11.865	3346	3351	3354	rBV2	317	334	0.02%	0.003%
80	11.990	3387	3390	3394	rVB2	345	225	0.01%	0.002%
81	12.161	3439	3443	3447	rVB3	290	232	0.01%	0.002%
82	12.267	3473	3476	3480	rBV2	340	252	0.02%	0.002%
83	12.637	3589	3591	3595	rVB	411	218	0.01%	0.002%
84	12.665	3595	3600	3604	rBV2	398	443	0.03%	0.004%
85	12.945	3682	3687	3689	rBV2	433	434	0.03%	0.003%
86	13.170	3754	3757	3760	rVB	446	310	0.02%	0.002%
87	13.254	3780	3783	3786	rBV3	392	290	0.02%	0.002%
88	13.453	3843	3845	3849	rVB3	409	272	0.02%	0.002%
89	13.524	3864	3867	3870	rBV2	386	233	0.02%	0.002%
90	13.643	3902	3904	3911	rVB4	236	208	0.01%	0.002%
91	13.768	3941	3943	3946	rVB2	645	385	0.02%	0.003%
92	13.791	3946	3950	3954	rBV3	326	317	0.02%	0.003%
93	13.939	3993	3996	3998	rBV	305	198	0.01%	0.002%
94	14.064	4029	4035	4039	rBV3	542	790	0.05%	0.006%
95	14.231	4083	4087	4089	rBV2	294	263	0.02%	0.002%
96	14.280	4099	4102	4104	rBV	376	276	0.02%	0.002%
97	15.511	4482	4485	4487	rBV2	442	272	0.02%	0.002%
98	15.530	4487	4491	4493	rBV2	821	620	0.04%	0.005%
99	15.630	4520	4522	4526	rBV2	455	235	0.02%	0.002%
100	16.109	4669	4671	4675	rBV2	641	375	0.02%	0.003%




Sum of corrected areas: 12408898

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020093.D
Acq On : 20 Jan 2021 22:04
Operator : SY/MD
Sample : M1181-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

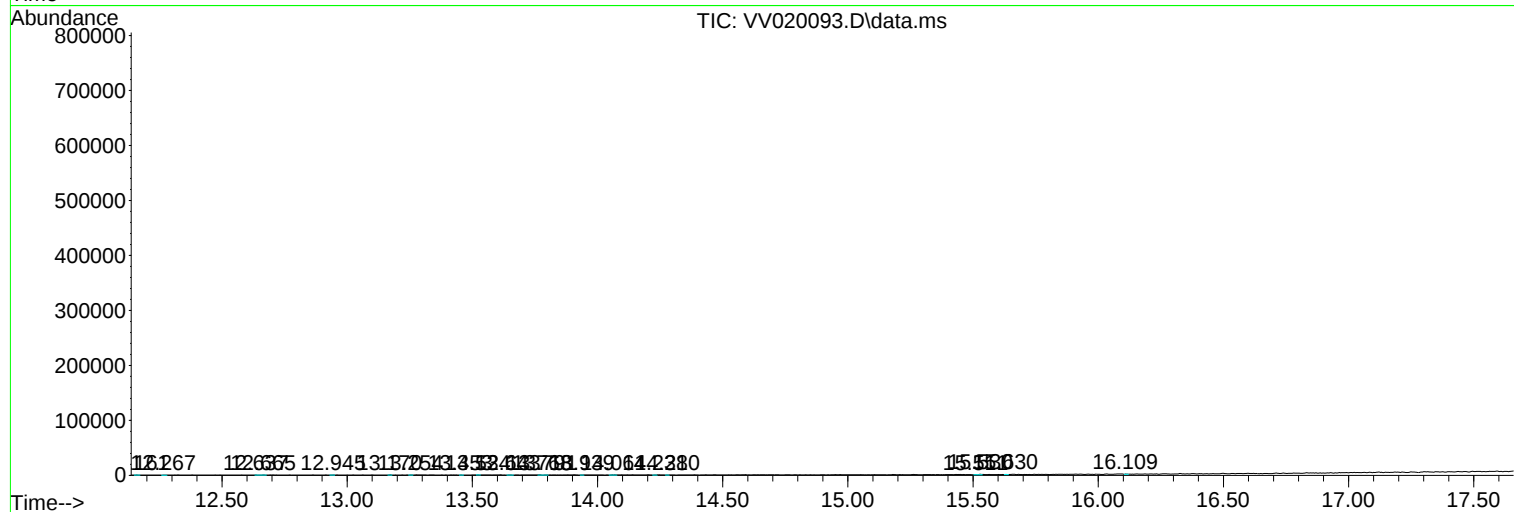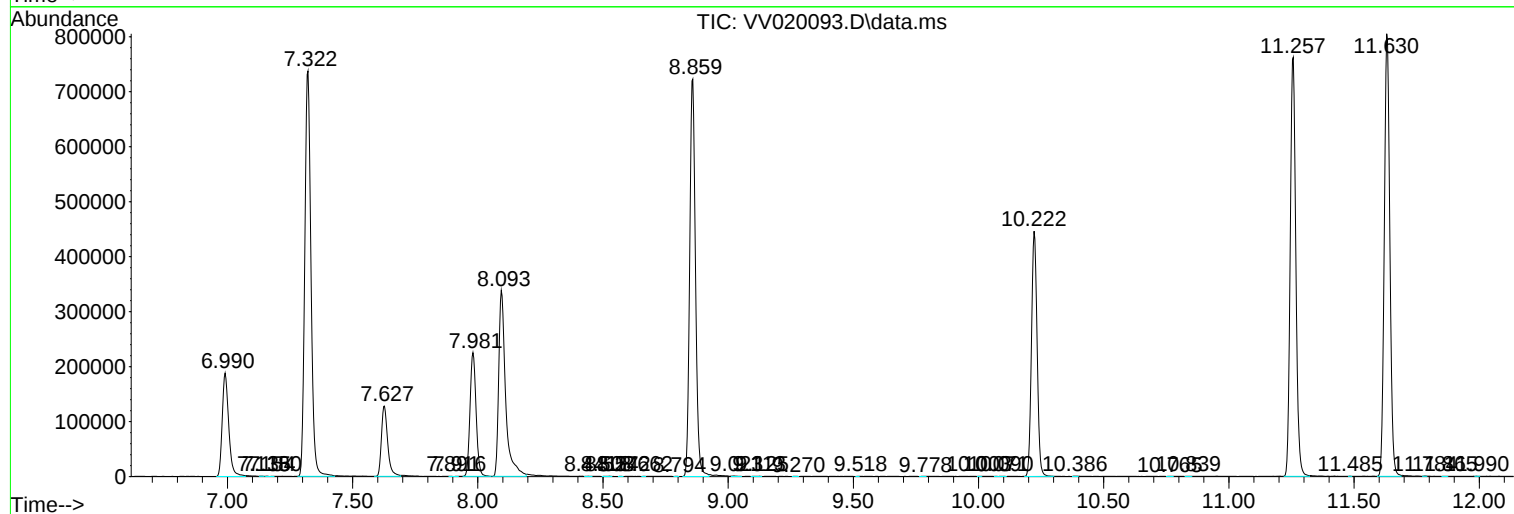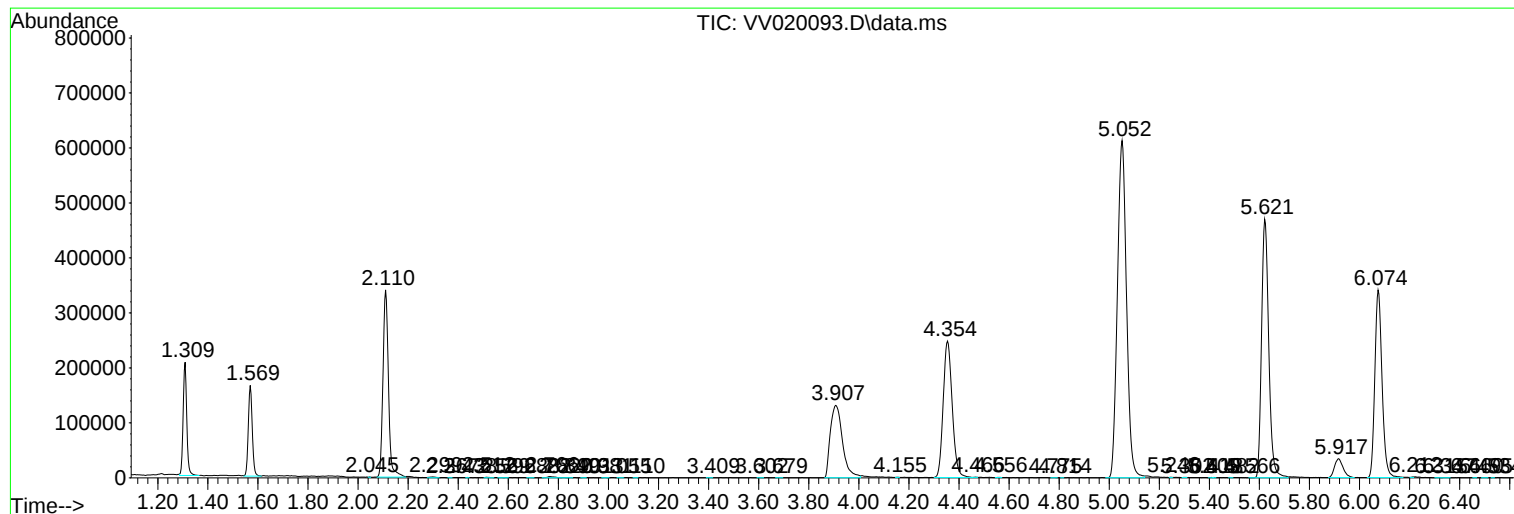

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020093.D
Acq On : 20 Jan 2021 22:04
Operator : SY/MD
Sample : M1181-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020093.D
Acq On : 20 Jan 2021 22:04
Operator : SY/MD
Sample : M1181-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
