

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020094.D
 Acq On : 20 Jan 2021 22:28
 Operator : SY/MD
 Sample : M1181-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

Signal : TIC: VV020094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	80	rVB	213624	209829	13.19%	1.607%
2	1.569	141	149	161	rVB	161887	180423	11.34%	1.382%
3	2.036	292	294	300	rVB3	682	388	0.02%	0.003%
4	2.110	306	317	338	rBV	342277	510540	32.10%	3.910%
5	2.296	369	375	384	rBV3	1551	1995	0.13%	0.015%
6	2.370	394	398	401	rBV2	445	478	0.03%	0.004%
7	2.444	418	421	424	rVB2	404	233	0.01%	0.002%
8	2.460	424	426	431	rBV2	316	235	0.01%	0.002%
9	2.508	437	441	443	rBV2	276	215	0.01%	0.002%
10	2.688	493	497	499	rBV2	310	220	0.01%	0.002%
11	2.740	511	513	516	rVV2	404	229	0.01%	0.002%
12	2.762	517	520	524	rVB2	711	529	0.03%	0.004%
13	2.830	539	541	546	rVB	257	207	0.01%	0.002%
14	3.277	677	680	685	rVB	340	357	0.02%	0.003%
15	3.466	736	739	741	rVV2	305	196	0.01%	0.002%
16	3.486	741	745	748	rVB	391	307	0.02%	0.002%
17	3.515	748	754	758	rBV2	345	537	0.03%	0.004%
18	3.540	758	762	765	rBV2	301	202	0.01%	0.002%
19	3.701	811	812	818	rVB2	347	284	0.02%	0.002%
20	3.740	818	824	826	rBV	318	241	0.02%	0.002%
21	3.778	833	836	838	rBV2	308	213	0.01%	0.002%
22	3.894	861	872	918	rBV	97184	304792	19.16%	2.334%
23	4.354	998	1015	1049	rBV	253733	627216	39.43%	4.803%
24	4.553	1074	1077	1080	rBV2	303	240	0.02%	0.002%
25	4.618	1094	1097	1103	rVB3	433	450	0.03%	0.003%
26	4.865	1172	1174	1179	rVB2	428	294	0.02%	0.002%
27	5.052	1214	1232	1268	rBV2	618001	1590635	100.00%	12.181%
28	5.434	1348	1351	1355	rVB2	488	349	0.02%	0.003%
29	5.505	1370	1373	1377	rVB2	293	194	0.01%	0.001%
30	5.621	1397	1409	1433	rBV	484507	961866	60.47%	7.366%
31	5.833	1469	1475	1481	rBV3	386	525	0.03%	0.004%
32	5.913	1488	1500	1519	rVV5	34553	80393	5.05%	0.616%
33	6.074	1536	1550	1569	rBV	344626	702004	44.13%	5.376%
34	6.209	1589	1592	1593	rBV2	515	316	0.02%	0.002%
35	6.576	1700	1706	1709	rBV	364	317	0.02%	0.002%
36	6.672	1733	1736	1738	rBV2	311	233	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020094.D
 Acq On : 20 Jan 2021 22:28
 Operator : SY/MD
 Sample : M1181-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

37	6.711	1742	1748	1751	rBV	253	242	0.02%	0.002%
38	6.801	1772	1776	1779	rBV2	312	230	0.01%	0.002%
39	6.990	1824	1835	1859	rBV	190966	344688	21.67%	2.640%
40	7.203	1897	1901	1904	rVB3	535	429	0.03%	0.003%
41	7.225	1904	1908	1911	rBV3	432	282	0.02%	0.002%
42	7.322	1924	1938	1958	rBV	754393	1301191	81.80%	9.964%
43	7.527	1999	2002	2006	rVB2	568	365	0.02%	0.003%
44	7.579	2015	2018	2021	rBV2	414	257	0.02%	0.002%
45	7.627	2021	2033	2056	rBV	133344	235004	14.77%	1.800%
46	7.981	2130	2143	2165	rVV	558769	931947	58.59%	7.137%
47	8.093	2168	2178	2210	rVV2	345888	669436	42.09%	5.126%
48	8.376	2263	2266	2271	rBV3	419	418	0.03%	0.003%
49	8.402	2271	2274	2277	rVB3	355	264	0.02%	0.002%
50	8.421	2277	2280	2285	rBV4	305	245	0.02%	0.002%
51	8.498	2301	2304	2307	rVV	297	231	0.01%	0.002%
52	8.598	2331	2335	2338	rBV3	428	314	0.02%	0.002%
53	8.633	2344	2346	2350	rVB3	364	234	0.01%	0.002%
54	8.733	2370	2377	2385	rVB4	945	1620	0.10%	0.012%
55	8.797	2395	2397	2401	rVB2	338	197	0.01%	0.002%
56	8.859	2403	2416	2439	rBV	741464	1193168	75.01%	9.137%
57	9.084	2484	2486	2490	rVV	365	214	0.01%	0.002%
58	9.106	2490	2493	2497	rVB3	338	222	0.01%	0.002%
59	9.158	2504	2509	2512	rVB2	647	579	0.04%	0.004%
60	9.206	2516	2524	2528	rVB	425	504	0.03%	0.004%
61	9.334	2561	2564	2567	rBV	338	206	0.01%	0.002%
62	9.360	2570	2572	2578	rVB2	306	259	0.02%	0.002%
63	9.540	2621	2628	2634	rVB	376	549	0.03%	0.004%
64	9.576	2634	2639	2642	rBV	300	355	0.02%	0.003%
65	9.659	2662	2665	2669	rBV	358	248	0.02%	0.002%
66	9.881	2731	2734	2741	rBV2	428	322	0.02%	0.002%
67	10.006	2770	2773	2778	rVB2	402	254	0.02%	0.002%
68	10.032	2778	2781	2784	rBV2	469	331	0.02%	0.003%
69	10.222	2828	2840	2861	rBV	451998	708337	44.53%	5.424%
70	10.318	2868	2870	2875	rVB3	682	479	0.03%	0.004%
71	10.392	2889	2893	2899	rVB3	782	900	0.06%	0.007%
72	10.428	2899	2904	2906	rBV2	238	231	0.01%	0.002%
73	10.945	3062	3065	3072	rVB2	387	411	0.03%	0.003%
74	11.080	3104	3107	3113	rVB2	446	357	0.02%	0.003%
75	11.186	3137	3140	3142	rBV2	450	269	0.02%	0.002%
76	11.257	3149	3162	3187	rBV	777910	1212004	76.20%	9.281%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020094.D
 Acq On : 20 Jan 2021 22:28
 Operator : SY/MD
 Sample : M1181-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

77	11.453	3221	3223	3229	rVB2	382	238	0.01%	0.002%
78	11.534	3244	3248	3251	rVB	271	218	0.01%	0.002%
79	11.559	3251	3256	3259	rBV2	435	338	0.02%	0.003%
80	11.633	3266	3279	3300	rBV	806607	1265105	79.53%	9.688%
81	12.174	3445	3447	3450	rVB2	430	206	0.01%	0.002%
82	12.485	3542	3544	3552	rVB2	239	212	0.01%	0.002%
83	12.566	3564	3569	3570	rBV2	339	285	0.02%	0.002%
84	12.575	3570	3572	3577	rVB2	337	299	0.02%	0.002%
85	12.656	3595	3597	3605	rVB3	598	623	0.04%	0.005%
86	12.704	3605	3612	3615	rBV2	406	494	0.03%	0.004%
87	12.823	3646	3649	3652	rBV	292	234	0.01%	0.002%
88	12.929	3679	3682	3687	rBV2	389	392	0.02%	0.003%
89	13.000	3701	3704	3706	rBV2	459	354	0.02%	0.003%
90	13.228	3771	3775	3779	rVB2	321	294	0.02%	0.002%
91	13.273	3786	3789	3790	rBV2	422	234	0.01%	0.002%
92	13.321	3801	3804	3808	rBV3	381	306	0.02%	0.002%
93	13.376	3816	3821	3824	rBV2	429	415	0.03%	0.003%
94	13.501	3856	3860	3864	rBV3	419	385	0.02%	0.003%
95	13.656	3905	3908	3911	rVB2	310	200	0.01%	0.002%
96	13.739	3926	3934	3938	rBV3	427	609	0.04%	0.005%
97	13.762	3938	3941	3944	rVV2	345	290	0.02%	0.002%
98	14.013	4016	4019	4023	rBV3	439	519	0.03%	0.004%
99	14.074	4035	4038	4042	rVB4	435	298	0.02%	0.002%
100	15.280	4410	4413	4418	rBV3	473	455	0.03%	0.003%




Sum of corrected areas: 13058478

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020094.D
Acq On : 20 Jan 2021 22:28
Operator : SY/MD
Sample : M1181-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

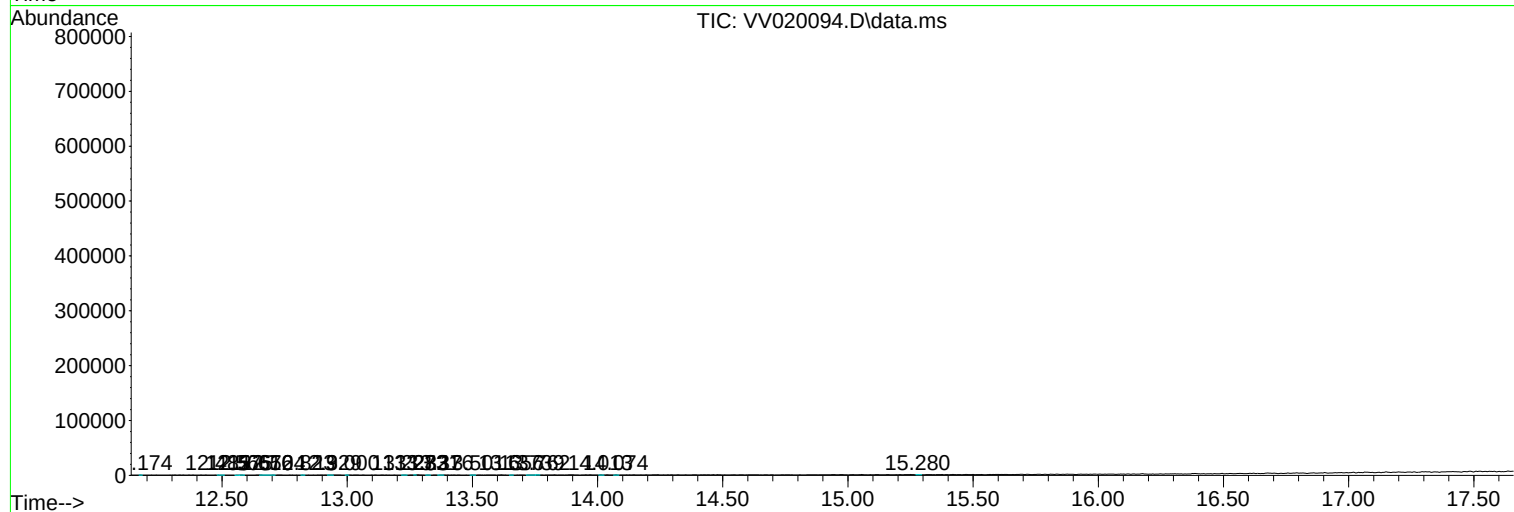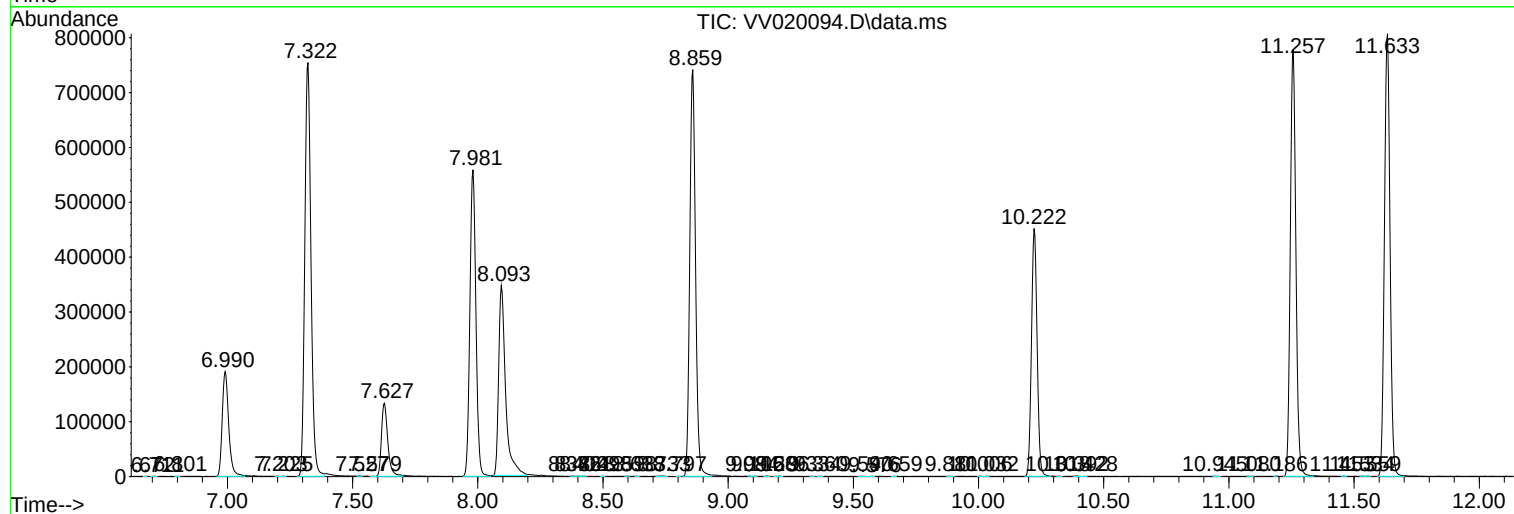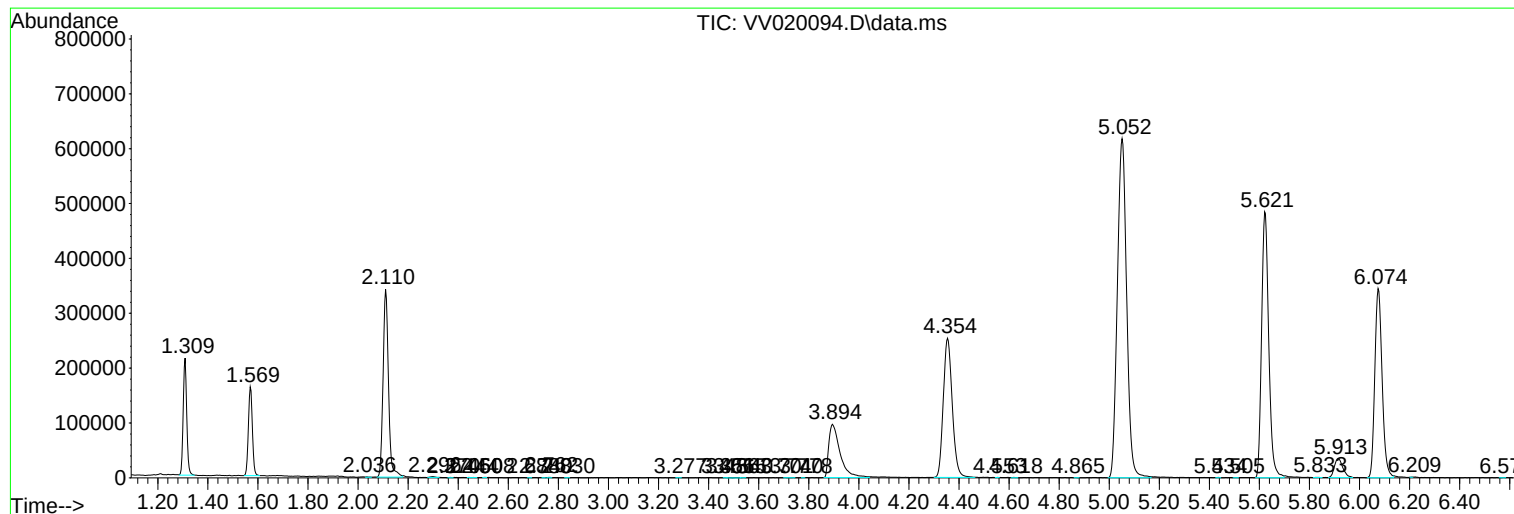

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020094.D
Acq On : 20 Jan 2021 22:28
Operator : SY/MD
Sample : M1181-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020094.D
Acq On : 20 Jan 2021 22:28
Operator : SY/MD
Sample : M1181-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
