

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020095.D
 Acq On : 20 Jan 2021 22:51
 Operator : SY/MD
 Sample : M1181-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

Signal : TIC: VV020095.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	84	rVB	218751	219044	13.22%	1.522%
2	1.569	141	149	162	rBV	166748	180447	10.89%	1.254%
3	1.997	279	282	285	rBV2	647	442	0.03%	0.003%
4	2.110	306	317	343	rBV	358698	541706	32.69%	3.765%
5	2.241	356	358	362	rVB3	457	277	0.02%	0.002%
6	2.293	371	374	380	rVV	738	673	0.04%	0.005%
7	2.341	386	389	391	rBV2	550	345	0.02%	0.002%
8	2.386	399	403	404	rBV2	490	280	0.02%	0.002%
9	2.431	415	417	420	rVB	434	233	0.01%	0.002%
10	2.454	420	424	425	rBV	444	270	0.02%	0.002%
11	2.466	425	428	431	rVV2	459	362	0.02%	0.003%
12	2.492	431	436	437	rVV2	314	263	0.02%	0.002%
13	2.505	437	440	444	rVV3	652	657	0.04%	0.005%
14	2.524	444	446	451	rVB3	506	354	0.02%	0.002%
15	2.557	451	456	459	rBV2	262	308	0.02%	0.002%
16	2.592	463	467	470	rBV2	433	360	0.02%	0.003%
17	2.647	480	484	490	rBV2	327	248	0.01%	0.002%
18	2.769	514	522	532	rBV4	2046	3706	0.22%	0.026%
19	2.868	551	553	557	rVB	286	208	0.01%	0.001%
20	3.013	593	598	599	rBV2	298	255	0.02%	0.002%
21	3.132	633	635	642	rVB3	291	247	0.01%	0.002%
22	3.187	650	652	659	rVB2	353	262	0.02%	0.002%
23	3.331	694	697	702	rBV2	244	249	0.02%	0.002%
24	3.402	716	719	722	rVB	368	208	0.01%	0.001%
25	3.675	799	804	807	rBV	328	375	0.02%	0.003%
26	3.775	832	835	837	rBV2	337	252	0.02%	0.002%
27	3.791	837	840	846	rVB	238	276	0.02%	0.002%
28	3.904	860	875	915	rBV2	128429	471920	28.48%	3.280%
29	4.354	998	1015	1041	rBV	260712	639033	38.56%	4.441%
30	4.595	1087	1090	1096	rVV4	307	314	0.02%	0.002%
31	4.704	1120	1124	1128	rBV3	494	457	0.03%	0.003%
32	4.807	1153	1156	1160	rBV2	265	217	0.01%	0.002%
33	4.923	1190	1192	1200	rVB2	221	209	0.01%	0.001%
34	5.052	1210	1232	1273	rBV2	631413	1623214	97.96%	11.281%
35	5.225	1282	1286	1288	rBV4	623	480	0.03%	0.003%
36	5.476	1363	1364	1369	rBV2	446	277	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020095.D
 Acq On : 20 Jan 2021 22:51
 Operator : SY/MD
 Sample : M1181-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

37	5.621	1397	1409	1434	rBV	499833	993302	59.94%	6.903%
38	5.920	1488	1502	1523	rBV5	77883	176597	10.66%	1.227%
39	6.074	1537	1550	1575	rBV	354976	718010	43.33%	4.990%
40	6.370	1638	1642	1644	rBV	256	213	0.01%	0.001%
41	6.466	1668	1672	1676	rBV2	273	225	0.01%	0.002%
42	6.929	1813	1816	1820	rVB2	306	263	0.02%	0.002%
43	6.990	1824	1835	1862	rBV	195210	351931	21.24%	2.446%
44	7.122	1872	1876	1880	rBV3	378	311	0.02%	0.002%
45	7.203	1896	1901	1903	rBV2	390	280	0.02%	0.002%
46	7.322	1925	1938	1967	rBV	769099	1328438	80.17%	9.232%
47	7.582	2017	2019	2022	rVB3	425	225	0.01%	0.002%
48	7.627	2022	2033	2060	rBV	134131	235700	14.22%	1.638%
49	7.752	2070	2072	2075	rVB	406	209	0.01%	0.001%
50	7.801	2084	2087	2090	rVB2	463	227	0.01%	0.002%
51	7.820	2090	2093	2096	rVB2	481	256	0.02%	0.002%
52	7.865	2104	2107	2109	rBV	394	237	0.01%	0.002%
53	7.981	2128	2143	2167	rBV	992378	1657098	100.00%	11.516%
54	8.093	2168	2178	2215	rVV2	360329	695471	41.97%	4.833%
55	8.351	2256	2258	2263	rVB2	456	253	0.02%	0.002%
56	8.473	2294	2296	2300	rVB3	322	218	0.01%	0.002%
57	8.604	2334	2337	2346	rVB2	324	408	0.02%	0.003%
58	8.666	2354	2356	2361	rVB2	264	220	0.01%	0.002%
59	8.727	2370	2375	2383	rBV3	1615	2222	0.13%	0.015%
60	8.859	2403	2416	2441	rBV	760334	1242065	74.95%	8.632%
61	9.045	2470	2474	2476	rVB2	393	275	0.02%	0.002%
62	9.100	2488	2491	2496	rBV2	310	276	0.02%	0.002%
63	9.135	2496	2502	2506	rBV3	355	361	0.02%	0.003%
64	9.164	2507	2511	2515	rVB2	262	255	0.02%	0.002%
65	9.936	2749	2751	2756	rVB2	225	206	0.01%	0.001%
66	10.029	2777	2780	2783	rBV2	424	249	0.02%	0.002%
67	10.141	2810	2815	2818	rBV2	236	230	0.01%	0.002%
68	10.222	2825	2840	2861	rBV	469667	732699	44.22%	5.092%
69	10.389	2887	2892	2894	rBV2	951	784	0.05%	0.005%
70	10.495	2917	2925	2926	rBV	208	313	0.02%	0.002%
71	10.621	2959	2964	2967	rBV3	433	375	0.02%	0.003%
72	10.965	3066	3071	3073	rBV	336	302	0.02%	0.002%
73	11.096	3110	3112	3117	rVB3	403	266	0.02%	0.002%
74	11.167	3133	3134	3139	rVB2	373	203	0.01%	0.001%
75	11.257	3150	3162	3182	rBV	821630	1258120	75.92%	8.744%
76	11.524	3240	3245	3248	rBV2	336	314	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020095.D
 Acq On : 20 Jan 2021 22:51
 Operator : SY/MD
 Sample : M1181-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

77	11.543	3248	3251	3252	rBV2	471	218	0.01%	0.002%
78	11.630	3266	3278	3305	rBV	822000	1291990	77.97%	8.979%
79	11.891	3354	3359	3362	rBV3	401	386	0.02%	0.003%
80	11.936	3370	3373	3377	rVB3	312	251	0.02%	0.002%
81	12.010	3394	3396	3402	rVB3	401	361	0.02%	0.003%
82	12.096	3420	3423	3425	rBV3	398	293	0.02%	0.002%
83	12.151	3437	3440	3447	rBV2	315	269	0.02%	0.002%
84	12.444	3529	3531	3536	rVB2	272	228	0.01%	0.002%
85	12.479	3537	3542	3546	rVB	450	439	0.03%	0.003%
86	12.591	3574	3577	3579	rBV2	301	221	0.01%	0.002%
87	12.707	3610	3613	3615	rBV2	327	216	0.01%	0.002%
88	12.762	3628	3630	3635	rVB2	530	300	0.02%	0.002%
89	13.280	3785	3791	3797	rBV4	599	726	0.04%	0.005%
90	13.312	3797	3801	3806	rVB3	556	581	0.04%	0.004%
91	13.337	3806	3809	3813	rBV2	504	527	0.03%	0.004%
92	13.415	3828	3833	3836	rBV	562	618	0.04%	0.004%
93	13.524	3863	3867	3868	rBV	418	308	0.02%	0.002%
94	13.701	3920	3922	3927	rVB	430	310	0.02%	0.002%
95	13.775	3942	3945	3952	rVB	383	336	0.02%	0.002%
96	13.833	3959	3963	3964	rBV2	317	230	0.01%	0.002%
97	14.080	4036	4040	4043	rBV2	369	348	0.02%	0.002%
98	14.116	4048	4051	4055	rVB2	368	294	0.02%	0.002%
99	14.138	4055	4058	4064	rBV2	477	520	0.03%	0.004%
100	16.286	4722	4726	4730	rBV6	1002	1092	0.07%	0.008%


Sum of corrected areas: 14389097

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020095.D
Acq On : 20 Jan 2021 22:51
Operator : SY/MD
Sample : M1181-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

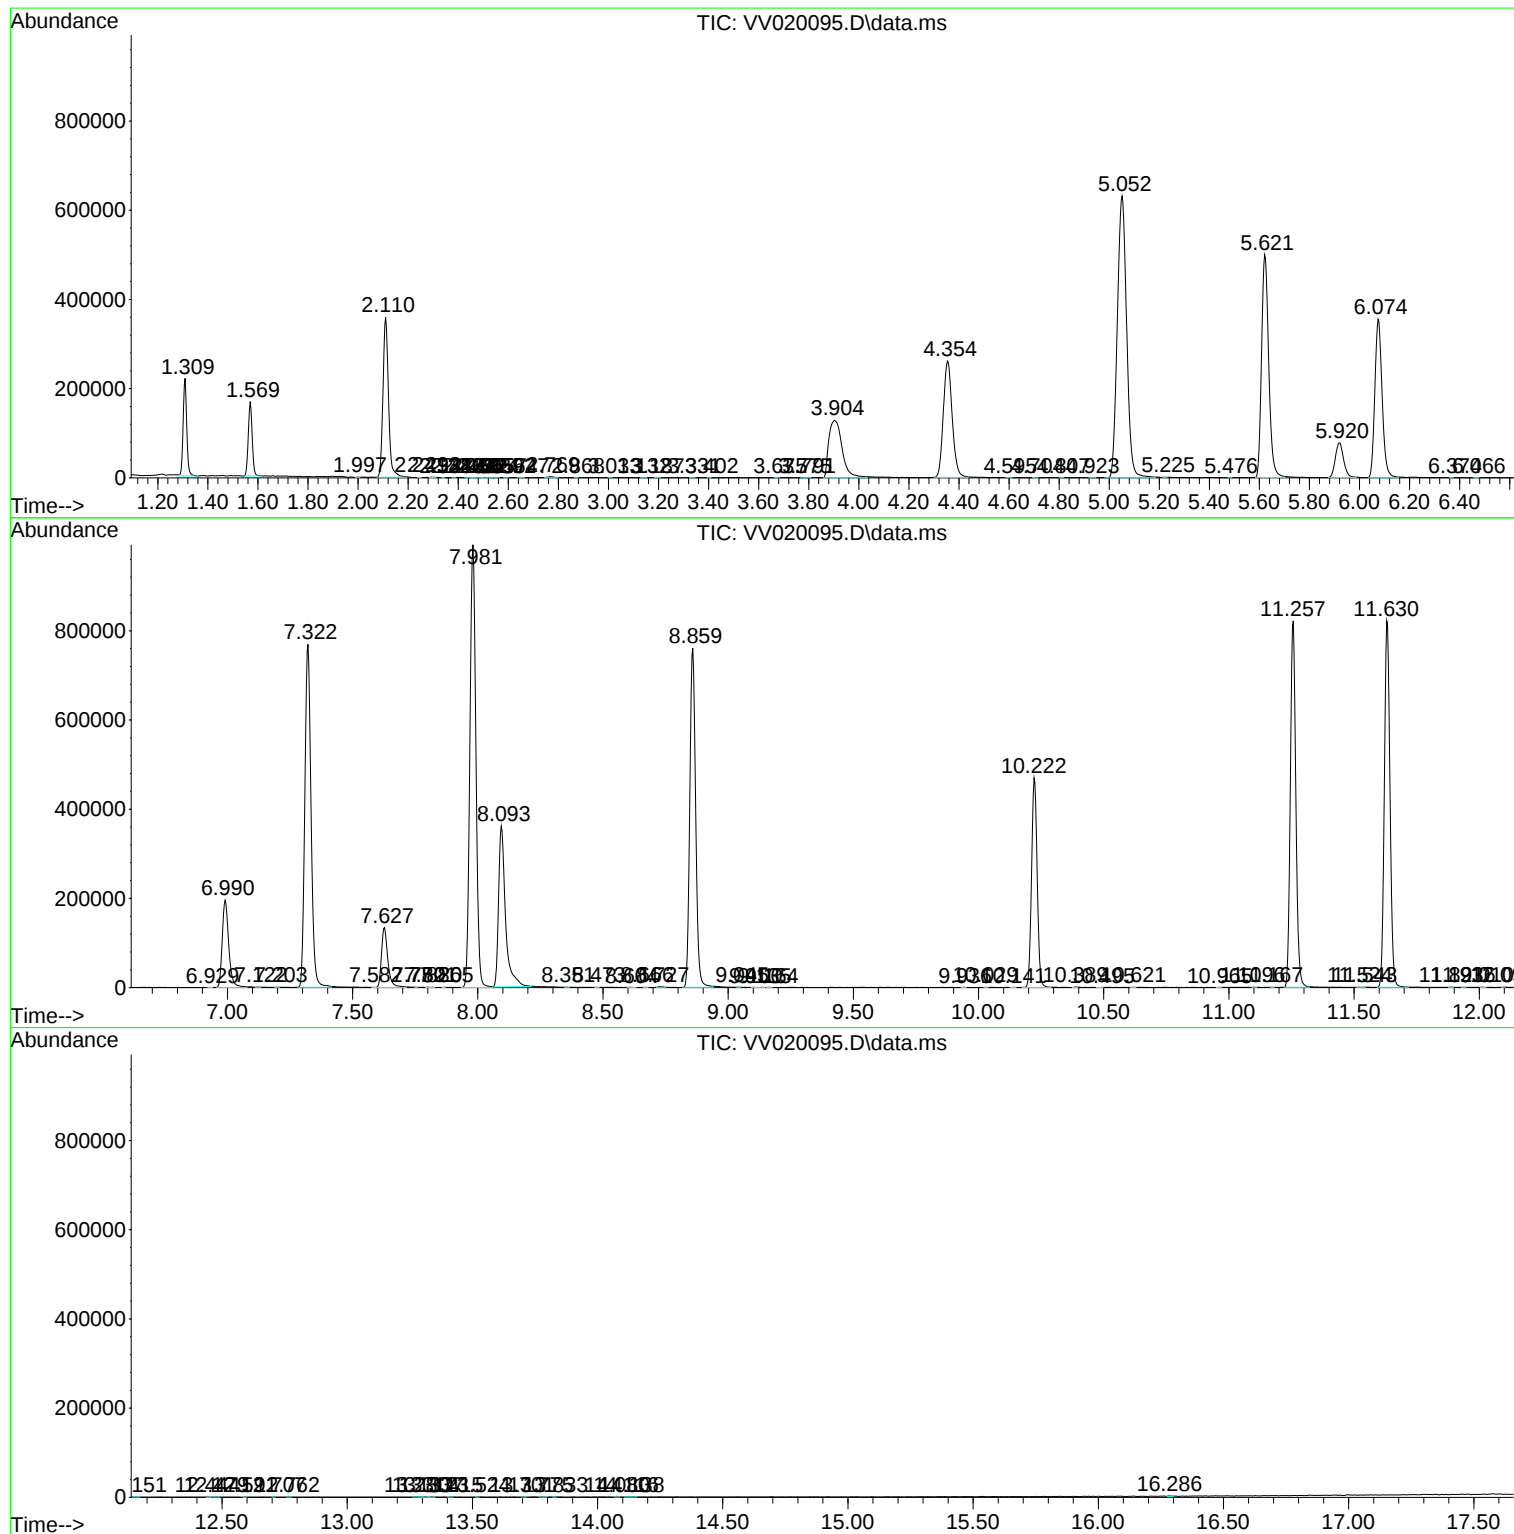

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020095.D
Acq On : 20 Jan 2021 22:51
Operator : SY/MD
Sample : M1181-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020095.D
Acq On : 20 Jan 2021 22:51
Operator : SY/MD
Sample : M1181-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
