

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020096.D
 Acq On : 20 Jan 2021 23:15
 Operator : SY/MD
 Sample : M1181-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

Signal : TIC: VV020096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	80	rVB	219392	219220	13.18%	1.681%
2	1.570	141	149	164	rVB	166225	186776	11.23%	1.433%
3	2.110	307	317	344	rVB	363235	542801	32.64%	4.163%
4	2.242	356	358	360	rBV	343	153	0.01%	0.001%
5	2.512	437	442	446	rVB3	777	842	0.05%	0.006%
6	2.766	514	521	522	rBV4	1351	1070	0.06%	0.008%
7	2.859	547	550	554	rBV2	271	304	0.02%	0.002%
8	2.878	554	556	557	rBV2	161	51	0.00%	0.000%
9	2.907	563	565	569	rBV2	183	138	0.01%	0.001%
10	3.039	603	606	609	rVB3	431	242	0.01%	0.002%
11	3.058	609	612	614	rBV2	178	125	0.01%	0.001%
12	3.135	634	636	639	rVB	252	133	0.01%	0.001%
13	3.151	639	641	643	rBV2	214	109	0.01%	0.001%
14	3.258	670	674	680	rVB2	229	242	0.01%	0.002%
15	3.283	680	682	683	rBV2	143	57	0.00%	0.000%
16	3.335	696	698	699	rBV	174	54	0.00%	0.000%
17	3.357	702	705	708	rBV2	296	196	0.01%	0.002%
18	3.489	742	746	747	rBV	191	158	0.01%	0.001%
19	3.775	832	835	836	rBV	154	110	0.01%	0.001%
20	3.804	842	844	846	rBV2	204	91	0.01%	0.001%
21	3.888	859	870	910	rBV	110456	340587	20.48%	2.612%
22	4.354	998	1015	1052	rBV	265626	657558	39.54%	5.044%
23	4.553	1076	1077	1081	rBV2	337	163	0.01%	0.001%
24	4.621	1096	1098	1100	rVB	129	54	0.00%	0.000%
25	4.637	1100	1103	1105	rBV	369	251	0.02%	0.002%
26	4.711	1124	1126	1129	rVB2	254	156	0.01%	0.001%
27	4.727	1129	1131	1134	rBV	111	51	0.00%	0.000%
28	4.743	1134	1136	1139	rBV2	262	178	0.01%	0.001%
29	4.791	1148	1151	1153	rBV	275	144	0.01%	0.001%
30	4.856	1169	1171	1173	rBV	139	76	0.00%	0.001%
31	4.926	1190	1193	1198	rVB3	339	310	0.02%	0.002%
32	4.958	1198	1203	1208	rBV2	193	227	0.01%	0.002%
33	4.984	1208	1211	1212	rBV	203	109	0.01%	0.001%
34	5.052	1213	1232	1262	rBV2	649273	1663221	100.00%	12.757%
35	5.438	1350	1352	1354	rBV2	289	164	0.01%	0.001%
36	5.495	1365	1370	1373	rBV2	326	324	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020096.D
 Acq On : 20 Jan 2021 23:15
 Operator : SY/MD
 Sample : M1181-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

37	5.550	1384	1387	1390	rBV2	283	211	0.01%	0.002%
38	5.621	1396	1409	1441	rBV	510160	1009192	60.68%	7.741%
39	5.798	1462	1464	1465	rBV	429	225	0.01%	0.002%
40	5.913	1487	1500	1524	rVB6	33773	78986	4.75%	0.606%
41	6.074	1536	1550	1573	rBV	365429	742296	44.63%	5.693%
42	6.460	1668	1670	1674	rBV	172	152	0.01%	0.001%
43	6.576	1704	1706	1709	rVB2	305	129	0.01%	0.001%
44	6.595	1709	1712	1716	rBV2	357	365	0.02%	0.003%
45	6.682	1736	1739	1740	rBV	120	72	0.00%	0.001%
46	6.711	1746	1748	1749	rBV	161	45	0.00%	0.000%
47	6.737	1754	1756	1758	rBV	174	92	0.01%	0.001%
48	6.949	1819	1822	1824	rBV3	258	163	0.01%	0.001%
49	6.991	1824	1835	1865	rVV	200548	362747	21.81%	2.782%
50	7.164	1887	1889	1894	rBV3	407	389	0.02%	0.003%
51	7.190	1894	1897	1899	rBV2	418	256	0.02%	0.002%
52	7.248	1913	1915	1921	rVB3	285	240	0.01%	0.002%
53	7.322	1921	1938	1959	rBV	780576	1358189	81.66%	10.417%
54	7.627	2023	2033	2052	rBV	139683	238252	14.32%	1.827%
55	7.900	2115	2118	2120	rBV	244	170	0.01%	0.001%
56	7.913	2120	2122	2125	rBV3	418	263	0.02%	0.002%
57	7.981	2131	2143	2158	rBV2	206951	344902	20.74%	2.645%
58	8.093	2168	2178	2207	rBV2	365707	699399	42.05%	5.364%
59	8.454	2289	2290	2294	rBV2	225	117	0.01%	0.001%
60	8.476	2294	2297	2305	rVB4	457	401	0.02%	0.003%
61	8.511	2305	2308	2311	rBV2	376	250	0.02%	0.002%
62	8.569	2323	2326	2332	rVB3	548	531	0.03%	0.004%
63	8.598	2332	2335	2337	rBV	364	201	0.01%	0.002%
64	8.643	2345	2349	2352	rBV	211	173	0.01%	0.001%
65	8.691	2361	2364	2366	rVB3	303	160	0.01%	0.001%
66	8.727	2371	2375	2384	rBV4	1132	1942	0.12%	0.015%
67	8.778	2389	2391	2394	rBV3	383	216	0.01%	0.002%
68	8.859	2404	2416	2442	rBV	774768	1262123	75.88%	9.681%
69	9.193	2517	2520	2523	rBV	331	267	0.02%	0.002%
70	9.588	2639	2643	2646	rBV2	381	335	0.02%	0.003%
71	9.826	2714	2717	2718	rBV	201	95	0.01%	0.001%
72	10.003	2769	2772	2773	rBV	446	268	0.02%	0.002%
73	10.097	2799	2801	2806	rBV3	337	227	0.01%	0.002%
74	10.222	2827	2840	2860	rBV	473723	740299	44.51%	5.678%
75	10.881	3039	3045	3048	rBV2	414	489	0.03%	0.004%
76	11.170	3132	3135	3137	rBV	474	313	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020096.D
Acq On : 20 Jan 2021 23:15
Operator : SY/MD
Sample : M1181-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

77	11.257	3150	3162	3188	rBV	823719	1261067	75.82%	9.672%
78	11.543	3249	3251	3256	rVB2	342	214	0.01%	0.002%
79	11.630	3266	3278	3299	rBV	831985	1314025	79.00%	10.079%
80	12.132	3432	3434	3437	rBV2	312	125	0.01%	0.001%
81	12.225	3462	3463	3464	rBV2	255	83	0.00%	0.001%
82	13.276	3787	3790	3793	rBV2	890	578	0.03%	0.004%




Sum of corrected areas: 13037679

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020096.D
Acq On : 20 Jan 2021 23:15
Operator : SY/MD
Sample : M1181-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

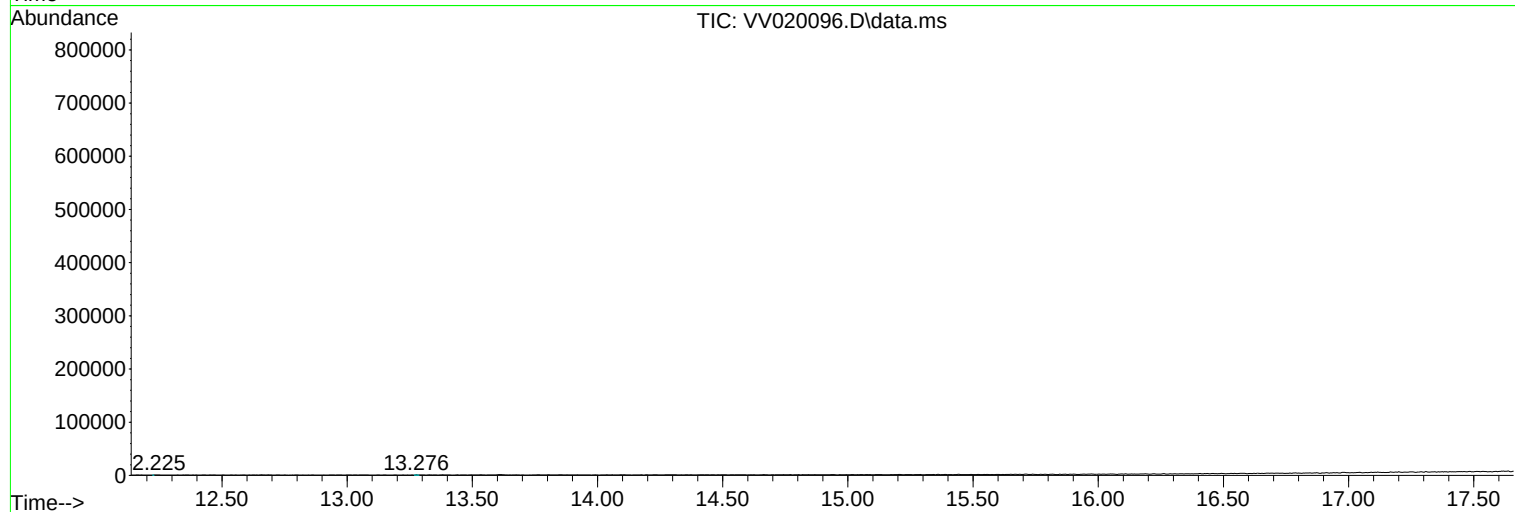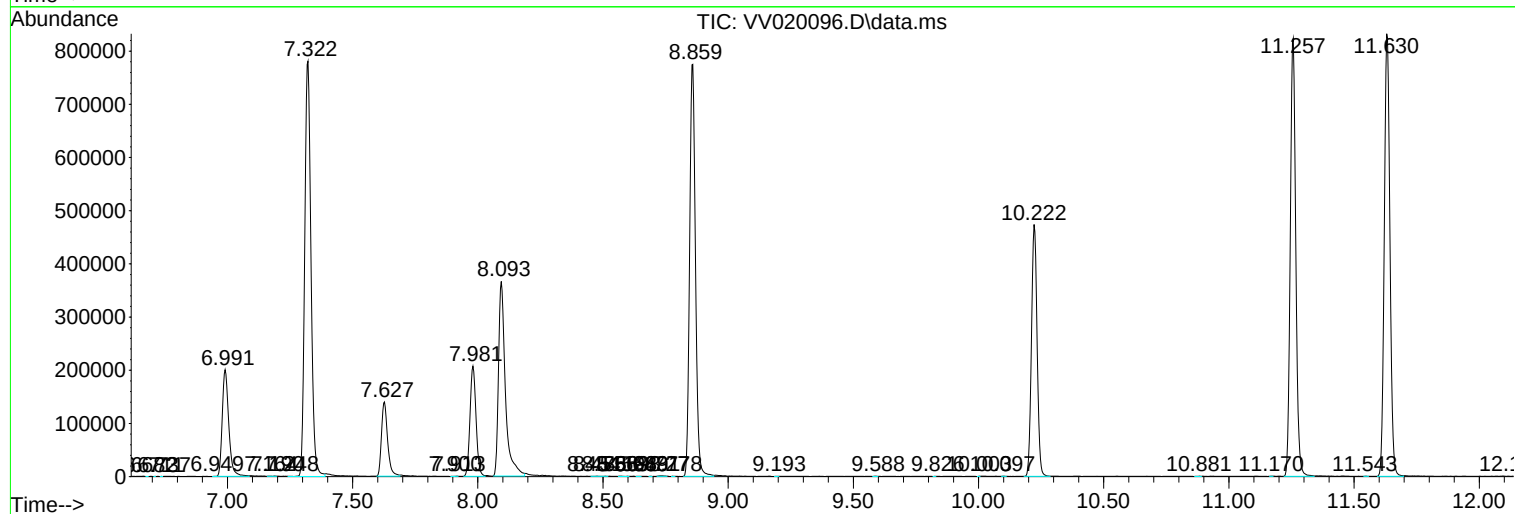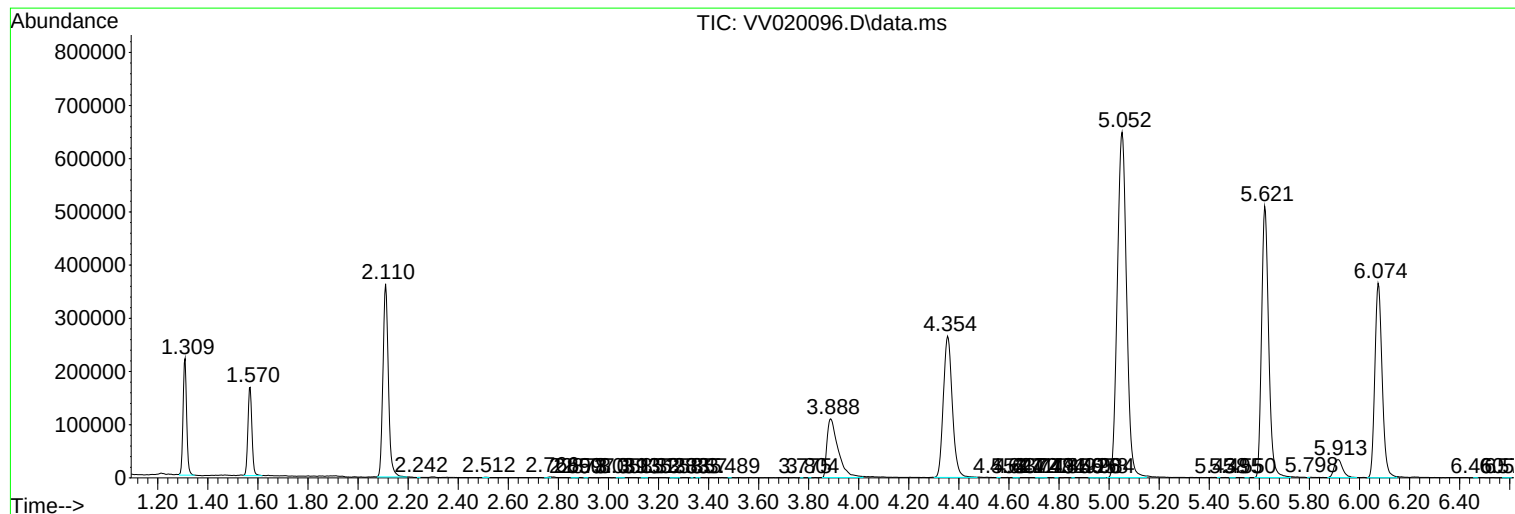

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020096.D
Acq On : 20 Jan 2021 23:15
Operator : SY/MD
Sample : M1181-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020096.D
Acq On : 20 Jan 2021 23:15
Operator : SY/MD
Sample : M1181-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
