

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020097.D
 Acq On : 20 Jan 2021 23:38
 Operator : SY/MD
 Sample : M1181-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

Signal : TIC: VV020097.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	83	rVB	215662	216517	13.32%	1.698%
2	1.566	141	148	160	rVB	163008	181791	11.18%	1.425%
3	2.039	292	295	297	rBV2	821	585	0.04%	0.005%
4	2.110	306	317	346	rVB	365651	547882	33.70%	4.295%
5	2.209	346	348	351	rVB3	1167	725	0.04%	0.006%
6	2.241	351	358	364	rBV4	478	606	0.04%	0.005%
7	2.502	435	439	440	rBV	778	409	0.03%	0.003%
8	2.511	440	442	446	rVB2	934	645	0.04%	0.005%
9	2.682	491	495	499	rBV2	414	323	0.02%	0.003%
10	2.714	501	505	508	rVB2	319	266	0.02%	0.002%
11	2.746	511	515	517	rBV	536	373	0.02%	0.003%
12	2.772	519	523	525	rBV2	628	417	0.03%	0.003%
13	2.904	561	564	568	rBV	231	253	0.02%	0.002%
14	3.174	645	648	653	rVB2	274	226	0.01%	0.002%
15	3.537	758	761	764	rVB2	273	208	0.01%	0.002%
16	3.614	780	785	787	rVB2	326	245	0.02%	0.002%
17	3.640	787	793	795	rBV2	360	300	0.02%	0.002%
18	3.884	858	869	902	rBV	108404	329420	20.26%	2.583%
19	4.238	976	979	983	rBV2	323	246	0.02%	0.002%
20	4.354	998	1015	1046	rVV	258172	649565	39.96%	5.093%
21	4.714	1123	1127	1130	rVB2	293	224	0.01%	0.002%
22	4.810	1153	1157	1158	rBV2	331	212	0.01%	0.002%
23	5.052	1215	1232	1262	rBV2	635153	1625673	100.00%	12.745%
24	5.225	1283	1286	1289	rBV3	606	430	0.03%	0.003%
25	5.286	1299	1305	1306	rBV3	345	296	0.02%	0.002%
26	5.418	1342	1346	1350	rBV3	436	405	0.02%	0.003%
27	5.454	1350	1357	1360	rBV2	484	520	0.03%	0.004%
28	5.498	1368	1371	1376	rVB3	457	401	0.02%	0.003%
29	5.624	1396	1410	1436	rBV	504670	1019506	62.71%	7.993%
30	5.913	1488	1500	1525	rVB4	32999	77578	4.77%	0.608%
31	6.074	1536	1550	1576	rBV	355604	721335	44.37%	5.655%
32	6.309	1621	1623	1627	rVB	433	293	0.02%	0.002%
33	6.334	1627	1631	1633	rBV	821	532	0.03%	0.004%
34	6.373	1640	1643	1647	rVB3	288	216	0.01%	0.002%
35	6.498	1678	1682	1685	rVV2	356	265	0.02%	0.002%
36	6.920	1809	1813	1816	rBV2	258	218	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020097.D
 Acq On : 20 Jan 2021 23:38
 Operator : SY/MD
 Sample : M1181-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

37	6.990	1824	1835	1863	rBV	191078	348545	21.44%	2.733%
38	7.177	1890	1893	1895	rBV3	331	222	0.01%	0.002%
39	7.322	1925	1938	1958	rBV	760067	1318343	81.10%	10.336%
40	7.556	2008	2011	2012	rBV	507	299	0.02%	0.002%
41	7.627	2021	2033	2057	rBV	134463	235256	14.47%	1.844%
42	7.746	2068	2070	2077	rVB3	669	590	0.04%	0.005%
43	7.810	2088	2090	2093	rBV2	335	215	0.01%	0.002%
44	7.981	2132	2143	2168	rVB	134851	228619	14.06%	1.792%
45	8.093	2168	2178	2217	rBV2	355579	688937	42.38%	5.401%
46	8.733	2367	2377	2387	rBV8	2179	4050	0.25%	0.032%
47	8.797	2393	2397	2404	rBV3	405	455	0.03%	0.004%
48	8.859	2404	2416	2451	rBV	776388	1259816	77.50%	9.877%
49	9.158	2501	2509	2520	rVB5	596	1112	0.07%	0.009%
50	9.206	2521	2524	2531	rBV2	362	383	0.02%	0.003%
51	9.350	2567	2569	2576	rVB	307	226	0.01%	0.002%
52	9.389	2576	2581	2585	rBV	508	452	0.03%	0.004%
53	9.592	2641	2644	2648	rBV2	232	230	0.01%	0.002%
54	9.669	2663	2668	2670	rBV	242	232	0.01%	0.002%
55	9.794	2701	2707	2711	rBV2	420	626	0.04%	0.005%
56	9.823	2711	2716	2720	rVV2	198	247	0.02%	0.002%
57	9.846	2720	2723	2728	rBV2	261	279	0.02%	0.002%
58	10.016	2770	2776	2784	rBV6	1346	1964	0.12%	0.015%
59	10.222	2828	2840	2862	rBV	454368	717035	44.11%	5.622%
60	10.370	2883	2886	2888	rBV2	370	224	0.01%	0.002%
61	10.386	2888	2891	2896	rVV3	581	494	0.03%	0.004%
62	10.569	2945	2948	2951	rBV3	421	236	0.01%	0.002%
63	10.611	2958	2961	2967	rBV3	248	316	0.02%	0.002%
64	10.836	3028	3031	3033	rBV2	301	207	0.01%	0.002%
65	10.942	3061	3064	3066	rBV	433	282	0.02%	0.002%
66	11.000	3079	3082	3085	rVB2	378	210	0.01%	0.002%
67	11.174	3134	3136	3139	rBV	360	219	0.01%	0.002%
68	11.257	3150	3162	3189	rBV	825727	1272754	78.29%	9.978%
69	11.437	3215	3218	3220	rBV3	561	436	0.03%	0.003%
70	11.630	3265	3278	3298	rBV	816856	1280233	78.75%	10.037%
71	11.810	3332	3334	3342	rVB2	675	578	0.04%	0.005%
72	11.945	3369	3376	3380	rBV3	457	648	0.04%	0.005%
73	12.032	3400	3403	3405	rBV	441	262	0.02%	0.002%
74	12.093	3415	3422	3431	rBV4	857	1199	0.07%	0.009%
75	12.299	3481	3486	3487	rVV2	289	220	0.01%	0.002%
76	12.453	3530	3534	3542	rBV4	330	417	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020097.D
 Acq On : 20 Jan 2021 23:38
 Operator : SY/MD
 Sample : M1181-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

77	12.611	3581	3583	3585	rBV	325	210	0.01%	0.002%
78	12.665	3596	3600	3604	rVB	634	483	0.03%	0.004%
79	12.694	3604	3609	3612	rBV	462	360	0.02%	0.003%
80	12.720	3614	3617	3622	rVB2	333	244	0.02%	0.002%
81	12.868	3661	3663	3667	rVB2	343	214	0.01%	0.002%
82	12.891	3667	3670	3673	rBV3	328	206	0.01%	0.002%
83	12.932	3680	3683	3688	rBV2	313	210	0.01%	0.002%
84	13.064	3722	3724	3729	rVB	462	235	0.01%	0.002%
85	13.125	3741	3743	3745	rBV	409	244	0.02%	0.002%
86	13.209	3766	3769	3772	rBV3	324	258	0.02%	0.002%
87	13.270	3785	3788	3798	rBV4	797	863	0.05%	0.007%
88	13.405	3827	3830	3832	rBV3	333	273	0.02%	0.002%
89	13.566	3876	3880	3881	rBV2	346	230	0.01%	0.002%
90	13.608	3890	3893	3900	rVB3	1028	1295	0.08%	0.010%
91	13.849	3964	3968	3972	rBV3	315	278	0.02%	0.002%
92	13.907	3984	3986	3993	rVB2	579	586	0.04%	0.005%
93	13.939	3993	3996	4000	rBV	369	326	0.02%	0.003%
94	14.093	4040	4044	4047	rBV3	485	492	0.03%	0.004%
95	14.273	4096	4100	4101	rBV2	470	292	0.02%	0.002%
96	14.421	4141	4146	4147	rBV2	500	422	0.03%	0.003%
97	14.923	4298	4302	4304	rBV2	426	296	0.02%	0.002%
98	15.025	4332	4334	4337	rBV3	461	209	0.01%	0.002%
99	15.087	4350	4353	4355	rBV2	446	335	0.02%	0.003%
100	15.418	4454	4456	4458	rBV3	437	235	0.01%	0.002%




Sum of corrected areas: 12754970

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020097.D
Acq On : 20 Jan 2021 23:38
Operator : SY/MD
Sample : M1181-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

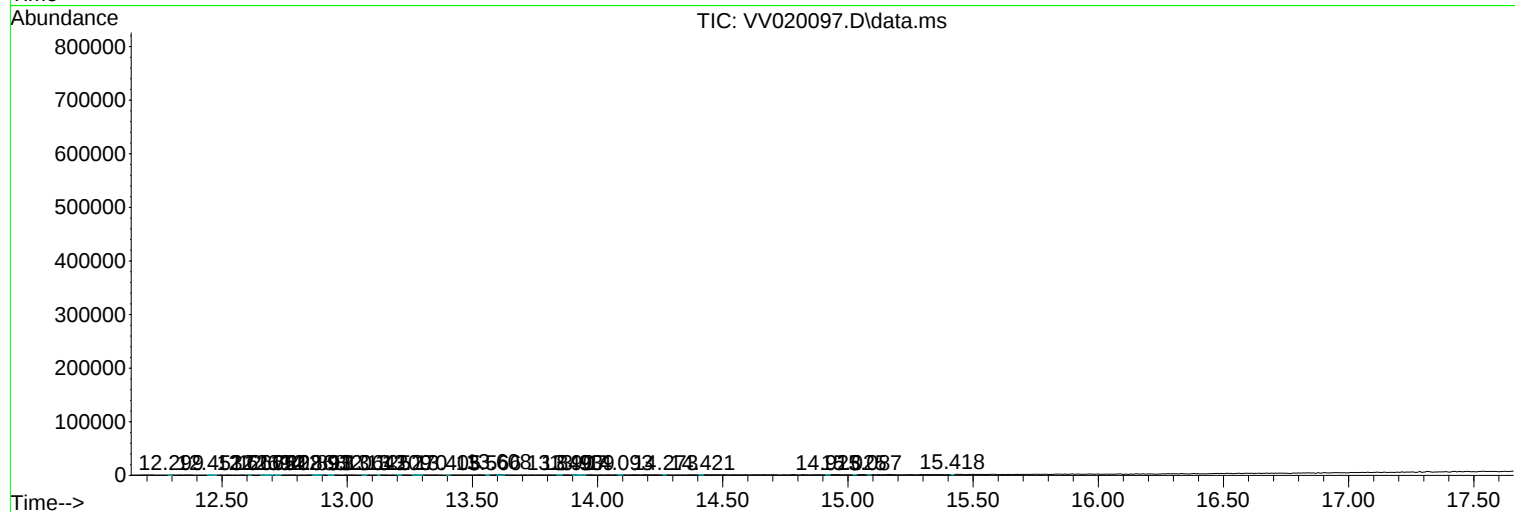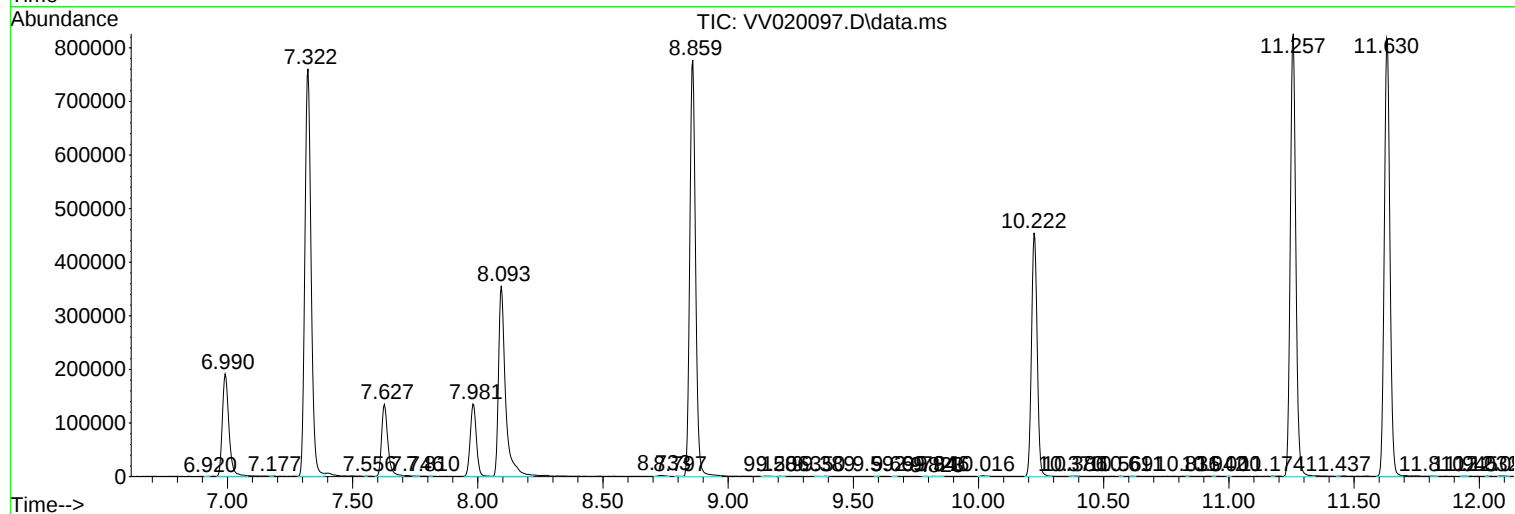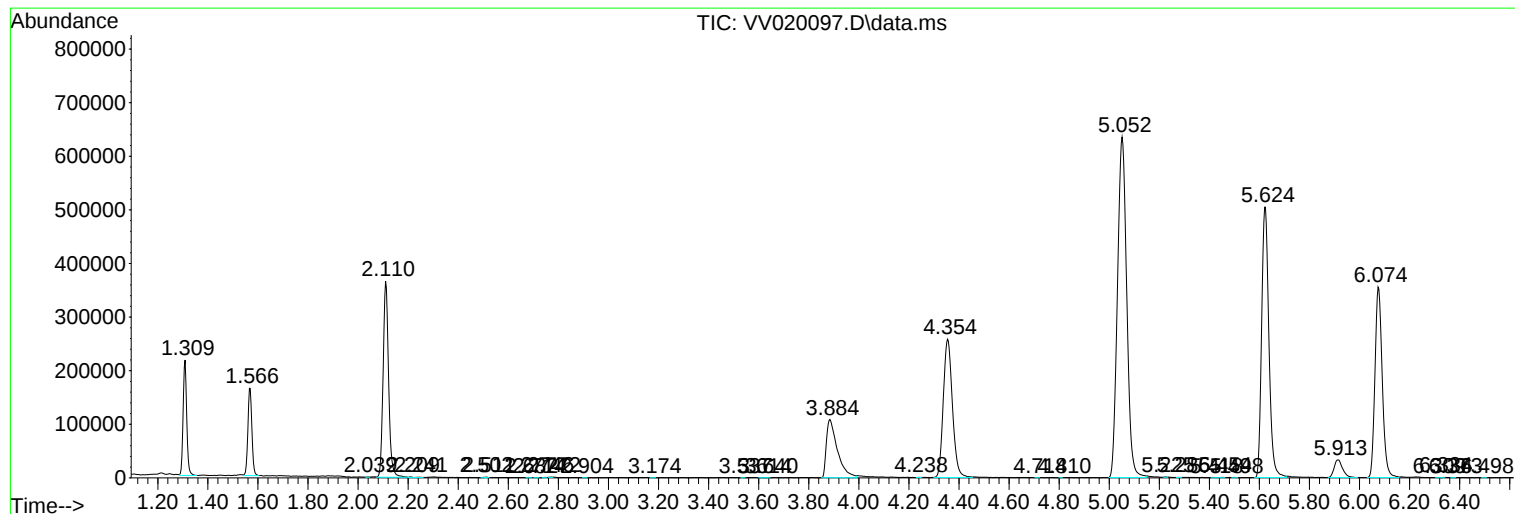

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020097.D
Acq On : 20 Jan 2021 23:38
Operator : SY/MD
Sample : M1181-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020097.D
Acq On : 20 Jan 2021 23:38
Operator : SY/MD
Sample : M1181-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------