

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020098.D
 Acq On : 21 Jan 2021 00:02
 Operator : SY/MD
 Sample : M1181-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E51

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

Signal : TIC: VV020098.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	87	rVB	230375	238208	13.99%	1.796%
2	1.569	142	149	159	rVB	178395	194061	11.40%	1.463%
3	2.110	307	317	344	rVB	375589	571951	33.59%	4.312%
4	2.357	391	394	398	rBV4	599	527	0.03%	0.004%
5	2.508	439	441	448	rVB4	627	588	0.03%	0.004%
6	2.553	453	455	460	rVB2	231	172	0.01%	0.001%
7	2.576	460	462	465	rBV2	259	173	0.01%	0.001%
8	2.647	482	484	489	rVB	434	279	0.02%	0.002%
9	2.669	489	491	492	rBV	198	62	0.00%	0.000%
10	2.698	498	500	504	rVB	388	155	0.01%	0.001%
11	2.836	540	543	546	rVB2	215	122	0.01%	0.001%
12	2.891	554	560	563	rBV2	323	330	0.02%	0.002%
13	2.987	586	590	593	rBV	271	201	0.01%	0.002%
14	3.113	627	629	631	rVB2	234	62	0.00%	0.000%
15	3.167	644	646	650	rBV2	134	100	0.01%	0.001%
16	3.200	650	656	659	rBV3	268	288	0.02%	0.002%
17	3.245	669	670	671	rBV3	180	54	0.00%	0.000%
18	3.277	677	680	686	rVB2	243	192	0.01%	0.001%
19	3.438	727	730	734	rBV	381	214	0.01%	0.002%
20	3.518	749	755	757	rBV2	252	260	0.02%	0.002%
21	3.540	758	762	764	rBV2	206	117	0.01%	0.001%
22	3.656	797	798	799	rBV2	130	41	0.00%	0.000%
23	3.685	806	807	809	rBV	137	76	0.00%	0.001%
24	3.695	809	810	811	rVV	174	45	0.00%	0.000%
25	3.884	858	869	910	rBV	116513	357057	20.97%	2.692%
26	4.354	999	1015	1041	rBV	273134	675043	39.65%	5.089%
27	4.614	1094	1096	1097	rBV	340	148	0.01%	0.001%
28	4.714	1123	1127	1129	rBV3	257	229	0.01%	0.002%
29	4.769	1141	1144	1147	rBV4	228	164	0.01%	0.001%
30	4.862	1170	1173	1178	rVB2	181	154	0.01%	0.001%
31	4.897	1178	1184	1188	rBV2	270	293	0.02%	0.002%
32	4.913	1188	1189	1190	rBV	258	69	0.00%	0.001%
33	4.949	1197	1200	1203	rBV2	208	163	0.01%	0.001%
34	5.052	1213	1232	1262	rBV2	656016	1702505	100.00%	12.835%
35	5.463	1354	1360	1364	rBV2	411	489	0.03%	0.004%
36	5.482	1364	1366	1367	rBV	260	114	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020098.D
 Acq On : 21 Jan 2021 00:02
 Operator : SY/MD
 Sample : M1181-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E51

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis

37	5.621	1395	1409	1437	rBV	516287	1032195	60.63%	7.782%
38	5.913	1487	1500	1521	rBV4	36170	82293	4.83%	0.620%
39	6.074	1536	1550	1580	rBV	372447	757180	44.47%	5.708%
40	6.338	1631	1632	1634	rBV	167	67	0.00%	0.001%
41	6.412	1650	1655	1657	rBV2	210	189	0.01%	0.001%
42	6.463	1669	1671	1673	rVB	213	83	0.00%	0.001%
43	6.482	1673	1677	1682	rBV2	212	243	0.01%	0.002%
44	6.518	1686	1688	1690	rBV	243	101	0.01%	0.001%
45	6.547	1695	1697	1701	rVB2	289	134	0.01%	0.001%
46	6.566	1701	1703	1705	rBV	248	136	0.01%	0.001%
47	6.663	1731	1733	1739	rVB3	458	265	0.02%	0.002%
48	6.695	1739	1743	1747	rBV2	420	401	0.02%	0.003%
49	6.759	1761	1763	1767	rBV	286	201	0.01%	0.002%
50	6.900	1805	1807	1810	rVV	235	101	0.01%	0.001%
51	6.926	1814	1815	1816	rVB	227	44	0.00%	0.000%
52	6.990	1823	1835	1856	rBV	203958	364605	21.42%	2.749%
53	7.322	1925	1938	1957	rBV	793327	1378564	80.97%	10.393%
54	7.627	2022	2033	2055	rBV	140894	244123	14.34%	1.840%
55	7.807	2087	2089	2094	rVB2	697	483	0.03%	0.004%
56	7.839	2095	2099	2102	rBV2	391	295	0.02%	0.002%
57	7.865	2102	2107	2109	rBV3	490	339	0.02%	0.003%
58	7.929	2123	2127	2129	rBV3	324	272	0.02%	0.002%
59	7.981	2131	2143	2158	rVV	140387	236364	13.88%	1.782%
60	8.093	2167	2178	2214	rBV2	378108	738758	43.39%	5.570%
61	8.643	2347	2349	2351	rBV2	267	135	0.01%	0.001%
62	8.678	2358	2360	2362	rBV	136	68	0.00%	0.001%
63	8.730	2369	2376	2387	rVB4	1666	3011	0.18%	0.023%
64	8.810	2399	2401	2403	rBV2	231	78	0.00%	0.001%
65	8.855	2403	2415	2438	rBV	787331	1283182	75.37%	9.674%
66	9.064	2477	2480	2483	rBV2	737	500	0.03%	0.004%
67	9.203	2519	2523	2526	rVB3	292	194	0.01%	0.001%
68	9.289	2548	2550	2554	rVB2	289	161	0.01%	0.001%
69	9.328	2560	2562	2564	rBV	252	91	0.01%	0.001%
70	9.444	2594	2598	2607	rVB2	299	331	0.02%	0.002%
71	9.482	2607	2610	2611	rVV	290	138	0.01%	0.001%
72	9.505	2615	2617	2619	rVV	275	124	0.01%	0.001%
73	9.534	2623	2626	2630	rVV	309	193	0.01%	0.001%
74	9.553	2630	2632	2639	rVB2	323	320	0.02%	0.002%
75	9.614	2649	2651	2652	rBV	165	76	0.00%	0.001%
76	9.630	2654	2656	2659	rBV2	332	172	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020098.D
 Acq On : 21 Jan 2021 00:02
 Operator : SY/MD
 Sample : M1181-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E51

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M

Title : VOC Analysis

77	9.752	2692	2694	2697	rVB2	341	189	0.01%	0.001%
78	9.775	2698	2701	2702	rBV	277	153	0.01%	0.001%
79	9.955	2755	2757	2759	rBV2	238	115	0.01%	0.001%
80	10.093	2797	2800	2802	rBV	301	163	0.01%	0.001%
81	10.222	2828	2840	2868	rVB	483309	752475	44.20%	5.673%
82	10.386	2889	2891	2892	rBV	411	154	0.01%	0.001%
83	10.473	2916	2918	2920	rBV	333	137	0.01%	0.001%
84	10.733	2996	2999	3001	rBV	507	272	0.02%	0.002%
85	11.257	3150	3162	3186	rBV	828144	1290719	75.81%	9.731%
86	11.453	3221	3223	3224	rBV	661	282	0.02%	0.002%
87	11.630	3266	3278	3295	rBV	859300	1348070	79.18%	10.163%
88	13.318	3801	3803	3807	rVB3	441	207	0.01%	0.002%
89	13.363	3813	3817	3818	rBV2	505	352	0.02%	0.003%




Sum of corrected areas: 13264204

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020098.D
Acq On : 21 Jan 2021 00:02
Operator : SY/MD
Sample : M1181-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

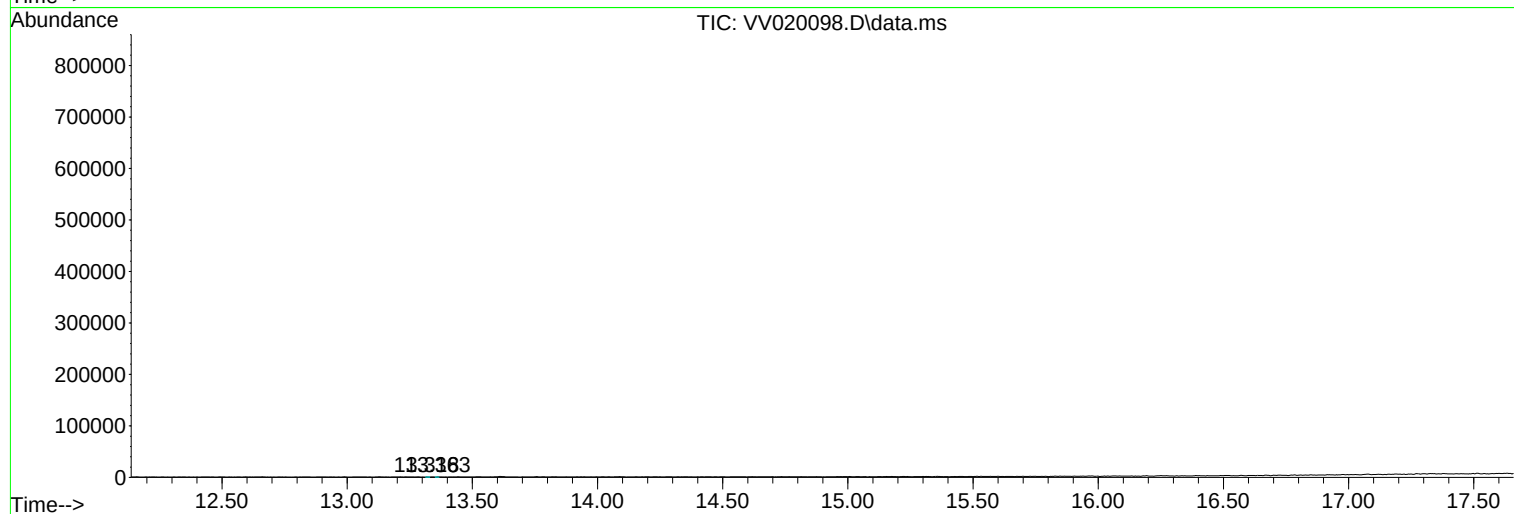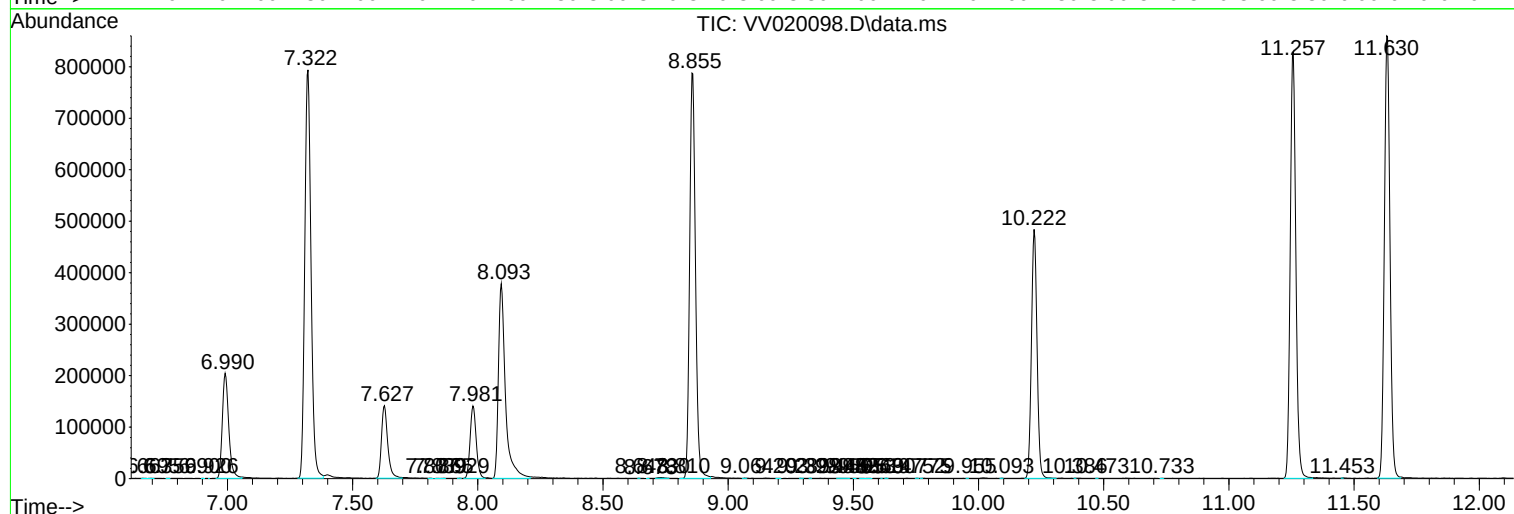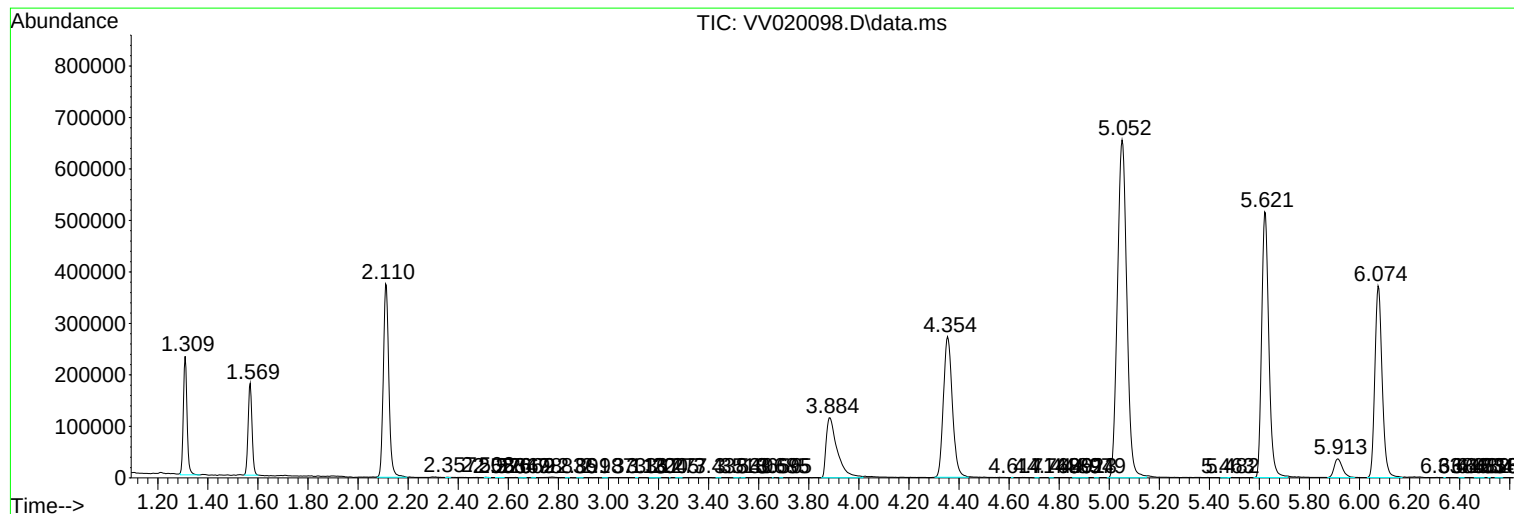

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020098.D
Acq On : 21 Jan 2021 00:02
Operator : SY/MD
Sample : M1181-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
Data File : VV020098.D
Acq On : 21 Jan 2021 00:02
Operator : SY/MD
Sample : M1181-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
