


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012021\
 Data File : VV020069.D
 Acq On : 20 Jan 2021 09:16
 Operator : SY/MD
 Sample : BFB84
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB84

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012021WMA.M
 Title : VOC Analysis
 Last Update : Wed Jan 20 23:39:20 2021

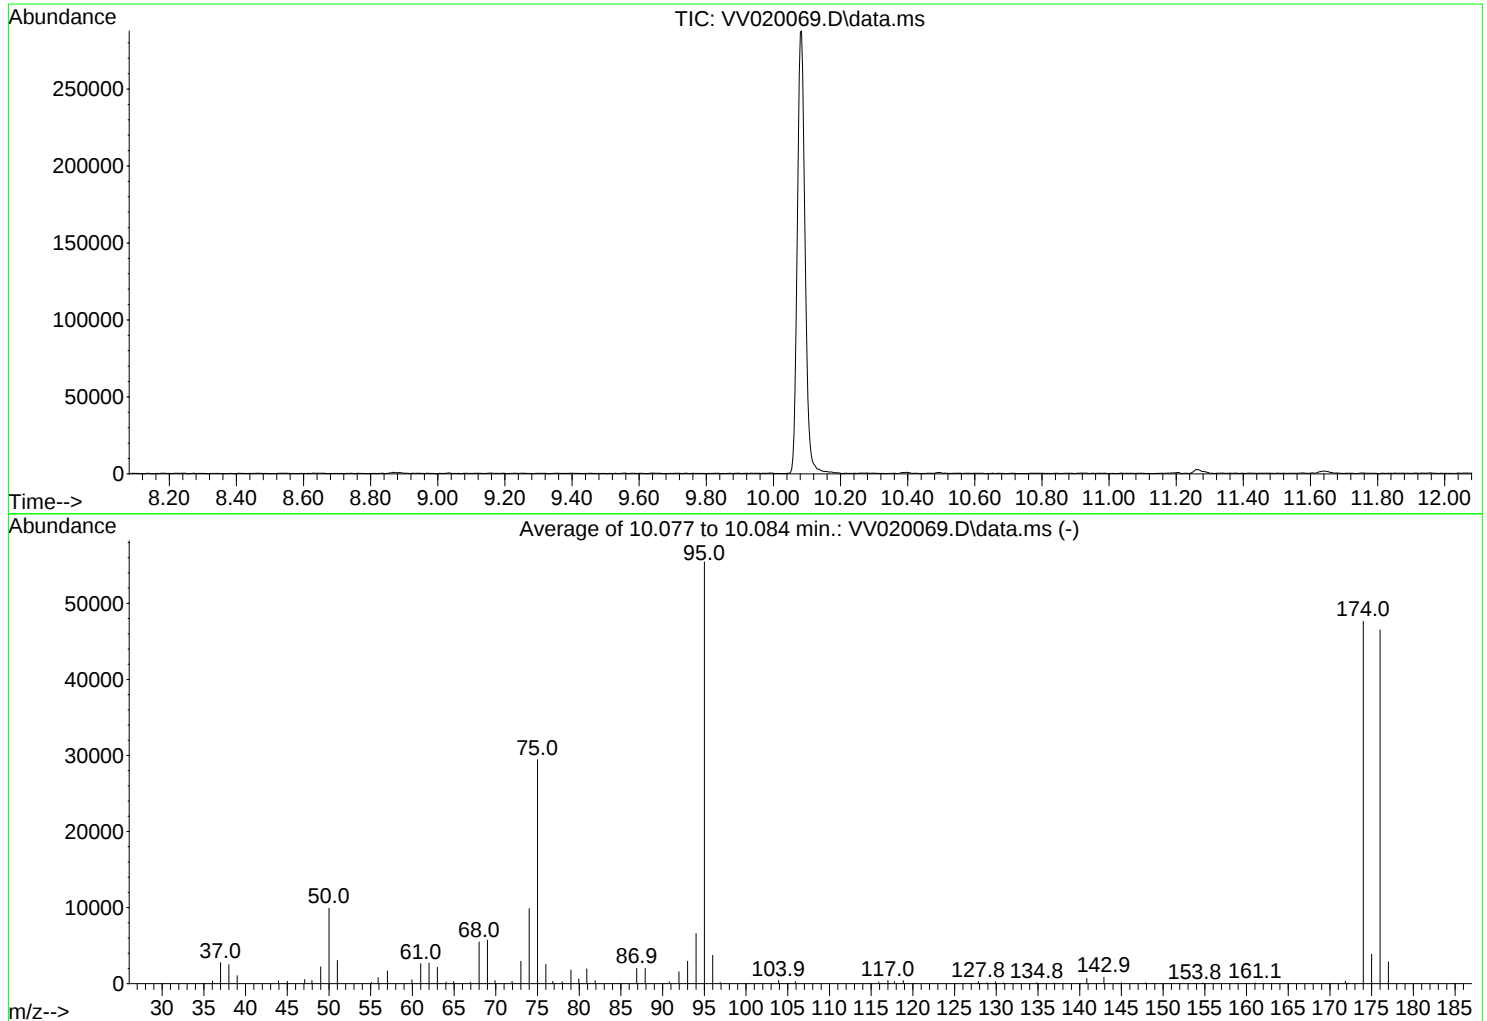

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2785

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	9901	PASS
75	95	30	80	53.1	29453	PASS
95	95	100	100	100.0	55461	PASS
96	95	5	9	6.7	3724	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.9	47637	PASS
175	174	5	9	8.1	3879	PASS
176	174	95	101	97.6	46507	PASS
177	176	5	9	6.2	2869	PASS

m/z	Abundance
39.90	153.0
43.90	231.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	369.0
37.00	2708.0
38.00	2452.0
39.00	1006.0
39.90	209.0
44.00	573.0
45.00	327.0
47.10	471.0
48.00	463.0
49.00	2078.0
50.00	9267.0
51.00	2920.0
55.10	163.0
55.90	797.0
57.00	1666.0
59.90	453.0
61.00	2463.0
62.00	2650.0
63.00	2107.0
64.00	179.0
64.90	237.0
66.90	211.0
68.00	5377.0
69.00	5453.0
69.90	402.0
72.00	259.0
73.00	2649.0
74.00	9464.0
75.00	28024.0
76.00	2342.0
76.90	298.0
78.00	258.0
79.00	1702.0
80.00	632.0
80.90	1789.0
81.90	397.0
86.90	1961.0
87.90	1782.0
90.80	192.0
91.90	1421.0
93.00	2658.0
94.00	6361.0
95.00	52368.0
96.00	3697.0
96.90	170.0
103.90	319.0
105.90	244.0
116.00	208.0
117.00	336.0
117.80	216.0
118.80	355.0
127.80	288.0
128.80	153.0
129.90	240.0
130.90	114.0
134.90	110.0
140.80	631.0
142.90	762.0
145.00	113.0
147.90	166.0
161.00	110.0
171.90	289.0
172.20	253.0
174.00	43152.0
175.00	3636.0
176.00	41936.0
177.00	2643.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	363.0
37.00	2863.0
38.00	2565.0
39.00	1089.0
39.90	147.0
44.00	632.0
45.00	325.0
47.10	566.0
48.00	439.0
49.00	2258.0
50.00	10227.0
51.00	3111.0
55.10	181.0
55.90	831.0
57.00	1713.0
59.90	550.0
61.00	2708.0
62.00	2767.0
63.00	2200.0
64.10	218.0
64.90	289.0
66.90	205.0
68.00	5684.0
69.00	5886.0
69.90	417.0
71.90	292.0
73.00	3041.0
74.00	10128.0
75.00	30320.0
76.00	2636.0
76.90	333.0
77.90	264.0
79.00	1840.0
79.90	665.0
80.90	2005.0
81.90	412.0
86.90	2052.0
87.90	2045.0
90.80	240.0
92.00	1558.0
93.00	3072.0
94.00	6782.0
95.00	57144.0
96.00	3877.0
96.90	165.0
103.90	427.0
105.90	267.0
115.90	194.0
117.00	441.0
117.80	257.0
118.80	441.0
127.90	278.0
128.90	124.0
129.90	238.0
130.90	130.0
134.90	122.0
136.90	103.0
140.90	712.0
142.90	880.0
145.00	143.0
147.90	140.0
154.80	126.0
161.10	120.0
171.90	309.0
174.00	49336.0
175.00	4023.0
176.00	48128.0
177.00	3009.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.10	373.0
37.00	2720.0
38.00	2480.0
39.00	1091.0
44.00	637.0
45.00	328.0
47.10	597.0
47.90	359.0
49.00	2276.0
50.00	10208.0
51.00	3107.0
55.10	169.0
55.90	806.0
57.00	1617.0
60.00	533.0
61.00	2718.0
62.00	2746.0
63.00	2107.0
64.10	262.0
65.00	282.0
67.00	182.0
68.00	5349.0
69.00	5810.0
69.90	404.0
71.90	315.0
73.00	3152.0
74.00	10018.0
75.00	30016.0
76.00	2587.0
76.80	323.0
77.90	213.0
79.00	1804.0
79.90	625.0
80.90	2037.0
81.90	414.0
86.90	2005.0
87.90	2154.0
90.80	256.0
92.00	1695.0
93.00	3098.0
94.00	6636.0
95.00	56872.0
96.00	3597.0
96.90	106.0
103.90	430.0
104.90	114.0
105.90	308.0
115.80	232.0
117.00	480.0
117.80	273.0
118.90	410.0
127.90	239.0
129.00	112.0
129.90	245.0
130.80	106.0
134.80	141.0
136.90	144.0
140.90	769.0
142.90	882.0
145.00	135.0
148.90	102.0
153.80	101.0
154.80	126.0
161.10	111.0
171.80	340.0
174.00	50424.0
175.00	3978.0
176.00	49456.0
177.00	2955.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84