




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
Data File : VV038454.D
Acq On : 20 Jan 2025 10:59
Operator : SY/MD
Sample : VV0120wBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK269

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/21/2025
Supervised By :Mahesh Dadoda 01/21/2025

Quant Time: Jan 21 00:57:16 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725wMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 21 00:50:24 2025
Response via : Initial Calibration

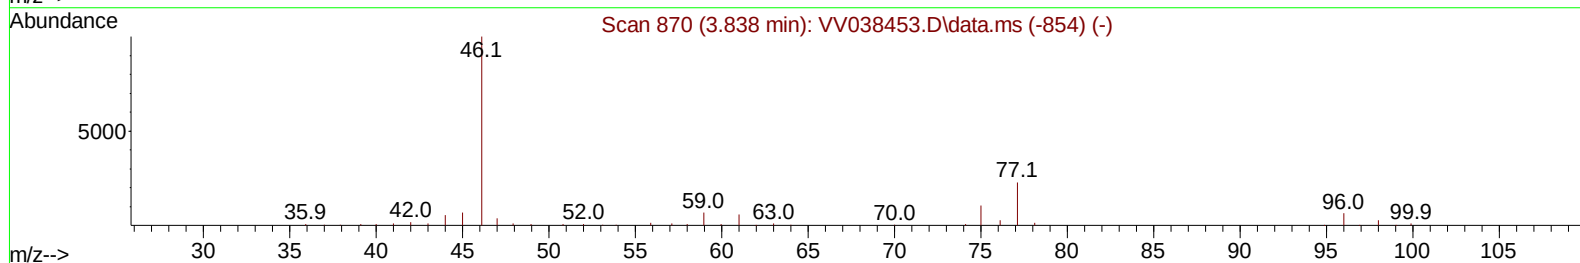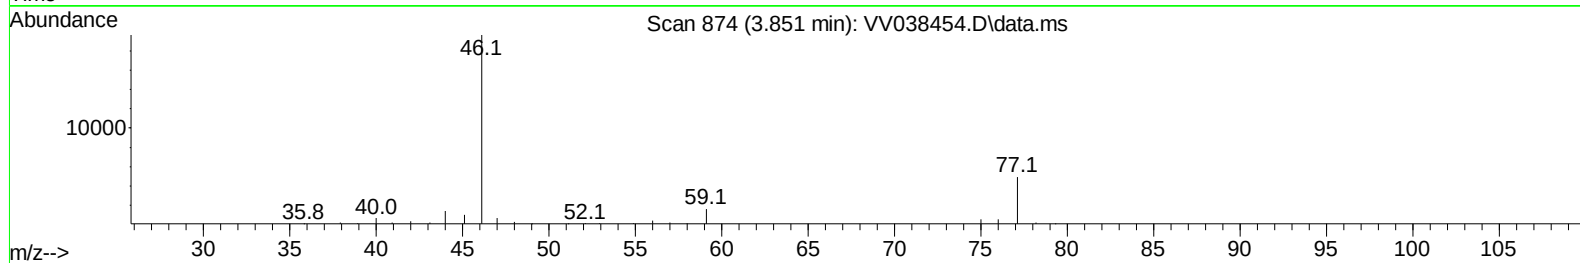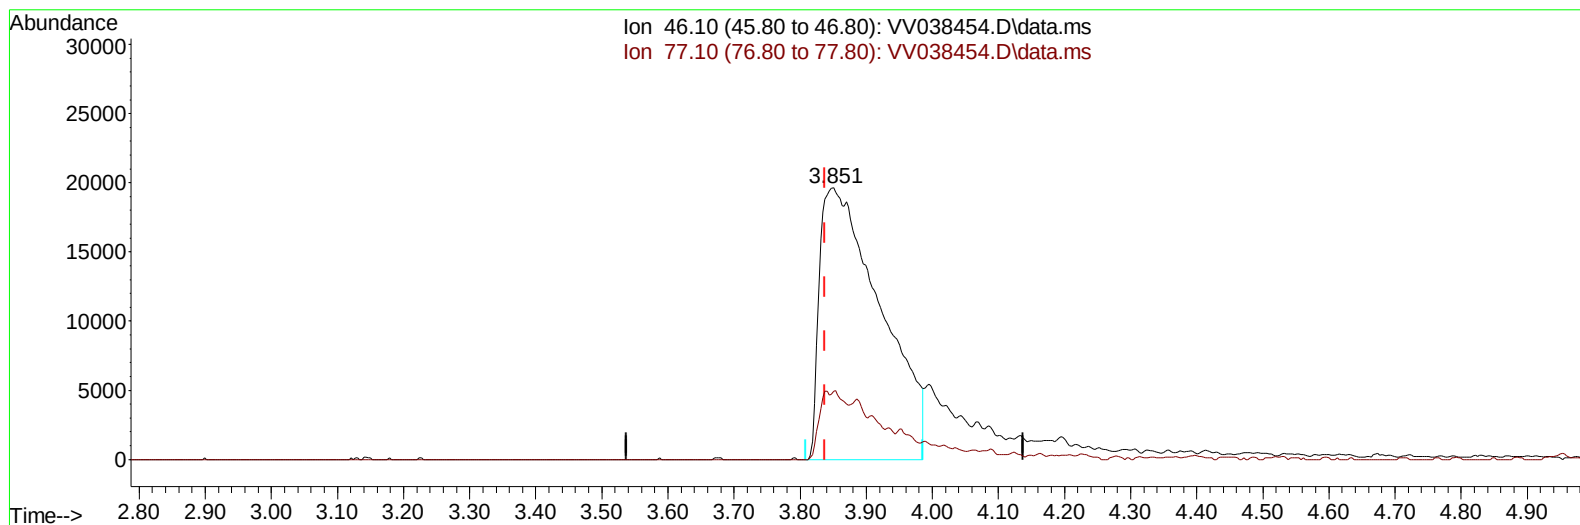

TIC: VV038454.D\data.ms

(20) 2-Butanone-d5 (S)**3.851min (+ 0.013) 34.23 ug/L****response 125718**

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.70	4.46#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
Data File : VV038454.D
Acq On : 20 Jan 2025 10:59
Operator : SY/MD
Sample : VV0120wBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK269

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/21/2025
Supervised By :Mahesh Dadoda 01/21/2025

Quant Time: Jan 21 00:57:16 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725wMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 21 00:50:24 2025
Response via : Initial Calibration

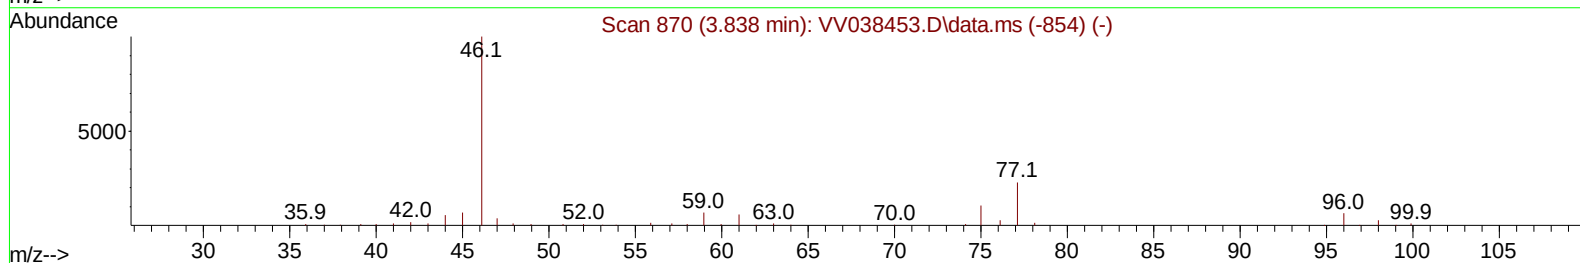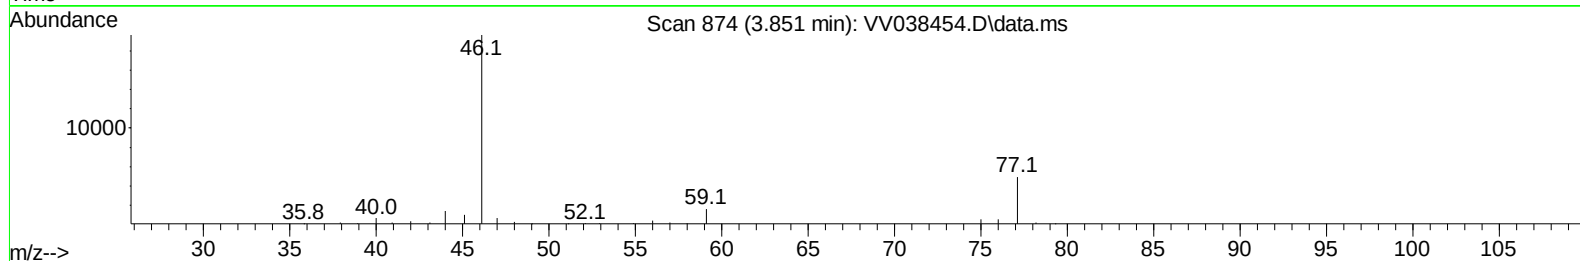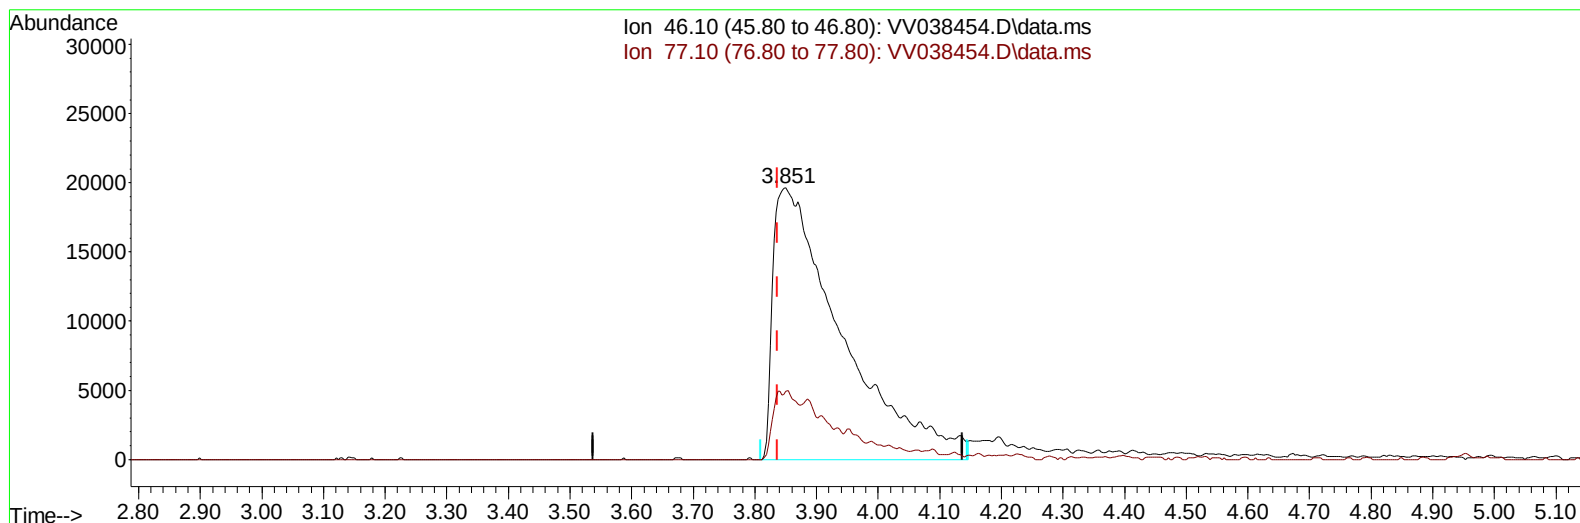

TIC: VV038454.D\data.ms

(20) 2-Butanone-d5 (S)**3.851min (+ 0.013) 41.45 ug/L m****response 152221**

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.70	3.69#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
 Data File : VV038454.D
 Acq On : 20 Jan 2025 10:59
 Operator : SY/MD
 Sample : VV0120WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK269

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/21/2025
 Supervised By :Mahesh Dadoda 01/21/2025

Quant Time: Jan 21 00:57:16 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 21 00:50:24 2025
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.526	114		211734	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117		225389	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152		91347	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.275	65		82240	4.710	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.200%	
7) Chloroethane-d5	1.529	69		70561	4.812	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.200%	
11) 1,1-Dichloroethene-d2	2.053	65		37702	4.792	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	95.800%	
20) 2-Butanone-d5	3.851	46		152221m	41.450	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	82.900%	
24) Chloroform-d	4.240	84		152842	4.670	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%	
26) 1,2-Dichloroethane-d4	4.937	65		73544	4.904	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.000%	
32) Benzene-d6	4.950	84		288267	4.644	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.800%	
36) 1,2-Dichloropropane-d6	5.979	67		94268	4.996	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.000%	
41) Toluene-d8	7.236	98		229914	4.123	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.400%	
43) trans-1,3-Dichloroprop...	7.558	79		27231	3.945	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.000%	
46) 2-Hexanone-d5	8.027	63		92104	33.824	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	67.640%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84		66106	4.419	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.400%	
66) 1,2-Dichlorobenzene-d4	11.554	152		78983	5.109	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.200%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
Data File : VV038454.D
Acq On : 20 Jan 2025 10:59
Operator : SY/MD
Sample : VV0120WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK269

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/21/2025
Supervised By :Mahesh Dadoda 01/21/2025

Quant Time: Jan 21 00:57:16 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 21 00:50:24 2025
Response via : Initial Calibration

