

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
 Data File : VV038459.D
 Acq On : 20 Jan 2025 13:15
 Operator : SY/MD
 Sample : Q1125-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B08

Quant Time: Jan 21 00:52:06 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 21 00:50:24 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	90233	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	93838	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	38034	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	37126	4.989	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.800%
7) Chloroethane-d5	1.532	69	31990	5.120	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.400%
11) 1,1-Dichloroethene-d2	2.053	65	16667	4.970	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	99.400%
20) 2-Butanone-d5	3.786	46	110693	70.728	ug/L	-0.05
Spiked Amount	50.000	Range	40 - 130	Recovery	=	141.460%#
24) Chloroform-d	4.243	84	68250	4.894	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
26) 1,2-Dichloroethane-d4	4.941	65	39050	6.110	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	122.200%
32) Benzene-d6	4.953	84	126359	4.889	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
36) 1,2-Dichloropropane-d6	5.986	67	42065	5.355	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.000%
41) Toluene-d8	7.243	98	94564	4.073	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.400%
43) trans-1,3-Dichloroprop...	7.564	79	12602	4.385	ug/L	0.02
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.800%
46) 2-Hexanone-d5	8.021	63	66764	58.890	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	117.780%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	46120	7.405	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	148.200%#
66) 1,2-Dichlorobenzene-d4	11.554	152	35398	5.499	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.000%
Target Compounds					Qvalue	
16) Methylene chloride	2.442	84	1750	0.211	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
Data File : VV038459.D
Acq On : 20 Jan 2025 13:15
Operator : SY/MD
Sample : Q1125-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B08

Quant Time: Jan 21 00:52:06 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 21 00:50:24 2025
Response via : Initial Calibration

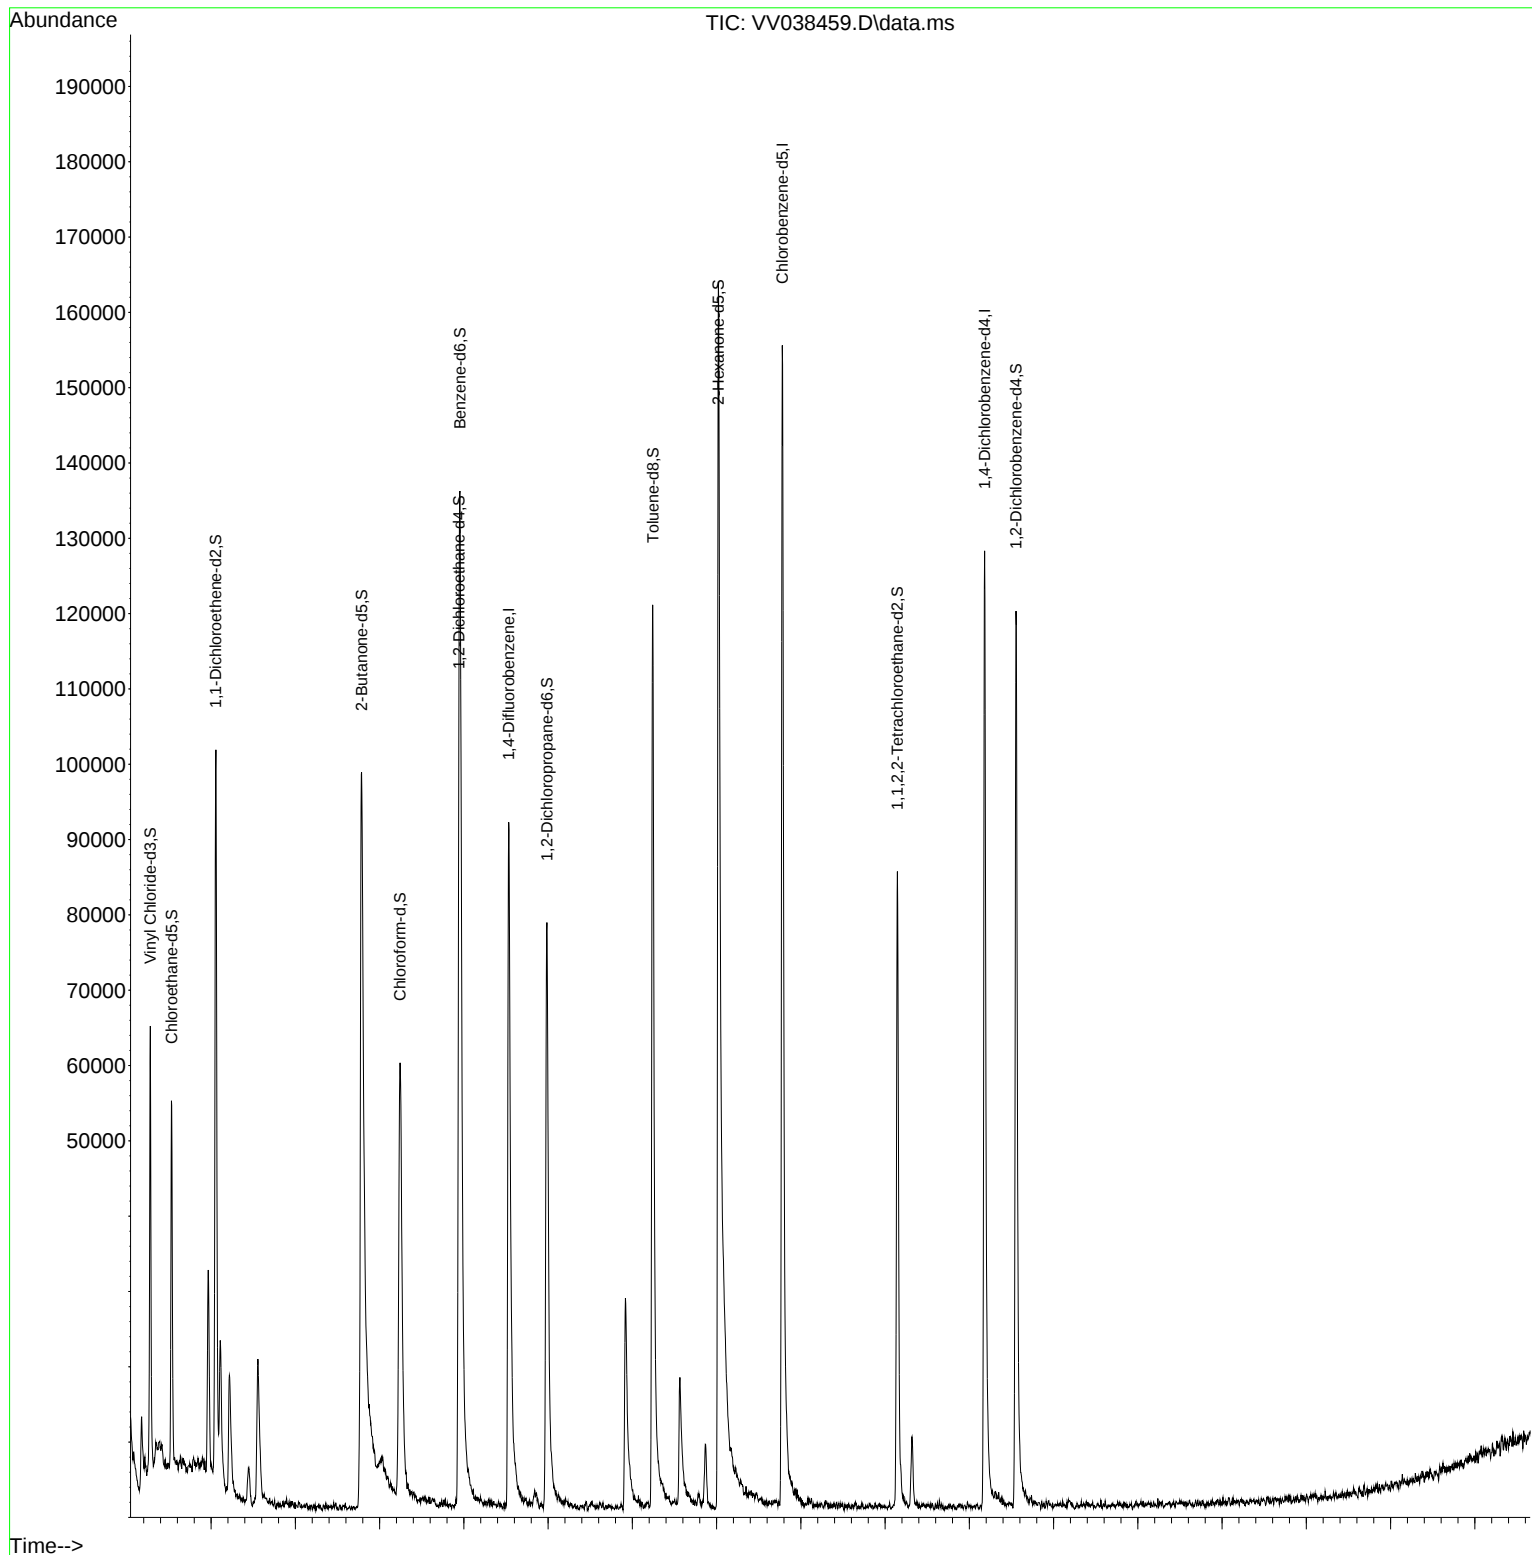

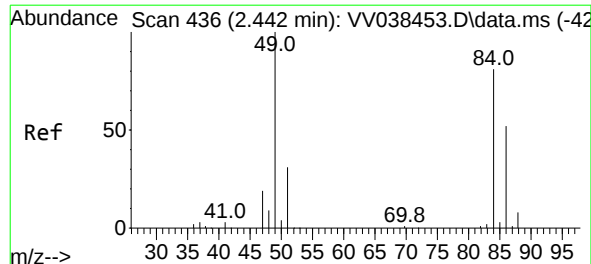

#16
Methylene chloride
Concen: 0.211 ug/L
RT: 2.442 min Scan# 43
Delta R.T. 0.000 min
Lab File: VV038459.D
Acq: 20 Jan 2025 13:15

Instrument :
MSVOA_V
ClientSampleId :
C0B08

Tgt Ion: 84 Resp: 1750
Ion Ratio Lower Upper
84 100
86 57.7 44.7 82.9
49 119.8 84.1 156.1

