

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
 Data File : VV038460.D
 Acq On : 20 Jan 2025 13:39
 Operator : SY/MD
 Sample : Q1125-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B10

Quant Time: Jan 21 00:52:21 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 21 00:50:24 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	191380	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	206043	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	81213	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	80059	5.073	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.400%
7) Chloroethane-d5	1.529	69	71077	5.363	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.200%
11) 1,1-Dichloroethene-d2	2.056	65	35998	5.062	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	101.200%
20) 2-Butanone-d5	3.789	46	161652	48.699	ug/L	-0.05
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.400%
24) Chloroform-d	4.239	84	155860	5.269	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.400%
26) 1,2-Dichloroethane-d4	4.937	65	75261	5.552	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.000%
32) Benzene-d6	4.953	84	291526	5.137	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.800%
36) 1,2-Dichloropropane-d6	5.982	67	93458	5.418	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.400%
41) Toluene-d8	7.236	98	229393	4.500	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.000%
43) trans-1,3-Dichloroprop...	7.558	79	28996	4.596	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.000%
46) 2-Hexanone-d5	8.021	63	103208	41.460	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.920%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	69636	5.092	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.800%
66) 1,2-Dichlorobenzene-d4	11.554	152	79024	5.749	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.000%
Target Compounds					Qvalue	
16) Methylene chloride	2.445	84	3075	0.175	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
Data File : VV038460.D
Acq On : 20 Jan 2025 13:39
Operator : SY/MD
Sample : Q1125-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COB10

Quant Time: Jan 21 00:52:21 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 21 00:50:24 2025
Response via : Initial Calibration

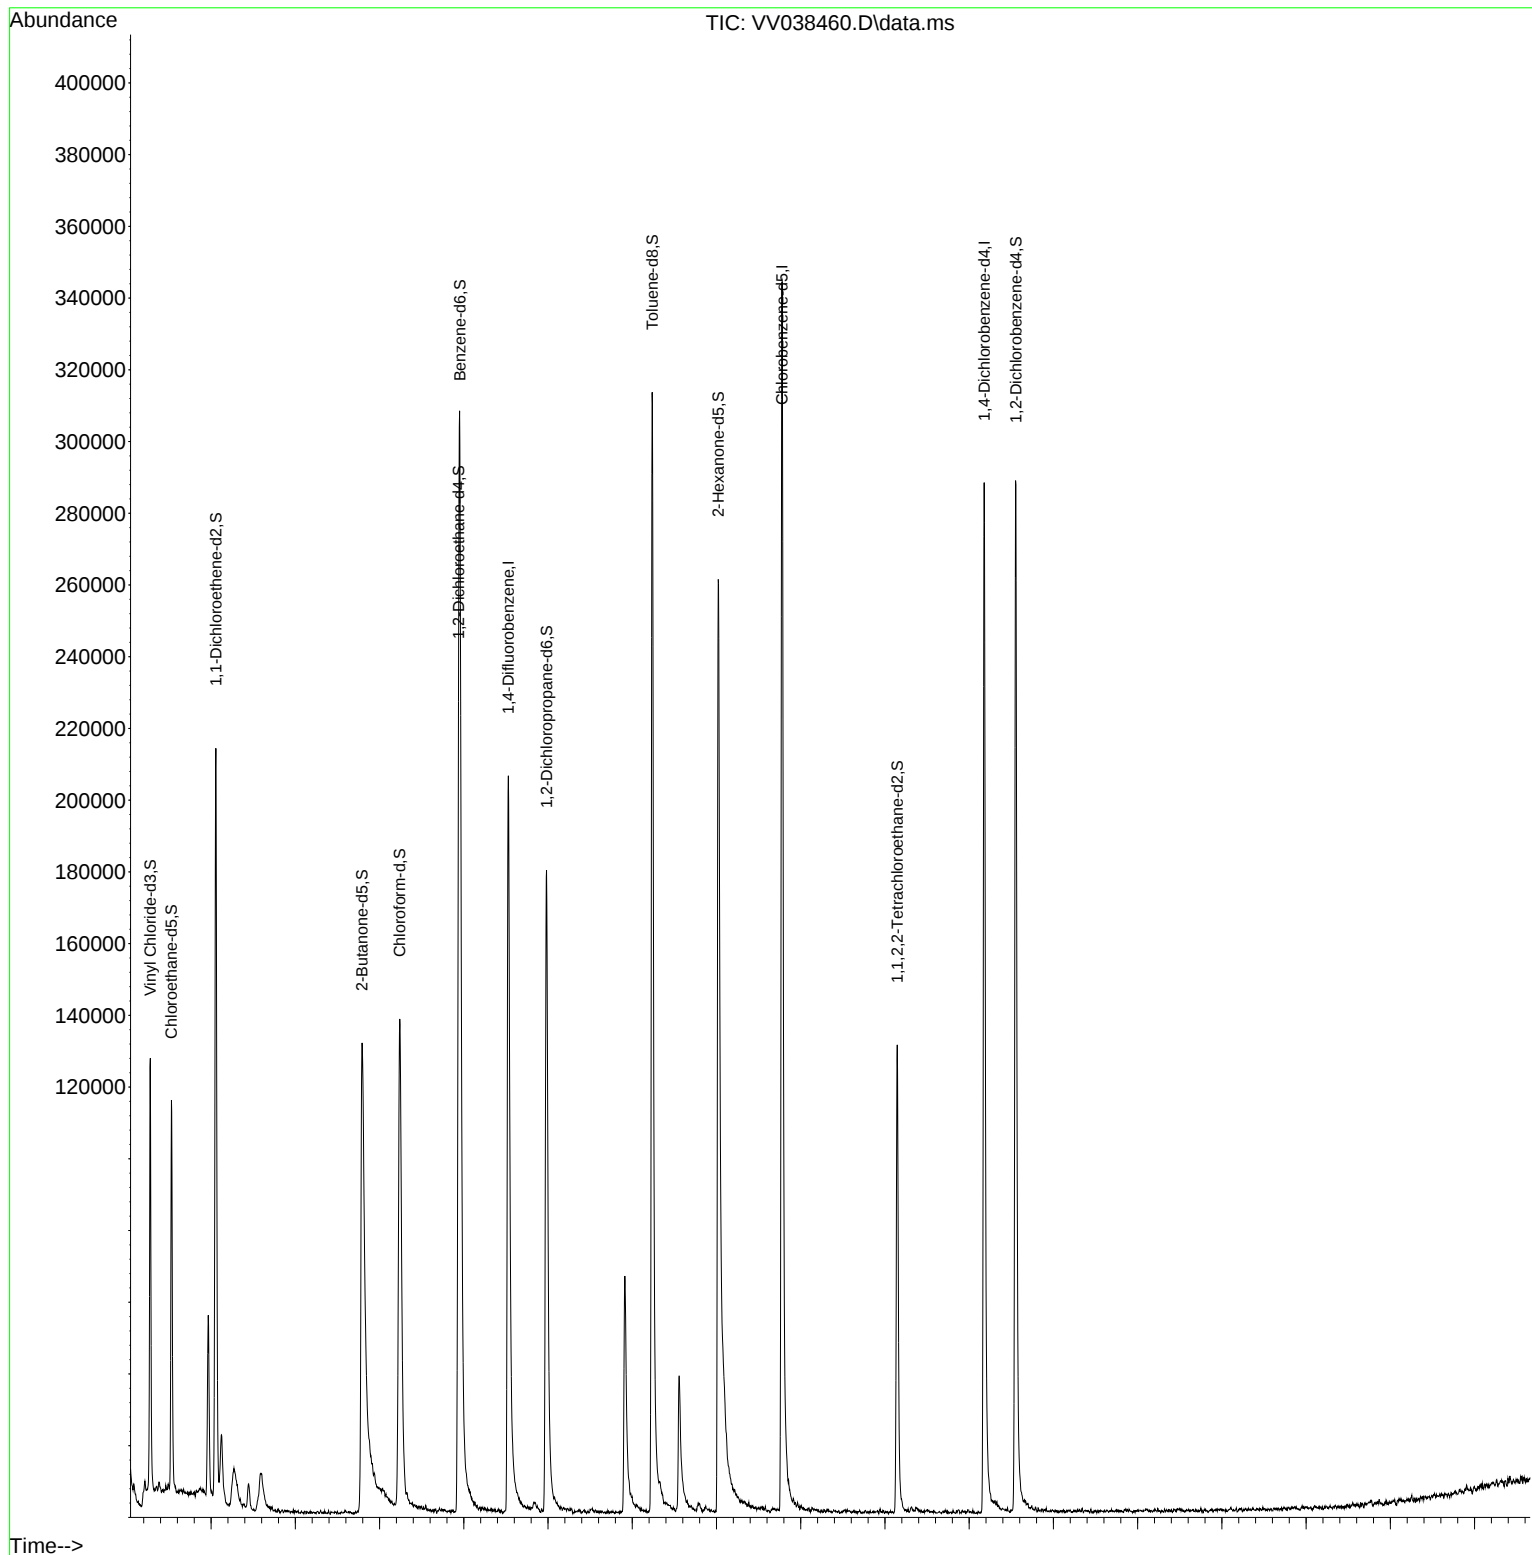

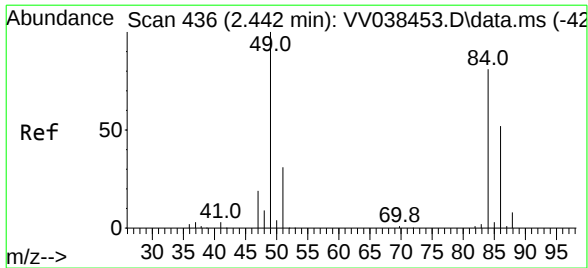

#16
 Methylene chloride
 Concen: 0.175 ug/L
 RT: 2.445 min Scan# 43
 Delta R.T. 0.003 min
 Lab File: VV038460.D
 Acq: 20 Jan 2025 13:39

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B10

Tgt Ion:	84	Resp:	3075
Ion	Ratio	Lower	Upper
84	100		
86	49.6	44.7	82.9
49	112.9	84.1	156.1

