

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
 Data File : VV038463.D
 Acq On : 20 Jan 2025 14:52
 Operator : SY/MD
 Sample : Q1125-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038463.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	35	42	52	rBV	7645	14202	2.05%	0.357%
2	1.278	68	74	88	rVB	57706	63641	9.17%	1.599%
3	1.384	102	107	113	rBV	10845	11298	1.63%	0.284%
4	1.532	144	153	162	rBV	52596	64415	9.29%	1.619%
5	1.969	281	289	298	rBV2	12462	19823	2.86%	0.498%
6	2.056	306	316	326	rBV	96527	143648	20.71%	3.610%
7	2.111	328	333	343	rVB	12965	21156	3.05%	0.532%
8	2.214	355	365	384	rBV	76477	143587	20.70%	3.608%
9	2.555	457	471	485	rBV	19044	42825	6.17%	1.076%
10	3.783	837	853	897	rBV2	210965	693723	100.00%	17.434%
11	4.243	984	996	1020	rBV2	57206	153736	22.16%	3.864%
12	4.953	1203	1217	1248	rBV3	137907	384895	55.48%	9.673%
13	5.532	1386	1397	1428	rBV2	95479	229216	33.04%	5.760%
14	5.985	1526	1538	1566	rBV2	77939	184209	26.55%	4.629%
15	6.918	1818	1828	1844	rBV3	29226	65248	9.41%	1.640%
16	7.239	1919	1928	1954	rBV	123941	249568	35.98%	6.272%
17	7.564	2019	2029	2050	rBV2	17482	43706	6.30%	1.098%
18	8.021	2162	2171	2212	rBV	193467	521998	75.25%	13.118%
19	8.783	2397	2408	2439	rBV	160765	306222	44.14%	7.696%
20	10.146	2819	2832	2854	rBV	90799	155688	22.44%	3.913%
21	11.181	3144	3154	3176	rBV	133467	242628	34.97%	6.097%
22	11.554	3258	3270	3289	rBV	124431	223725	32.25%	5.622%

Sum of corrected areas: 3979157




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
Data File : VV038463.D
Acq On : 20 Jan 2025 14:52
Operator : SY/MD
Sample : Q1125-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

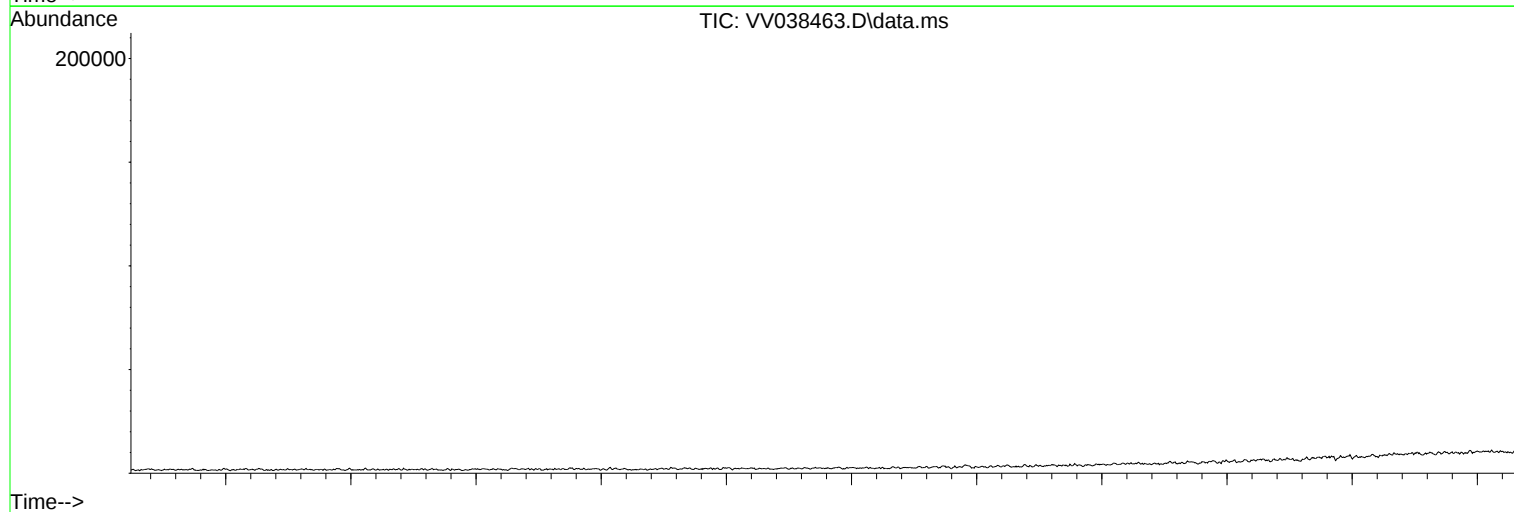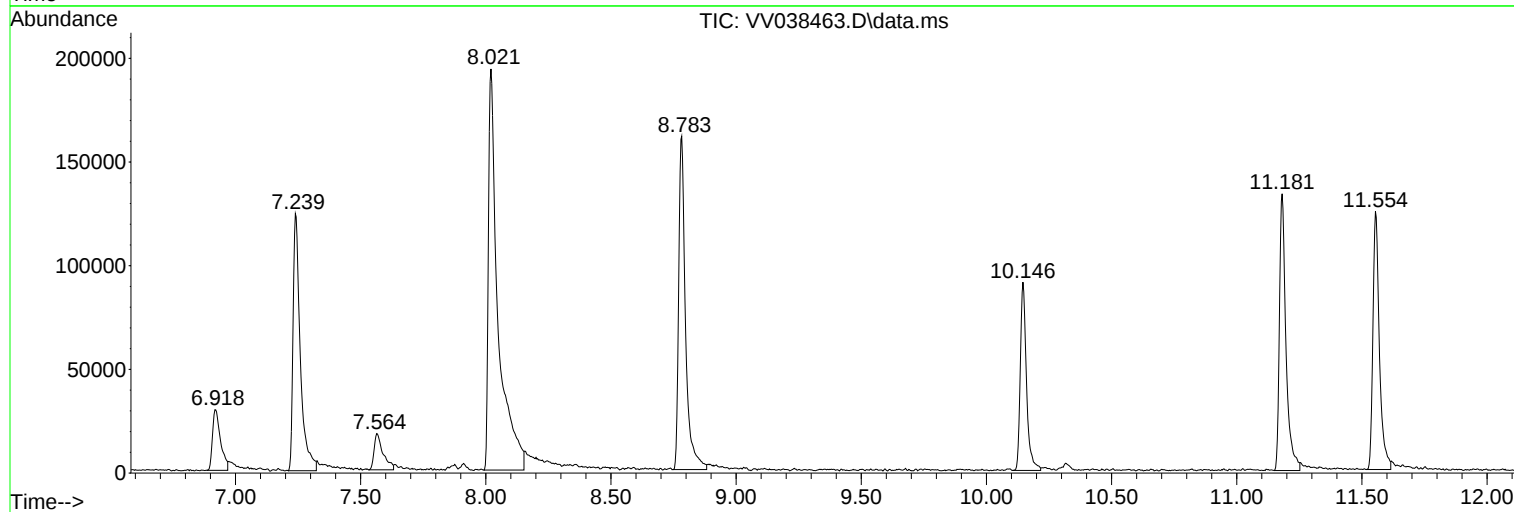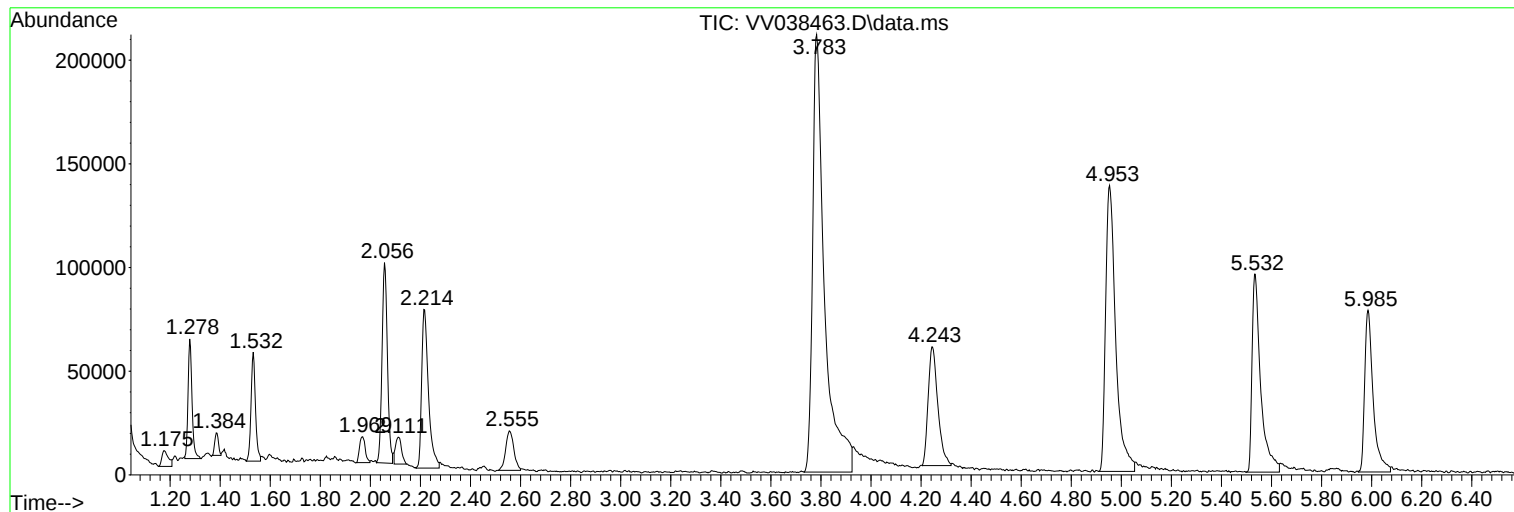

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
Data File : VV038463.D
Acq On : 20 Jan 2025 14:52
Operator : SY/MD
Sample : Q1125-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
Data File : VV038463.D
Acq On : 20 Jan 2025 14:52
Operator : SY/MD
Sample : Q1125-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
