

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
 Data File : VV038470.D
 Acq On : 20 Jan 2025 17:38
 Operator : SY/MD
 Sample : Q1125-11
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B09

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.191	40	47	64	rBV5	24393	61405	8.16%	0.885%
2	1.275	67	73	89	rVV	114722	138060	18.34%	1.989%
3	1.381	92	106	124	rVB4	19286	51871	6.89%	0.747%
4	1.532	145	153	167	rBV	100766	121056	16.08%	1.744%
5	1.963	281	287	301	rVB2	13500	21004	2.79%	0.303%
6	2.053	306	315	329	rVV	190753	291124	38.67%	4.194%
7	2.124	332	337	351	rVB3	10792	22725	3.02%	0.327%
8	2.304	372	393	398	rBV2	17242	49107	6.52%	0.708%
9	2.551	460	470	479	rBV3	6527	11981	1.59%	0.173%
10	3.802	840	859	902	rBV4	184746	717311	95.28%	10.335%
11	3.985	908	916	952	rVB2	35031	108062	14.35%	1.557%
12	4.239	978	995	1021	rBV2	128189	348709	46.32%	5.024%
13	4.950	1202	1216	1252	rBV3	283934	752813	100.00%	10.846%
14	5.529	1386	1396	1424	rBV	210521	472444	62.76%	6.807%
15	5.982	1523	1537	1563	rBV	168353	368931	49.01%	5.315%
16	6.911	1817	1826	1849	rBV2	60174	135536	18.00%	1.953%
17	7.236	1917	1927	1955	rBV	279942	535992	71.20%	7.722%
18	7.558	2018	2027	2058	rBV2	35012	83513	11.09%	1.203%
19	7.905	2126	2135	2146	rBV4	14287	26632	3.54%	0.384%
20	8.024	2162	2172	2215	rBV	287914	744774	98.93%	10.730%
21	8.776	2397	2406	2438	rBV	359825	650457	86.40%	9.371%
22	10.146	2818	2832	2853	rBV	135885	232526	30.89%	3.350%
23	11.178	3143	3153	3177	rBV	312518	525295	69.78%	7.568%
24	11.554	3259	3270	3294	rBV	275094	469473	62.36%	6.764%




Sum of corrected areas: 6940801

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
Data File : VV038470.D
Acq On : 20 Jan 2025 17:38
Operator : SY/MD
Sample : Q1125-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

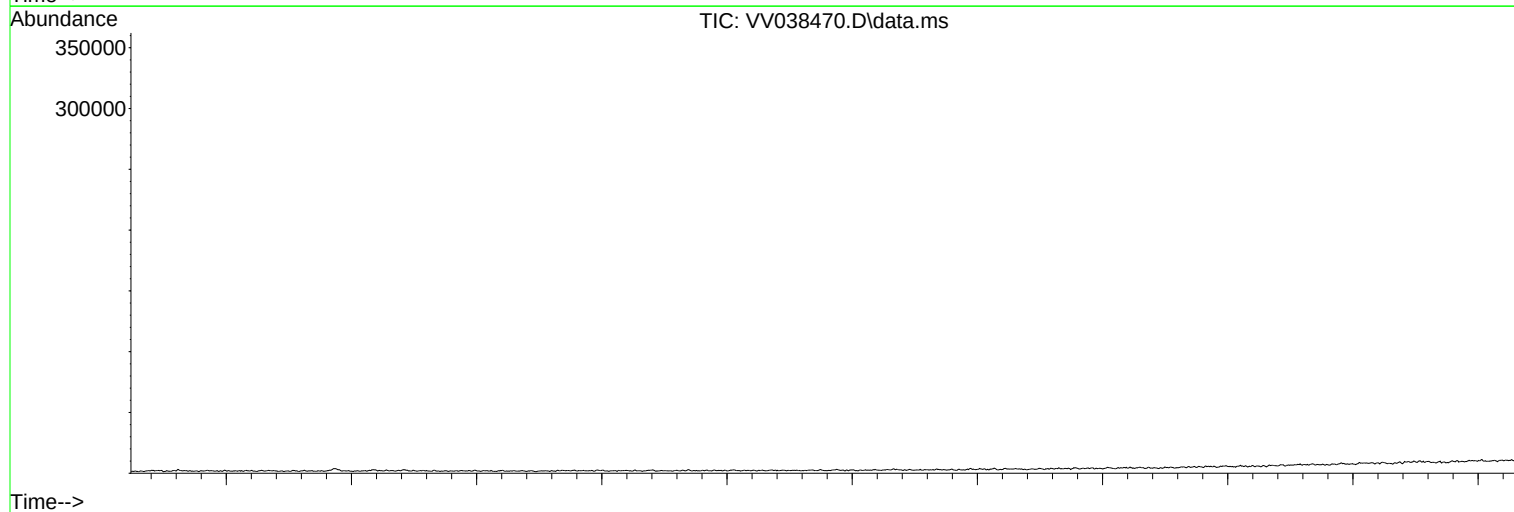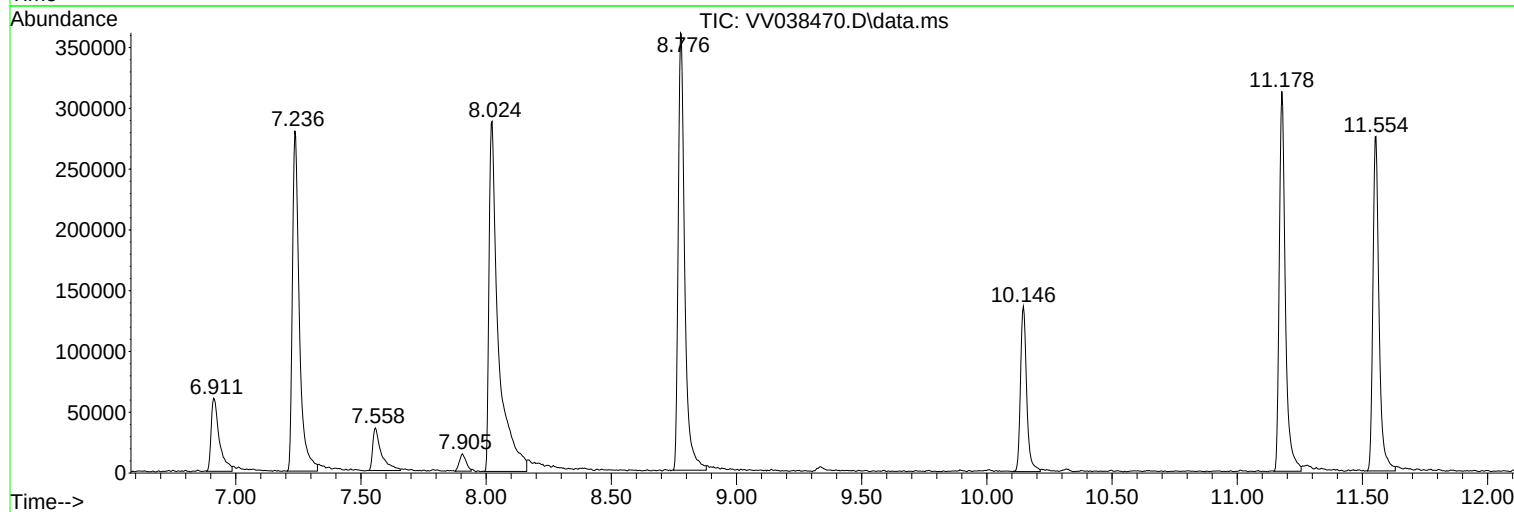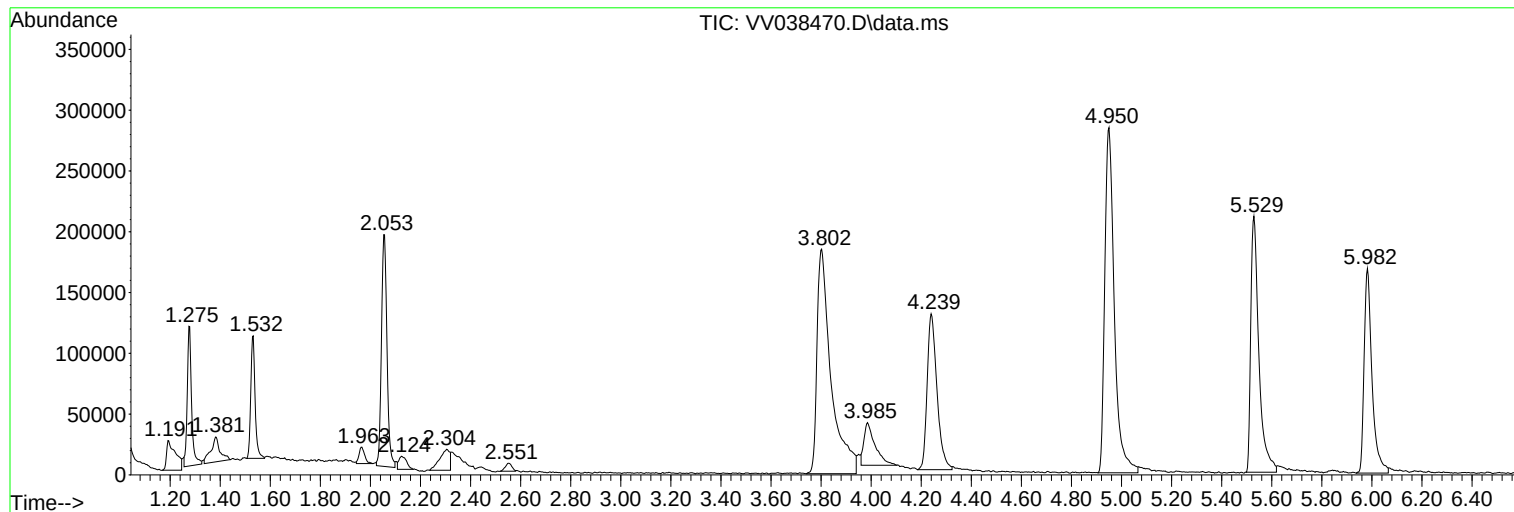

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
Data File : VV038470.D
Acq On : 20 Jan 2025 17:38
Operator : SY/MD
Sample : Q1125-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Quant Title : TRACE VOA SFAM1.0










TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

Peak Number 4 Ethyl Acetate Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.985	1.14 ug/L	108062	1,4-Difluorobenzene	5.529

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Ethyl Acetate	88	C4H8O2	000141-78-6	86
2	Ethyl Acetate	88	C4H8O2	000141-78-6	86
3	Ethyl Acetate	88	C4H8O2	000141-78-6	78
4	Ethyl Acetate	88	C4H8O2	000141-78-6	78
5	CH3C(O)CH2CH2OH	88	C4H8O2	000590-90-9	53

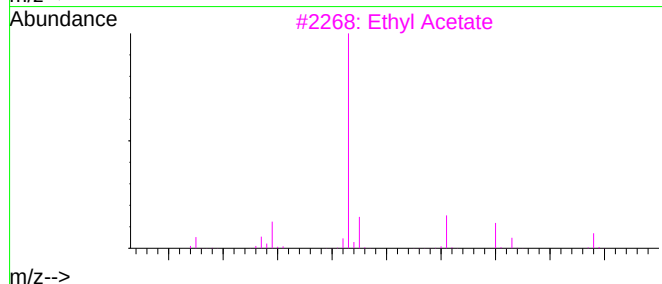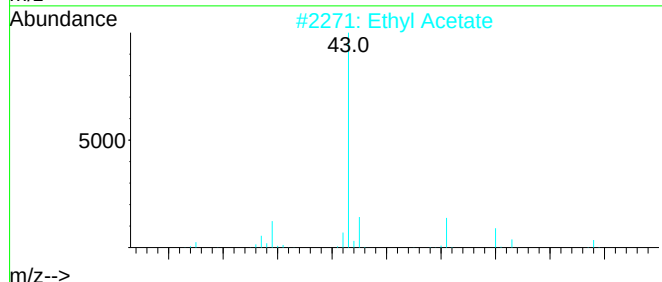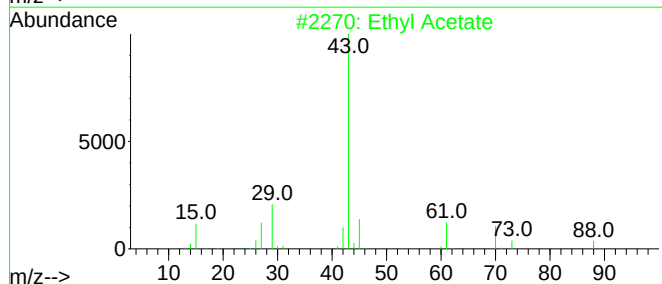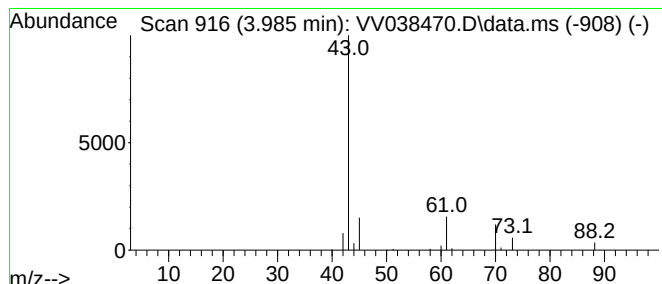

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
Data File : VV038470.D
Acq On : 20 Jan 2025 17:38
Operator : SY/MD
Sample : Q1125-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethyl Acetate	3.985	1.1	ug/L	108062	1	5.529	472444	5.0