
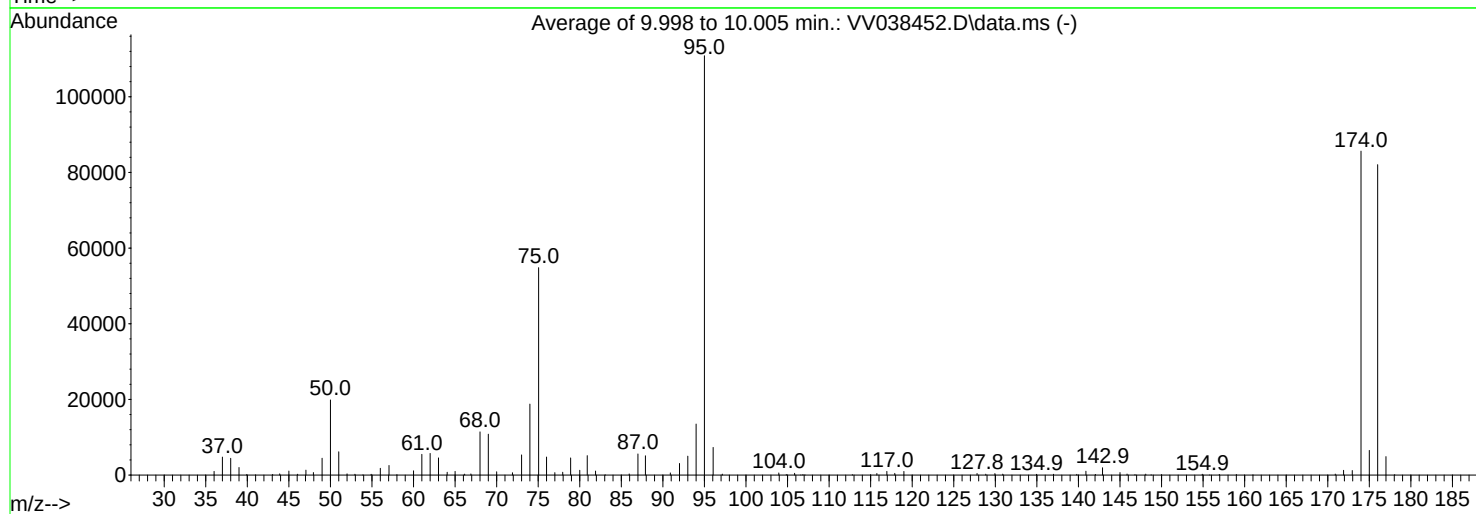


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012025\
Data File : VV038452.D
Acq On : 20 Jan 2025 09:30
Operator : SY/MD
Sample : BFB299
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB299

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jan 21 00:50:24 2025

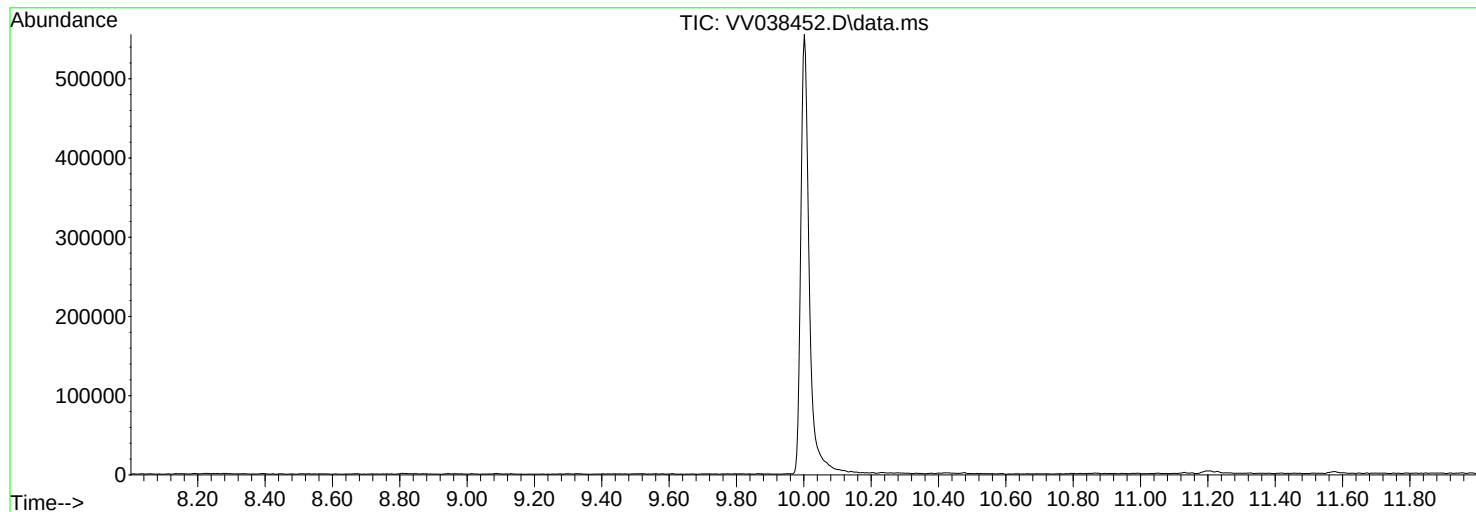

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2774

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	19856	PASS
75	95	30	80	49.5	54835	PASS
95	95	100	100	100.0	110856	PASS
96	95	5	9	6.6	7309	PASS
173	174	0.00	2	1.4	1205	PASS
174	95	50	120	77.2	85635	PASS
175	174	5	9	7.6	6527	PASS
176	174	95	105	95.8	82056	PASS
177	176	5	10	6.0	4889	PASS

m/z	Abundance
40.00	526.0
41.70	102.0
43.80	547.0
49.20	119.0
54.90	147.0
245.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB299

m/z	Abundance
36.00	962.0
37.00	5047.0
38.00	4383.0
39.00	2101.0
39.90	659.0
43.10	160.0
44.00	925.0
45.00	1061.0
46.10	228.0
47.00	1213.0
48.00	628.0
49.00	4554.0
50.00	19392.0
51.00	6457.0
52.00	255.0
53.10	221.0
54.90	373.0
56.00	1819.0
57.10	2502.0
60.00	1084.0
61.00	5308.0
62.00	5783.0
63.00	4632.0
64.00	703.0
65.00	915.0
66.20	225.0
66.90	328.0
68.00	11019.0
69.00	10764.0
70.00	819.0
71.90	704.0
73.00	5277.0
74.00	18656.0
75.00	54824.0
76.00	4475.0
76.90	622.0
77.90	746.0
78.90	4355.0
80.00	1171.0
80.90	5058.0
81.90	1020.0
85.90	330.0
87.00	5374.0
87.90	5239.0
90.90	502.0
92.00	3038.0
93.00	4907.0
94.00	13524.0
95.00	110624.0
96.10	7265.0
97.20	220.0
104.00	453.0
104.80	162.0
105.80	496.0
106.90	169.0
112.80	108.0
115.00	117.0
115.80	381.0
116.90	889.0
117.90	498.0
119.00	867.0
127.80	397.0
128.90	250.0
130.00	454.0
130.90	195.0
134.90	216.0
137.00	211.0
139.80	201.0
140.90	1010.0
142.10	152.0
142.90	1905.0
145.00	632.0
145.80	290.0
146.80	132.0
148.10	284.0
148.70	113.0
150.00	165.0
154.90	243.0
157.00	197.0
159.00	149.0
161.00	124.0
170.90	293.0
171.90	1144.0
172.90	1095.0
174.00	82152.0
175.00	6205.0
176.00	78688.0
177.00	4722.0

Instrument :
MSVOA_V
ClientSampleId :
BFB299

m/z	Abundance
36.00	1018.0
37.00	4834.0
38.00	4551.0
39.00	2064.0
39.90	641.0
43.00	164.0
44.00	889.0
45.00	1124.0
46.10	227.0
47.10	1334.0
48.00	693.0
49.00	4695.0
50.00	20328.0
51.00	6279.0
52.00	329.0
52.90	241.0
54.90	401.0
56.00	1859.0
57.00	2617.0
58.00	130.0
60.00	1155.0
61.00	5652.0
62.00	5943.0
63.00	4746.0
64.00	768.0
65.00	998.0
66.10	273.0
66.90	309.0
68.00	11703.0
69.00	11059.0
70.00	909.0
71.90	646.0
73.00	5492.0
74.00	19304.0
75.00	56280.0
76.00	4956.0
77.00	641.0
78.00	788.0
78.90	4734.0
80.00	1305.0
80.90	5411.0
81.90	1084.0
85.90	314.0
87.00	5817.0
87.90	5229.0
90.90	595.0
92.00	3150.0
93.00	5168.0
94.00	13888.0
95.00	114240.0
96.10	7525.0
97.10	272.0
104.00	568.0
104.80	132.0
105.90	472.0
106.70	131.0
107.00	131.0
112.80	120.0
115.00	108.0
115.80	426.0
116.90	991.0
117.90	476.0
119.00	1025.0
127.80	448.0
128.90	259.0
130.00	414.0
130.90	278.0
135.00	217.0
137.00	232.0
139.80	207.0
140.90	1043.0
142.10	177.0
142.90	2050.0
145.00	684.0
145.90	295.0
146.80	129.0
148.10	267.0
148.80	122.0
150.00	149.0
154.90	246.0
156.90	148.0
159.00	137.0
170.90	274.0
171.90	1276.0
173.00	1244.0
174.00	88984.0
175.00	6754.0
176.00	85200.0
177.00	5071.0
178.10	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB299

m/z	Abundance
36.00	959.0
37.00	4421.0
38.00	4369.0
39.00	1849.0
39.90	576.0
41.00	117.0
43.00	156.0
44.00	806.0
45.00	1012.0
46.00	227.0
47.10	1369.0
47.80	691.0
49.00	4452.0
50.00	19848.0
51.00	5731.0
52.00	392.0
52.90	226.0
53.90	110.0
54.90	325.0
56.00	1706.0
57.00	2494.0
58.00	149.0
60.00	1140.0
61.00	5485.0
62.00	5466.0
63.00	4246.0
64.10	765.0
65.00	1026.0
66.10	250.0
66.90	296.0
68.00	11558.0
69.00	10635.0
70.00	911.0
71.90	514.0
73.00	5226.0
74.00	18352.0
75.10	53400.0
76.00	4904.0
77.10	685.0
78.00	705.0
78.90	4494.0
80.00	1330.0
80.90	4961.0
81.90	1113.0
83.10	120.0
86.00	279.0
87.00	5583.0
87.90	4847.0
90.90	607.0
92.00	3038.0
93.00	4934.0
94.00	13040.0
95.00	107704.0
96.00	7138.0
97.10	260.0
103.90	654.0
104.90	124.0
105.90	447.0
106.60	116.0
107.10	120.0
112.80	125.0
115.70	456.0
117.00	1049.0
117.90	384.0
119.00	1010.0
127.80	411.0
128.80	205.0
129.90	370.0
130.90	302.0
135.00	197.0
137.00	211.0
139.80	177.0
140.90	1020.0
142.00	167.0
142.90	1865.0
145.00	697.0
145.90	257.0
146.80	128.0
148.10	205.0
154.90	206.0
155.80	130.0
156.90	159.0
159.00	135.0
170.90	249.0
171.90	1368.0
173.00	1277.0
174.00	85768.0
175.00	6623.0
176.00	82280.0
177.00	4874.0
178.00	190.0

Instrument :
MSVOA_V
ClientSampleId :
BFB299