

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV012120\
 Data File : VV014364.D
 Acq On : 21 Jan 2020 10:13
 Operator : SY/MD
 Sample : VV0121WBL01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK53

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.229	38	43	49	rVB2	36323	31578	1.06%	0.136%
2	1.319	63	71	83	rVB	388248	396883	13.32%	1.712%
3	1.586	146	154	167	rVB	295046	340626	11.43%	1.470%
4	2.129	314	323	337	rVB	490166	694139	23.30%	2.995%
5	2.537	442	450	459	rBV	37843	58071	1.95%	0.251%
6	3.958	878	892	937	rBV	250898	1115313	37.43%	4.812%
7	4.399	1009	1029	1054	rBV	499467	1236075	41.49%	5.333%
8	5.093	1225	1245	1276	rBV2	1144911	2791142	93.68%	12.042%
9	5.659	1409	1421	1444	rBV	931155	1856569	62.31%	8.010%
10	6.116	1549	1563	1580	rBV	652789	1329205	44.61%	5.735%
11	7.026	1836	1846	1863	rBV	351389	640172	21.49%	2.762%
12	7.357	1936	1949	1967	rBV	1290775	2238755	75.14%	9.659%
13	7.662	2033	2044	2061	rBV	221482	375695	12.61%	1.621%
14	8.135	2177	2191	2218	rBV	1548201	2979365	100.00%	12.854%
15	8.891	2413	2426	2447	rBV	1350001	2218606	74.47%	9.572%
16	10.254	2839	2850	2862	rBV	469113	732761	24.59%	3.161%
17	10.415	2888	2900	2908	rBV6	18956	39056	1.31%	0.168%
18	11.289	3159	3172	3186	rBV	1384758	2126311	71.37%	9.173%
19	11.666	3275	3289	3303	rBV	1227513	1912932	64.21%	8.253%
20	12.289	3470	3483	3496	rBV	33369	65809	2.21%	0.284%


Sum of corrected areas: 23179063

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV012120\
Data File : VV014364.D
Acq On : 21 Jan 2020 10:13
Operator : SY/MD
Sample : VV0121WBL01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK53

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

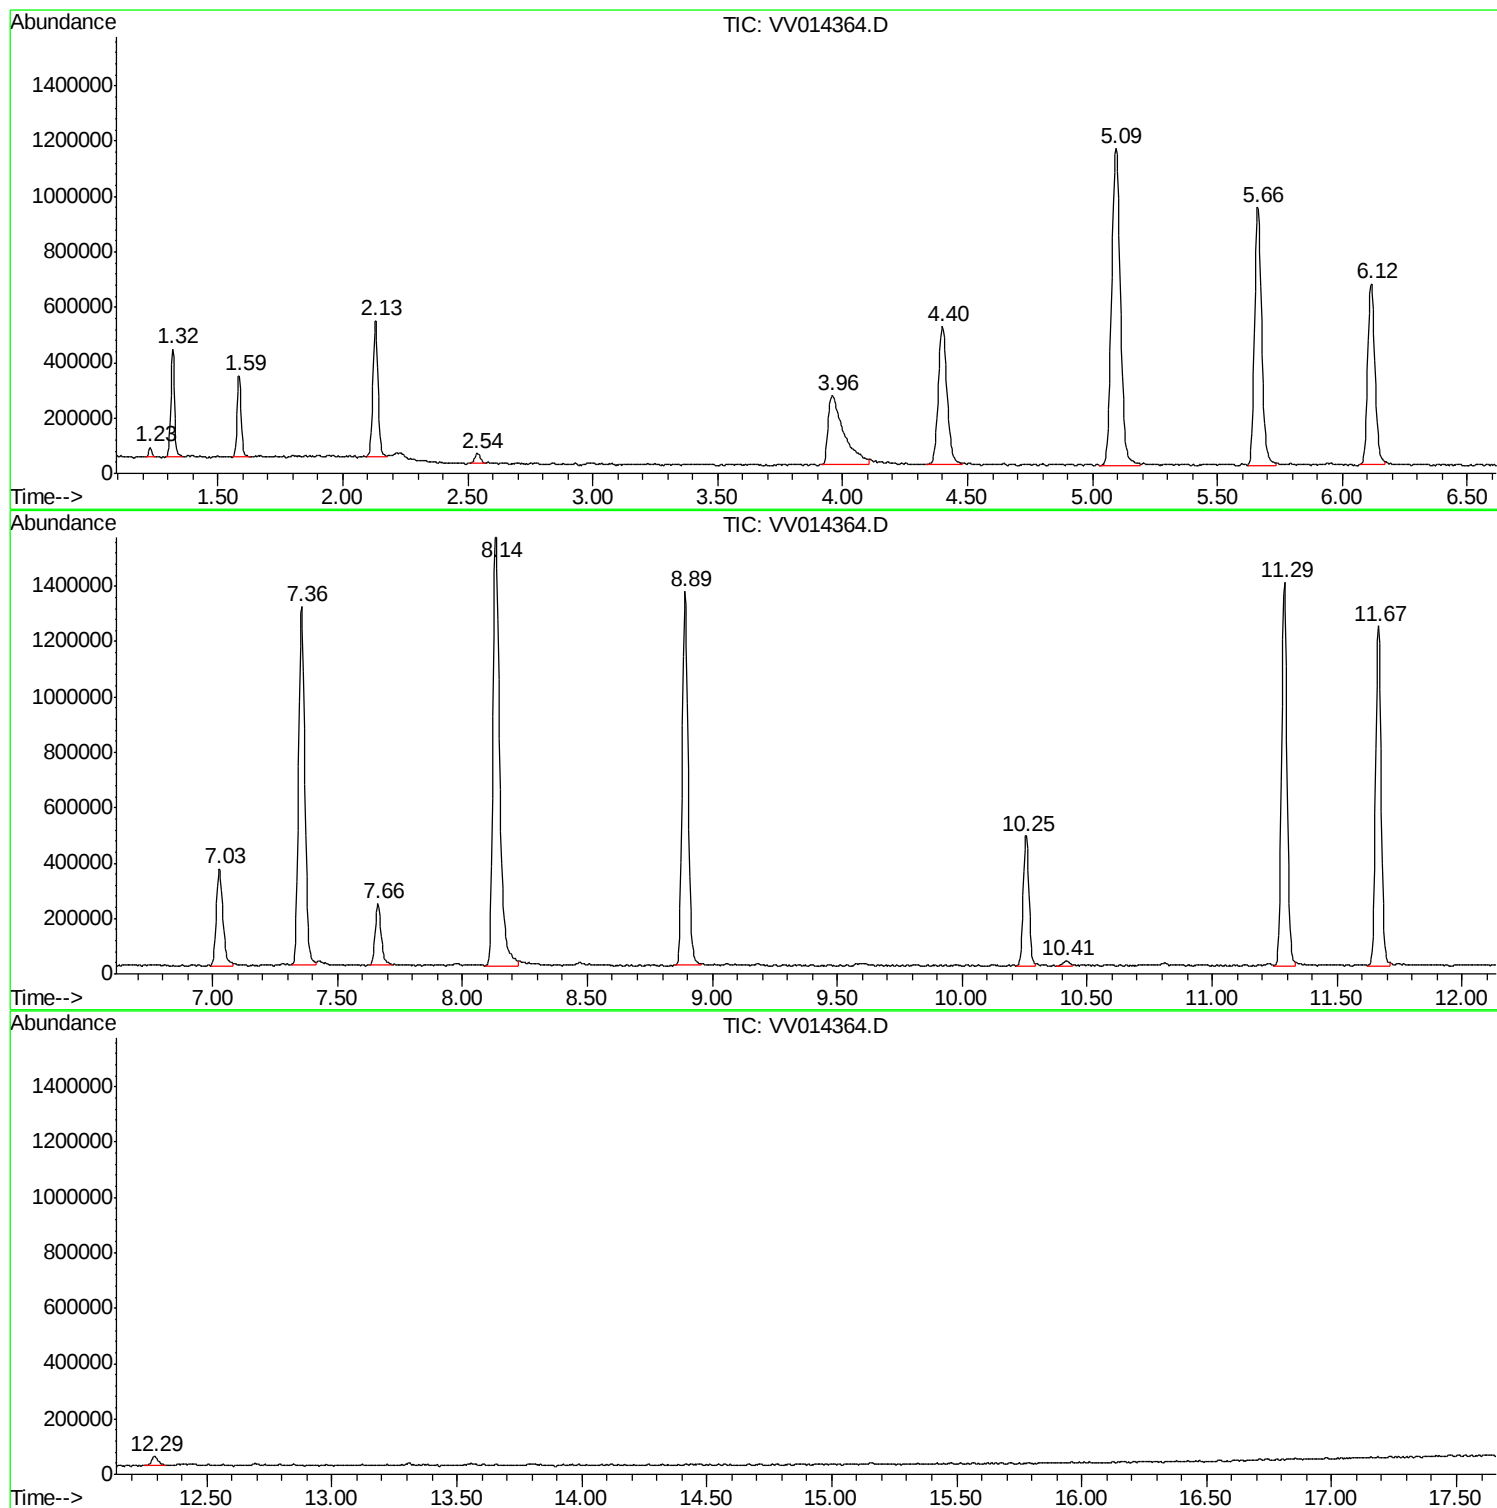

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV012120\
Data File : VV014364.D
Acq On : 21 Jan 2020 10:13
Operator : SY/MD
Sample : VV0121WBL01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK53










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.03	1.72 ug/L	640172	1,4-Difluorobenzene	5.66

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Thiatricyclo[3.1.1.0(2,4)]heptane	112	C6H8S	1000221-37-0	37
2		Thiophosgene	114	CCl2S	000463-71-8	28
3		Methane, oxvbis[chloro-	114	C2H4Cl2O	000542-88-1	23
4		2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	23
5		2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	9

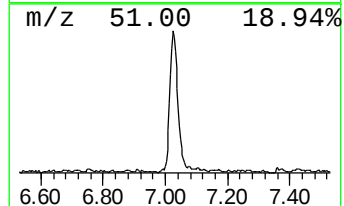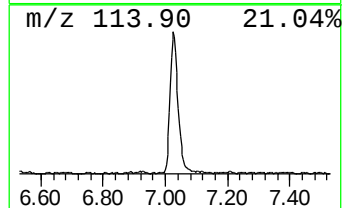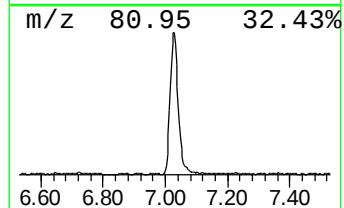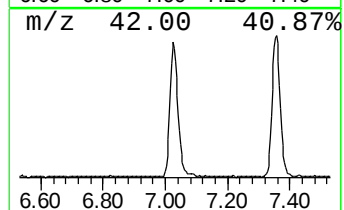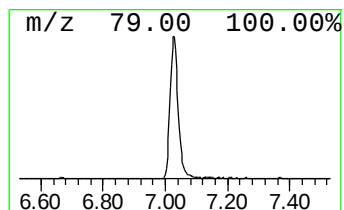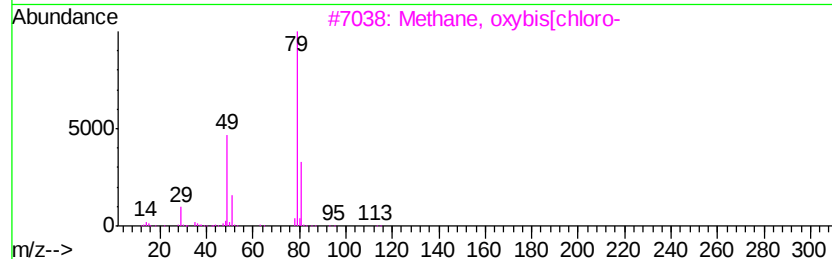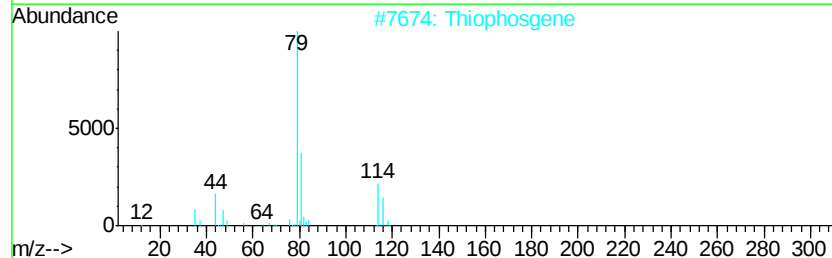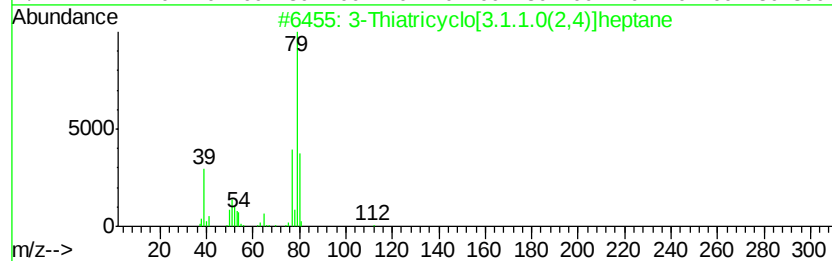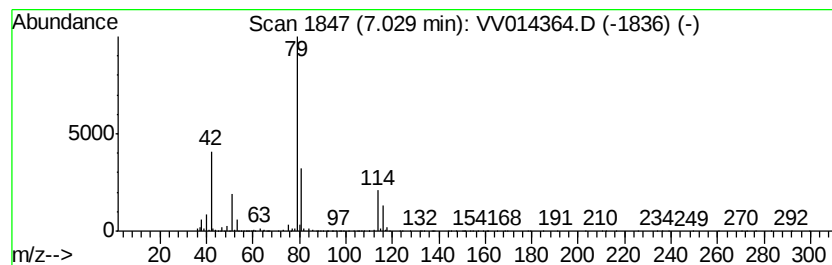

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV012120\
Data File : VV014364.D
Acq On : 21 Jan 2020 10:13
Operator : SY/MD
Sample : VV0121WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK53

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.03	1.7	ug/L	640172	1	5.66	1856570	5.0