

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020109.D
 Acq On : 21 Jan 2021 15:20
 Operator : SY/MD
 Sample : VV0121MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK85

Quant Time: Jan 22 06:44:05 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 22 06:43:18 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.621	114	438981	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.859	117	495902	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.257	152	211066	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.306	65	171649	52.72	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	105.44%
7) Chloroethane-d5	1.570	69	144622	53.07	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	106.14%
11) 1,1-Dichloroethene-d2	2.110	63	252446	38.82	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.64%
21) 2-Butanone-d5	3.891	46	204973	91.80	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.80%
24) Chloroform-d	4.354	84	287731	47.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.36%
26) 1,2-Dichloroethane-d4	5.036	65	210427	49.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.56%
32) Benzene-d6	5.055	84	558353	40.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.78%
36) 1,2-Dichloropropane-d6	6.074	67	186330	43.22	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.44%
41) Toluene-d8	7.318	98	526606	41.45	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.90%
43) trans-1,3-Dichloroprop...	7.627	79	92144	43.68	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.36%
47) 2-Hexanone-d5	8.093	63	119643	66.76	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	66.76%
57) 1,1,2,2-Tetrachloroeth...	10.222	84	209254	35.46	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	70.92%
64) 1,2-Dichlorobenzene-d4	11.633	152	230099	58.02	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	116.04%
Target Compounds						
48) 2-Hexanone	8.151	43	13011	2.88	ug/L	Qvalue # 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020109.D
Acq On : 21 Jan 2021 15:20
Operator : SY/MD
Sample : VV0121MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK85


Quant Time: Jan 22 06:44:05 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 22 06:43:18 2021
Response via : Initial Calibration

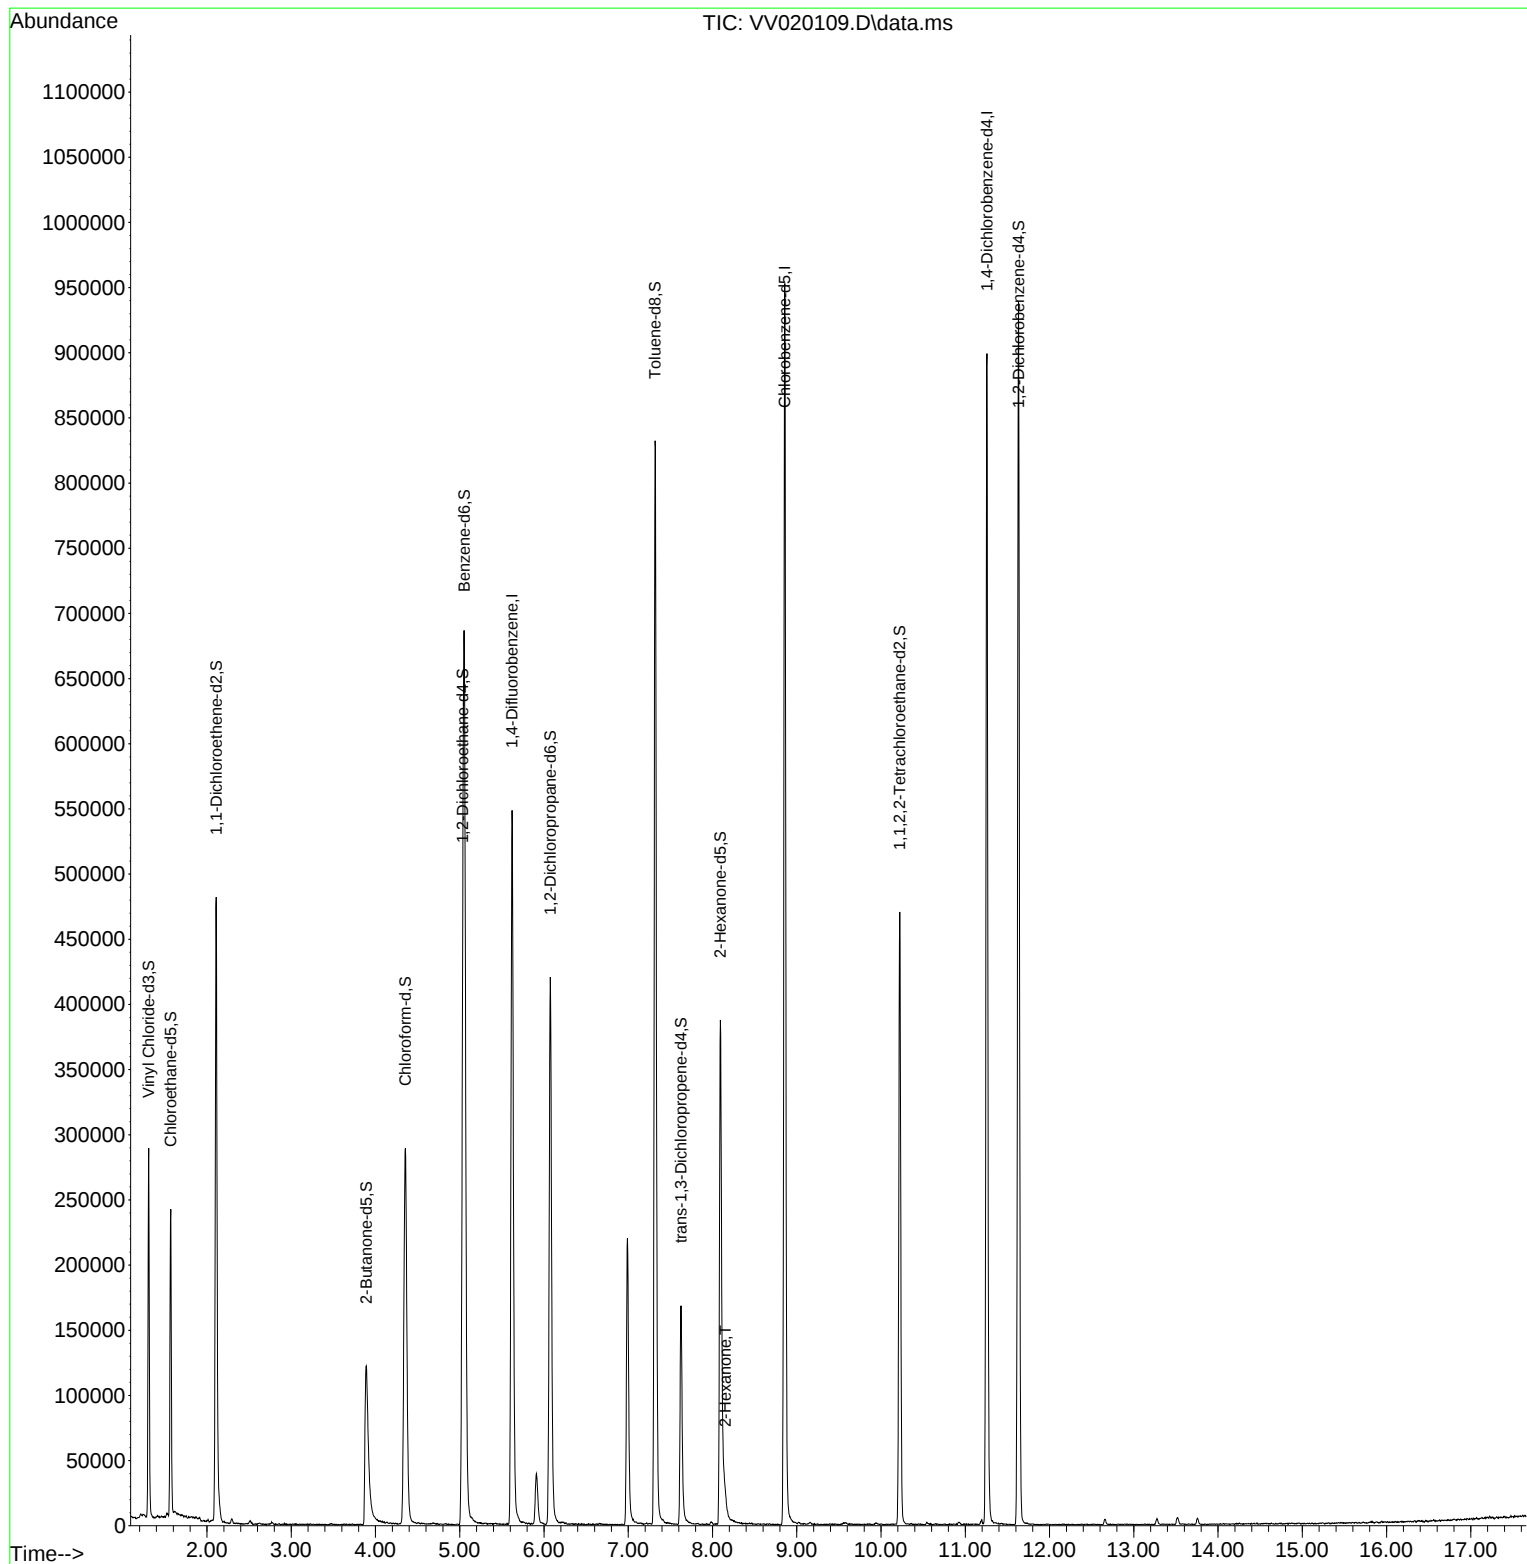

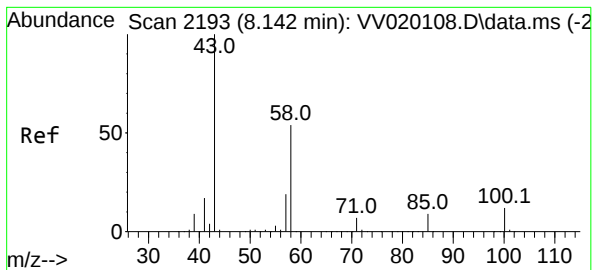

#48
 2-Hexanone
 Concen: 2.88 ug/L
 RT: 8.151 min Scan# 2196
 Delta R.T. 0.010 min
 Lab File: VV020109.D
 Acq: 21 Jan 2021 15:20

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK85

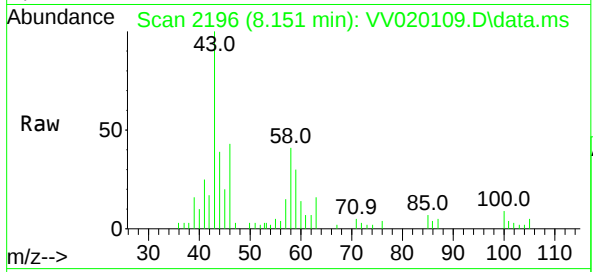

Tgt Ion: 43	Resp: 13011
Ion Ratio	Lower Upper
43	100
58	39.4 41.8 62.6#
57	5.5 15.0 22.4#
100	1.4 8.9 13.3#

