

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020110.D
 Acq On : 21 Jan 2021 15:43
 Operator : SY/MD
 Sample : VV0121WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020110.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	84	rVB	267287	262572	15.43%	1.971%
2	1.570	142	149	162	rBV	218175	244380	14.36%	1.835%
3	2.110	307	317	349	rVB	448921	694039	40.78%	5.211%
4	2.351	391	392	395	rBV2	389	265	0.02%	0.002%
5	2.512	436	442	447	rBV6	2063	2901	0.17%	0.022%
6	2.563	454	458	463	rBV4	669	775	0.05%	0.006%
7	2.602	467	470	471	rBV2	818	454	0.03%	0.003%
8	2.698	496	500	501	rBV2	499	339	0.02%	0.003%
9	2.962	580	582	585	rBV3	768	415	0.02%	0.003%
10	3.039	604	606	610	rVB3	678	402	0.02%	0.003%
11	3.065	610	614	618	rBV3	562	466	0.03%	0.003%
12	3.090	618	622	623	rVB2	434	245	0.01%	0.002%
13	3.103	623	626	630	rBV4	592	511	0.03%	0.004%
14	3.225	661	664	667	rBV3	285	255	0.01%	0.002%
15	3.338	696	699	701	rBV	383	300	0.02%	0.002%
16	3.351	701	703	706	rVV3	582	308	0.02%	0.002%
17	3.373	707	710	712	rVV3	542	292	0.02%	0.002%
18	3.389	712	715	717	rVB2	651	299	0.02%	0.002%
19	3.422	717	725	727	rBV4	383	443	0.03%	0.003%
20	3.434	727	729	731	rVB3	548	258	0.02%	0.002%
21	3.512	749	753	757	rBV2	377	342	0.02%	0.003%
22	3.557	765	767	772	rBV3	521	289	0.02%	0.002%
23	3.653	794	797	800	rBV3	385	242	0.01%	0.002%
24	3.679	800	805	806	rVV4	419	343	0.02%	0.003%
25	3.769	830	833	836	rBV2	430	304	0.02%	0.002%
26	3.897	862	873	910	rBV	119264	391451	23.00%	2.939%
27	4.354	999	1015	1040	rBV	284944	694539	40.81%	5.214%
28	4.672	1111	1114	1117	rBV4	682	629	0.04%	0.005%
29	4.991	1209	1213	1214	rBV2	720	411	0.02%	0.003%
30	5.052	1215	1232	1257	rVV2	662452	1702081	100.00%	12.778%
31	5.409	1341	1343	1347	rBV4	690	448	0.03%	0.003%
32	5.556	1385	1389	1391	rBV4	513	393	0.02%	0.003%
33	5.576	1392	1395	1396	rBV3	621	280	0.02%	0.002%
34	5.621	1397	1409	1441	rVV	478592	951522	55.90%	7.144%
35	5.910	1487	1499	1515	rBV4	35996	76478	4.49%	0.574%
36	6.074	1536	1550	1583	rBV	382968	788775	46.34%	5.922%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020110.D
 Acq On : 21 Jan 2021 15:43
 Operator : SY/MD
 Sample : VV0121WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	6.421	1654	1658	1660	rBV5	492	443	0.03%	0.003%
38	6.528	1687	1691	1694	rVV	682	417	0.02%	0.003%
39	6.592	1709	1711	1713	rBV3	460	250	0.01%	0.002%
40	6.698	1742	1744	1745	rBV2	723	304	0.02%	0.002%
41	6.730	1752	1754	1757	rBV4	577	258	0.02%	0.002%
42	6.791	1771	1773	1777	rVB2	984	530	0.03%	0.004%
43	6.827	1780	1784	1787	rBV2	974	693	0.04%	0.005%
44	6.991	1823	1835	1861	rBV	208726	383127	22.51%	2.876%
45	7.187	1894	1896	1898	rBV3	744	415	0.02%	0.003%
46	7.322	1925	1938	1956	rBV	758650	1303747	76.60%	9.788%
47	7.624	2022	2032	2050	rBV	146873	260513	15.31%	1.956%
48	7.939	2128	2130	2136	rVB4	609	513	0.03%	0.004%
49	7.971	2136	2140	2141	rBV4	1460	874	0.05%	0.007%
50	8.007	2150	2151	2156	rVB2	1033	572	0.03%	0.004%
51	8.093	2167	2178	2214	rBV2	433687	877043	51.53%	6.584%
52	8.453	2288	2290	2293	rVB3	1105	412	0.02%	0.003%
53	8.473	2293	2296	2299	rBV4	825	639	0.04%	0.005%
54	8.569	2324	2326	2328	rVB3	675	255	0.01%	0.002%
55	8.585	2328	2331	2333	rVB2	608	350	0.02%	0.003%
56	8.601	2333	2336	2339	rBV4	584	489	0.03%	0.004%
57	8.727	2370	2375	2380	rBV5	628	698	0.04%	0.005%
58	8.855	2404	2415	2444	rBV	754465	1232193	72.39%	9.251%
59	9.148	2503	2506	2509	rBV3	1323	883	0.05%	0.007%
60	9.257	2536	2540	2544	rBV2	932	973	0.06%	0.007%
61	9.402	2582	2585	2587	rBV2	502	308	0.02%	0.002%
62	9.453	2597	2601	2602	rBV2	711	407	0.02%	0.003%
63	9.463	2602	2604	2607	rBV2	725	338	0.02%	0.003%
64	9.482	2607	2610	2613	rBV2	817	565	0.03%	0.004%
65	9.537	2624	2627	2628	rBV2	665	332	0.02%	0.002%
66	9.547	2628	2630	2632	rVV2	738	257	0.02%	0.002%
67	9.563	2632	2635	2638	rBV4	961	721	0.04%	0.005%
68	9.762	2692	2697	2702	rBV4	713	833	0.05%	0.006%
69	9.913	2741	2744	2746	rVB2	533	278	0.02%	0.002%
70	9.936	2747	2751	2754	rBV4	1615	1237	0.07%	0.009%
71	10.045	2781	2785	2788	rBV2	515	445	0.03%	0.003%
72	10.068	2789	2792	2794	rVV2	466	299	0.02%	0.002%
73	10.084	2794	2797	2798	rVV2	534	346	0.02%	0.003%
74	10.145	2812	2816	2818	rBV3	654	481	0.03%	0.004%
75	10.222	2827	2840	2866	rBV	505099	795772	46.75%	5.974%
76	10.357	2877	2882	2885	rBV3	765	621	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020110.D
 Acq On : 21 Jan 2021 15:43
 Operator : SY/MD
 Sample : VV0121WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

77	10.373	2885	2887	2890	rVB3	819	394	0.02%	0.003%
78	10.389	2890	2892	2893	rBV	706	254	0.01%	0.002%
79	10.431	2901	2905	2907	rBV2	678	455	0.03%	0.003%
80	10.553	2936	2943	2948	rBV7	1680	2084	0.12%	0.016%
81	10.678	2980	2982	2986	rVB	673	316	0.02%	0.002%
82	10.704	2986	2990	2991	rBV	539	433	0.03%	0.003%
83	10.904	3050	3052	3053	rBV	614	250	0.01%	0.002%
84	10.990	3076	3079	3084	rVB2	597	557	0.03%	0.004%
85	11.042	3091	3095	3096	rBV2	506	375	0.02%	0.003%
86	11.122	3117	3120	3123	rBV2	469	367	0.02%	0.003%
87	11.199	3132	3144	3149	rBV9	2433	3678	0.22%	0.028%
88	11.254	3150	3161	3186	rBV	816761	1289756	75.78%	9.683%
89	11.521	3242	3244	3249	rVB2	564	417	0.02%	0.003%
90	11.630	3260	3278	3295	rBV	828171	1323390	77.75%	9.935%
91	11.932	3369	3372	3374	rBV2	537	391	0.02%	0.003%
92	11.961	3378	3381	3385	rVV3	407	425	0.02%	0.003%
93	12.302	3482	3487	3492	rBV3	450	573	0.03%	0.004%
94	12.325	3492	3494	3496	rBV	532	295	0.02%	0.002%
95	12.514	3548	3553	3554	rBV3	372	301	0.02%	0.002%
96	12.656	3592	3597	3605	rVB8	3095	4153	0.24%	0.031%
97	12.691	3605	3608	3614	rVB2	413	324	0.02%	0.002%
98	12.733	3617	3621	3624	rVV4	453	385	0.02%	0.003%
99	13.518	3860	3865	3866	rBV2	1934	1586	0.09%	0.012%
100	14.016	4016	4020	4021	rBV2	580	450	0.03%	0.003%


Sum of corrected areas: 13319886

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020110.D
Acq On : 21 Jan 2021 15:43
Operator : SY/MD
Sample : VV0121WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

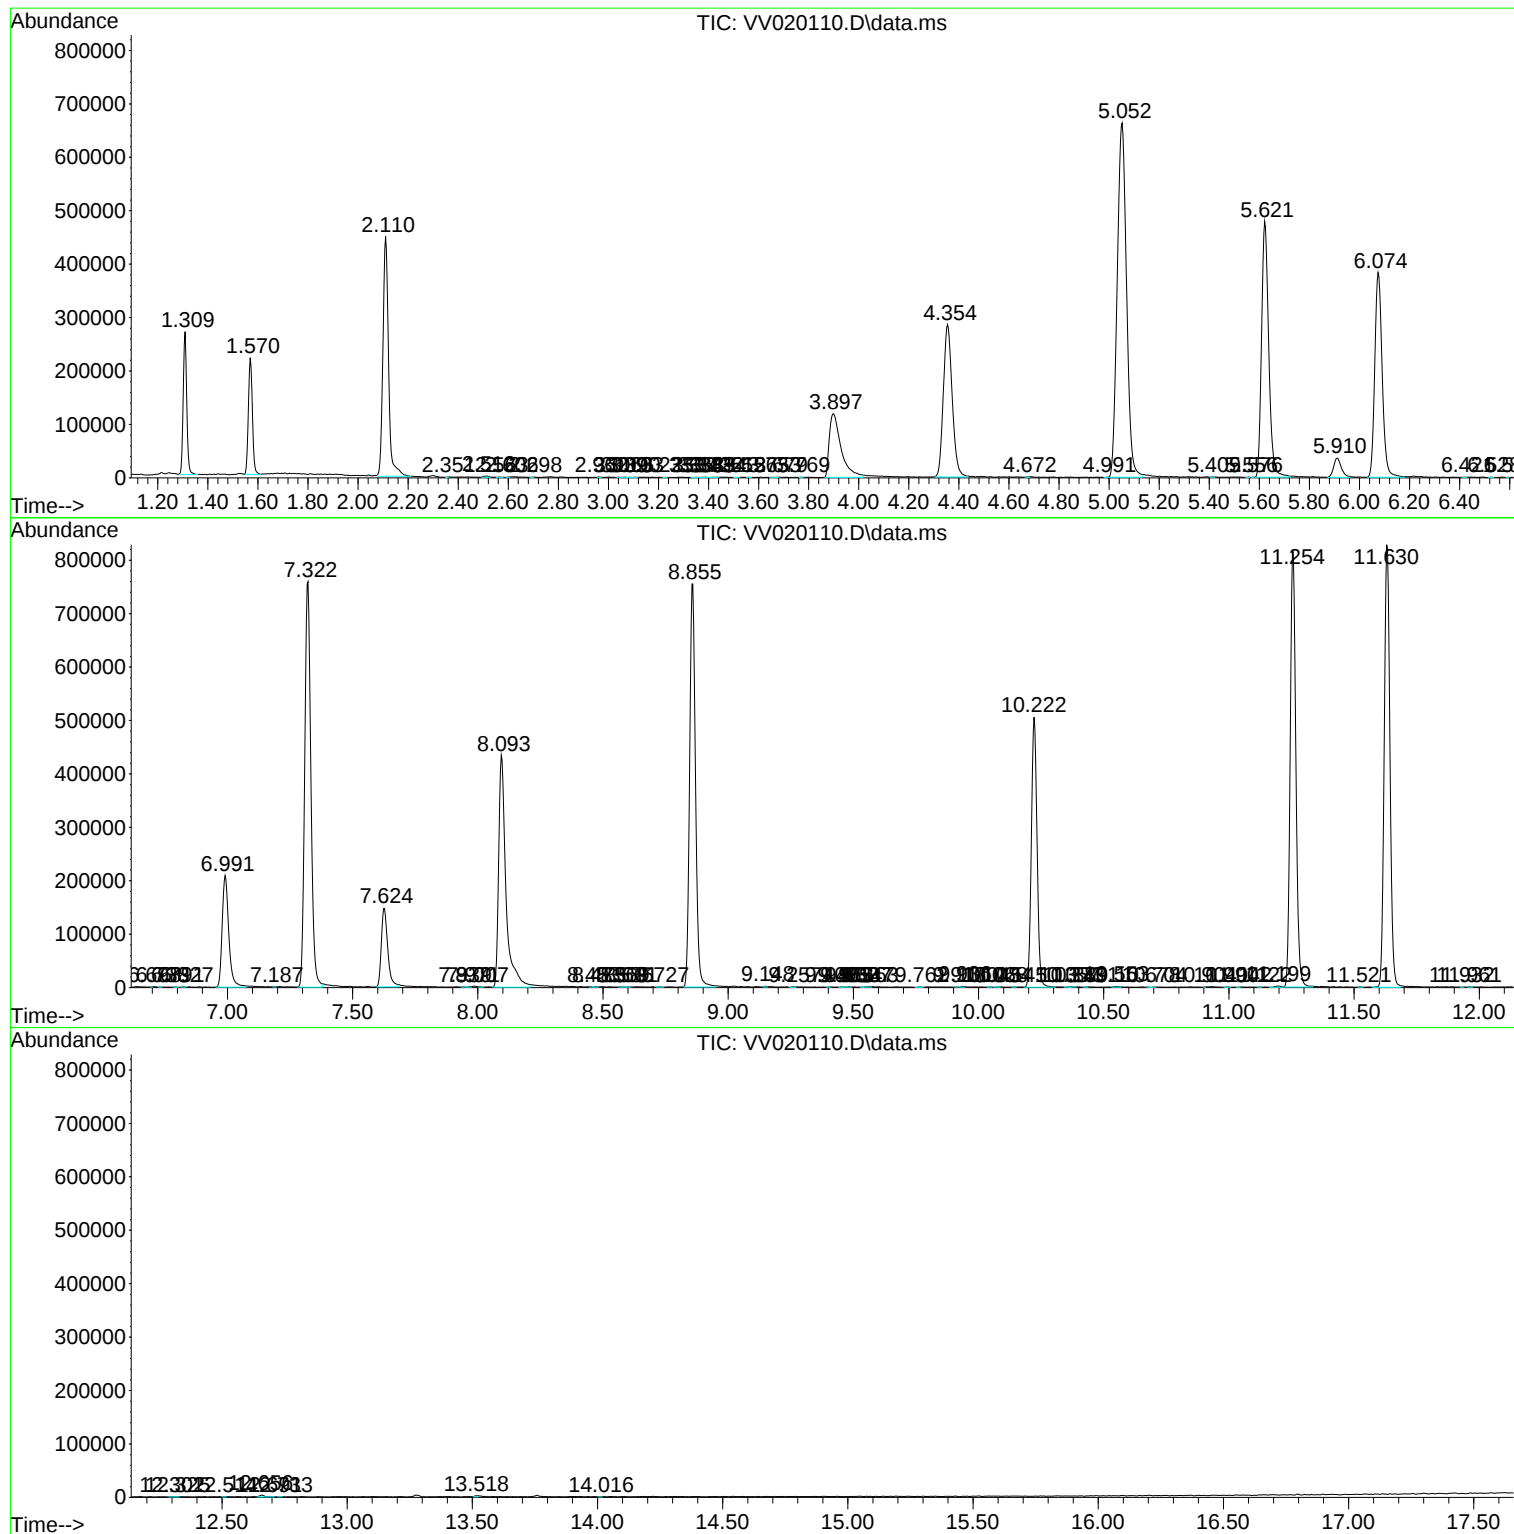

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020110.D
Acq On : 21 Jan 2021 15:43
Operator : SY/MD
Sample : VV0121WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020110.D
Acq On : 21 Jan 2021 15:43
Operator : SY/MD
Sample : VV0121WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
