

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020111.D
 Acq On : 21 Jan 2021 16:07
 Operator : SY/MD
 Sample : M1181-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020111.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	86	rVB2	307456	331789	20.19%	2.304%
2	1.569	143	149	158	rVB	209674	231286	14.08%	1.606%
3	2.110	308	317	345	rVB	430404	654217	39.82%	4.542%
4	2.547	450	453	455	rBV3	803	440	0.03%	0.003%
5	2.772	512	523	542	rVB3	39530	81997	4.99%	0.569%
6	2.933	572	573	575	rBV2	426	175	0.01%	0.001%
7	2.962	580	582	585	rBV	620	352	0.02%	0.002%
8	3.003	592	595	596	rBV2	587	237	0.01%	0.002%
9	3.036	602	605	607	rVB2	811	447	0.03%	0.003%
10	3.061	607	613	617	rBV4	963	822	0.05%	0.006%
11	3.100	622	625	627	rBV2	541	407	0.02%	0.003%
12	3.190	651	653	655	rBV	473	299	0.02%	0.002%
13	3.219	659	662	664	rBV2	829	486	0.03%	0.003%
14	3.286	678	683	684	rBV2	571	410	0.02%	0.003%
15	3.319	691	693	694	rBV2	376	168	0.01%	0.001%
16	3.515	751	754	758	rBV4	404	357	0.02%	0.002%
17	3.576	769	773	774	rBV2	279	200	0.01%	0.001%
18	3.640	791	793	795	rVB2	493	183	0.01%	0.001%
19	3.656	795	798	804	rBV6	445	566	0.03%	0.004%
20	3.785	834	838	842	rBV2	673	511	0.03%	0.004%
21	3.810	844	846	849	rBV2	357	245	0.01%	0.002%
22	3.836	852	854	856	rBV3	765	356	0.02%	0.002%
23	3.913	860	878	904	rBV3	288499	915321	55.71%	6.355%
24	4.212	970	971	974	rBV3	1037	556	0.03%	0.004%
25	4.354	1000	1015	1037	rBV	269102	651671	39.66%	4.524%
26	4.782	1146	1148	1151	rBV3	709	527	0.03%	0.004%
27	4.823	1159	1161	1165	rVB2	885	494	0.03%	0.003%
28	5.052	1213	1232	1269	rBV2	619437	1643130	100.00%	11.408%
29	5.396	1337	1339	1340	rBV2	471	176	0.01%	0.001%
30	5.466	1358	1361	1362	rBV	430	223	0.01%	0.002%
31	5.499	1367	1371	1376	rBV7	1185	1179	0.07%	0.008%
32	5.621	1395	1409	1436	rBV	527931	1055074	64.21%	7.325%
33	5.917	1490	1501	1526	rVB8	25290	64728	3.94%	0.449%
34	6.074	1536	1550	1583	rBV	379169	770722	46.91%	5.351%
35	6.299	1617	1620	1623	rBV4	945	793	0.05%	0.006%
36	6.425	1654	1659	1663	rVB3	870	714	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012121\
 Data File : VW020111.D
 Acq On : 21 Jan 2021 16:07
 Operator : SY/MD
 Sample : M1181-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	6.508	1683	1685	1689	rVB3	453	322	0.02%	0.002%
38	6.537	1689	1694	1697	rBV2	396	343	0.02%	0.002%
39	6.569	1700	1704	1709	rVB3	640	599	0.04%	0.004%
40	6.595	1709	1712	1714	rBV2	593	413	0.03%	0.003%
41	6.736	1752	1756	1758	rBV3	641	446	0.03%	0.003%
42	6.756	1760	1762	1764	rBV2	503	222	0.01%	0.002%
43	6.814	1776	1780	1782	rBV2	292	262	0.02%	0.002%
44	6.843	1786	1789	1790	rBV2	456	239	0.01%	0.002%
45	6.868	1794	1797	1801	rBV4	367	337	0.02%	0.002%
46	6.894	1801	1805	1809	rBV2	489	394	0.02%	0.003%
47	6.990	1823	1835	1869	rBV	219141	405737	24.69%	2.817%
48	7.322	1925	1938	1959	rBV	820202	1426805	86.83%	9.906%
49	7.627	2022	2033	2056	rBV	146227	262706	15.99%	1.824%
50	7.891	2112	2115	2117	rBV3	641	450	0.03%	0.003%
51	7.984	2136	2144	2154	rVB6	5888	9787	0.60%	0.068%
52	8.093	2167	2178	2214	rBV2	402829	801138	48.76%	5.562%
53	8.579	2326	2329	2330	rBV2	581	329	0.02%	0.002%
54	8.640	2345	2348	2351	rBV2	643	478	0.03%	0.003%
55	8.695	2362	2365	2367	rBV2	536	268	0.02%	0.002%
56	8.711	2368	2370	2374	rVV2	604	413	0.03%	0.003%
57	8.801	2396	2398	2402	rBV3	351	274	0.02%	0.002%
58	8.859	2402	2416	2442	rBV	895594	1470960	89.52%	10.212%
59	9.051	2475	2476	2479	rVB3	554	189	0.01%	0.001%
60	9.071	2479	2482	2485	rBV2	462	395	0.02%	0.003%
61	9.116	2494	2496	2499	rBV2	623	386	0.02%	0.003%
62	9.238	2532	2534	2536	rBV2	472	209	0.01%	0.001%
63	9.354	2567	2570	2576	rBV3	520	397	0.02%	0.003%
64	9.434	2593	2595	2596	rBV2	416	224	0.01%	0.002%
65	9.772	2693	2700	2702	rBV3	537	556	0.03%	0.004%
66	9.817	2712	2714	2715	rBV2	434	172	0.01%	0.001%
67	9.826	2715	2717	2720	rVV3	568	336	0.02%	0.002%
68	9.887	2735	2736	2741	rBV3	318	188	0.01%	0.001%
69	9.936	2748	2751	2757	rBV4	1285	1307	0.08%	0.009%
70	10.048	2782	2786	2787	rBV2	471	267	0.02%	0.002%
71	10.071	2791	2793	2795	rVV2	522	291	0.02%	0.002%
72	10.090	2795	2799	2805	rVB4	524	563	0.03%	0.004%
73	10.170	2820	2824	2826	rVB3	409	247	0.02%	0.002%
74	10.222	2826	2840	2859	rBV	517599	813992	49.54%	5.651%
75	10.334	2873	2875	2878	rVB2	547	310	0.02%	0.002%
76	10.460	2909	2914	2915	rBV2	544	429	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020111.D
 Acq On : 21 Jan 2021 16:07
 Operator : SY/MD
 Sample : M1181-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

77	10.643	2965	2971	2972	rBV	675	437	0.03%	0.003%
78	10.752	3003	3005	3013	rVB5	472	298	0.02%	0.002%
79	10.836	3028	3031	3033	rBV2	316	211	0.01%	0.001%
80	10.862	3036	3039	3041	rBV3	790	470	0.03%	0.003%
81	10.923	3053	3058	3066	rBV5	2333	2512	0.15%	0.017%
82	11.026	3087	3090	3091	rBV	413	209	0.01%	0.001%
83	11.035	3091	3093	3097	rVB3	463	327	0.02%	0.002%
84	11.090	3108	3110	3116	rVB4	828	441	0.03%	0.003%
85	11.145	3124	3127	3131	rBV4	315	327	0.02%	0.002%
86	11.199	3137	3144	3149	rVB7	2120	2805	0.17%	0.019%
87	11.254	3149	3161	3183	rBV	927956	1438117	87.52%	9.984%
88	11.495	3234	3236	3242	rVB2	513	375	0.02%	0.003%
89	11.630	3265	3278	3296	rBV	832665	1332406	81.09%	9.251%
90	11.855	3346	3348	3353	rVV4	439	249	0.02%	0.002%
91	11.952	3374	3378	3383	rBV4	406	440	0.03%	0.003%
92	12.257	3469	3473	3477	rBV3	1636	1549	0.09%	0.011%
93	12.366	3502	3507	3511	rBV4	794	992	0.06%	0.007%
94	12.408	3516	3520	3525	rBV5	864	725	0.04%	0.005%
95	12.473	3537	3540	3543	rBV2	726	490	0.03%	0.003%
96	13.273	3784	3789	3790	rBV3	2464	1965	0.12%	0.014%
97	13.579	3882	3884	3887	rBV3	504	308	0.02%	0.002%
98	13.630	3897	3900	3901	rBV	514	290	0.02%	0.002%
99	13.759	3933	3940	3944	rBV3	1793	2240	0.14%	0.016%
100	14.498	4167	4170	4174	rBV4	835	756	0.05%	0.005%




Sum of corrected areas: 14403577

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020111.D
Acq On : 21 Jan 2021 16:07
Operator : SY/MD
Sample : M1181-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F1E28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

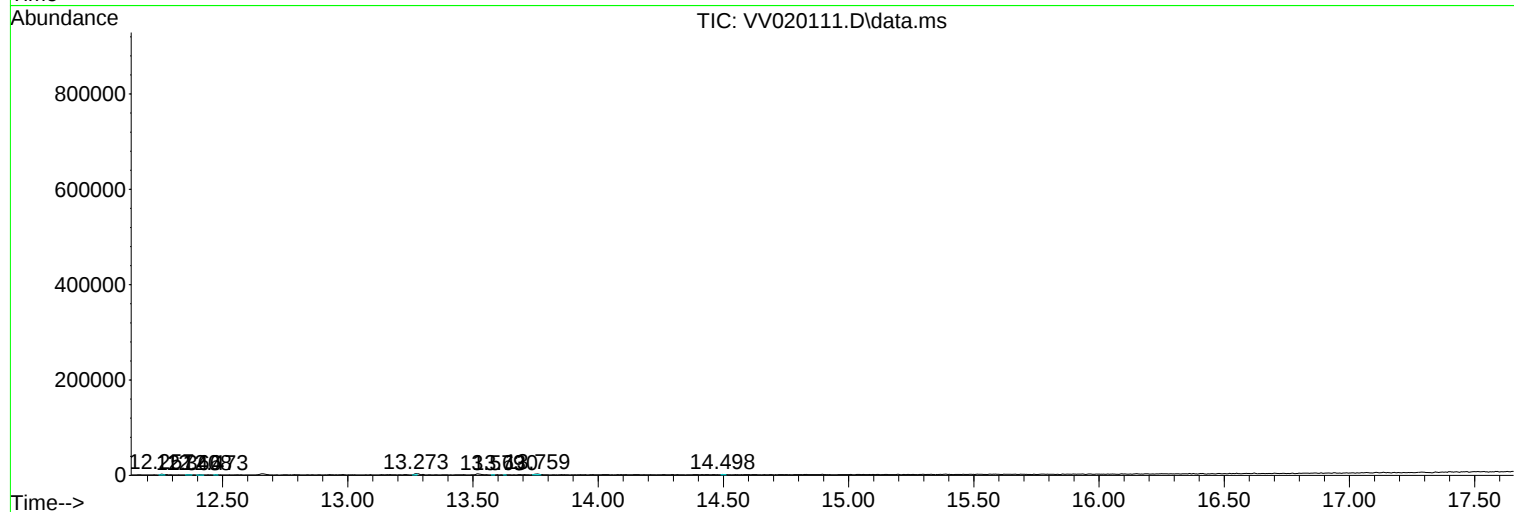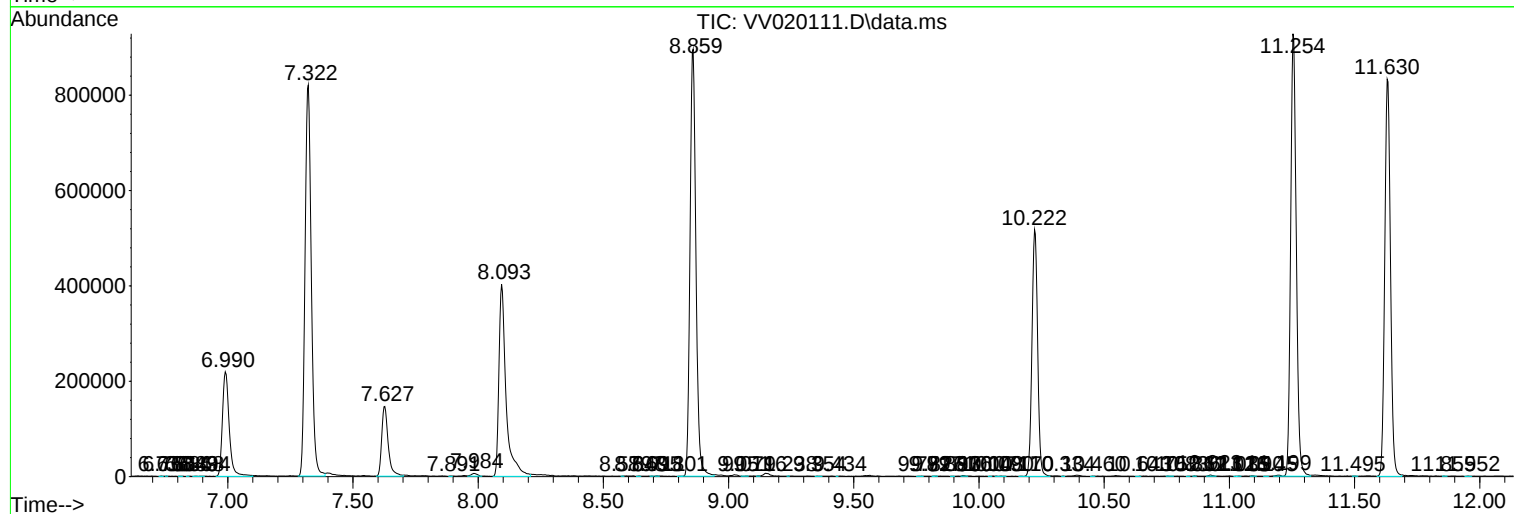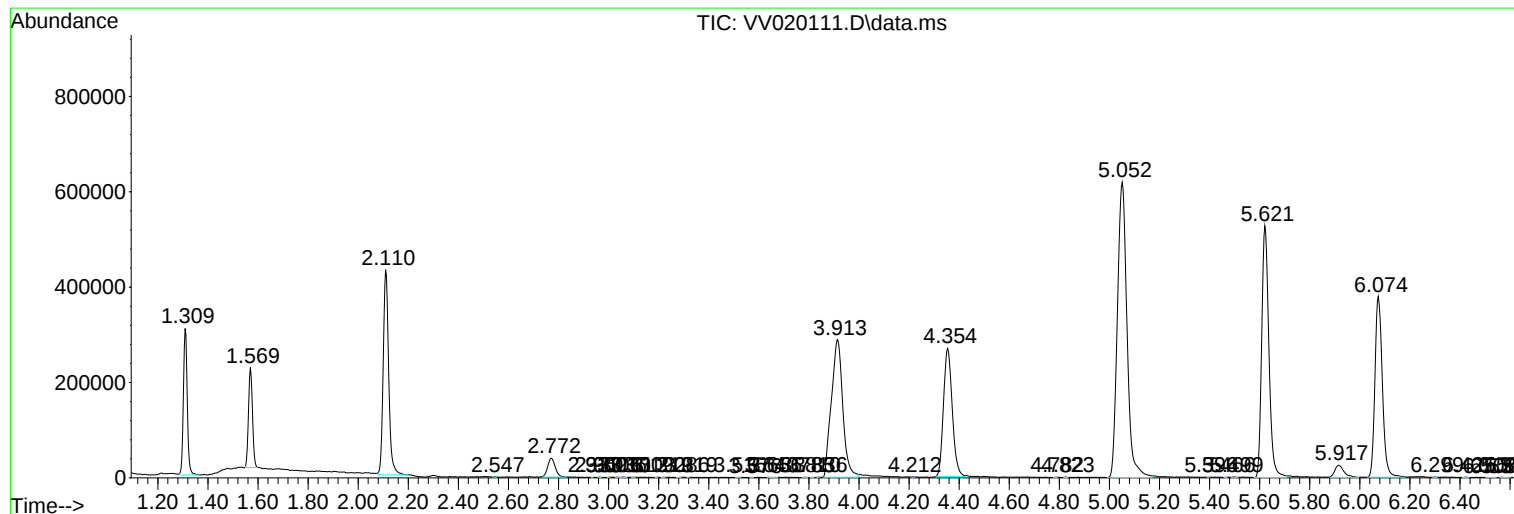

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020111.D
Acq On : 21 Jan 2021 16:07
Operator : SY/MD
Sample : M1181-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020111.D
Acq On : 21 Jan 2021 16:07
Operator : SY/MD
Sample : M1181-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------