

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020112.D
 Acq On : 21 Jan 2021 16:30
 Operator : SY/MD
 Sample : M1181-01DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E20DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	62	69	87	rVB2	656148	721541	38.03%	4.215%
2	1.569	142	149	163	rVB	254067	285732	15.06%	1.669%
3	2.110	307	317	340	rVB	490435	748563	39.45%	4.373%
4	2.476	430	431	433	rBV2	517	238	0.01%	0.001%
5	2.611	469	473	474	rBV3	817	636	0.03%	0.004%
6	2.765	510	521	536	rBV2	16203	30407	1.60%	0.178%
7	2.901	559	563	566	rBV2	1020	887	0.05%	0.005%
8	2.987	585	590	594	rVB6	630	635	0.03%	0.004%
9	3.019	598	600	603	rBV2	417	297	0.02%	0.002%
10	3.122	628	632	636	rBV2	579	584	0.03%	0.003%
11	3.309	687	690	693	rBV4	590	396	0.02%	0.002%
12	3.412	719	722	724	rVB2	814	492	0.03%	0.003%
13	3.486	741	745	747	rBV3	615	428	0.02%	0.003%
14	3.582	773	775	776	rBV3	627	255	0.01%	0.001%
15	3.675	802	804	806	rBV3	854	533	0.03%	0.003%
16	3.823	845	850	851	rBV4	726	624	0.03%	0.004%
17	3.913	859	878	908	rBV2	574085	1657771	87.37%	9.684%
18	4.290	993	995	997	rBV2	638	226	0.01%	0.001%
19	4.354	999	1015	1043	rVV	311538	766685	40.41%	4.478%
20	4.640	1101	1104	1107	rBV4	727	527	0.03%	0.003%
21	4.791	1149	1151	1155	rBV4	683	513	0.03%	0.003%
22	4.839	1164	1166	1168	rBV3	696	384	0.02%	0.002%
23	4.962	1202	1204	1207	rBV2	366	252	0.01%	0.001%
24	5.052	1213	1232	1267	rBV2	731479	1897355	100.00%	11.083%
25	5.402	1339	1341	1343	rBV2	806	412	0.02%	0.002%
26	5.476	1361	1364	1366	rBV3	632	317	0.02%	0.002%
27	5.495	1366	1370	1371	rBV3	1079	678	0.04%	0.004%
28	5.621	1397	1409	1449	rVV	610098	1214979	64.04%	7.097%
29	5.910	1490	1499	1512	rBV2	28141	55053	2.90%	0.322%
30	6.010	1527	1530	1532	rBV4	565	363	0.02%	0.002%
31	6.074	1537	1550	1578	rVV	434345	870171	45.86%	5.083%
32	6.328	1627	1629	1635	rVB2	559	357	0.02%	0.002%
33	6.360	1635	1639	1640	rBV2	537	264	0.01%	0.002%
34	6.473	1673	1674	1675	rVV	770	270	0.01%	0.002%
35	6.502	1679	1683	1686	rVV2	520	371	0.02%	0.002%
36	6.527	1689	1691	1694	rVV	523	284	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020112.D
 Acq On : 21 Jan 2021 16:30
 Operator : SY/MD
 Sample : M1181-01DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E20DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	6.543	1694	1696	1699	rVV2	596	369	0.02%	0.002%
38	6.560	1699	1701	1704	rVB	542	250	0.01%	0.001%
39	6.650	1723	1729	1731	rBV3	759	621	0.03%	0.004%
40	6.704	1742	1746	1750	rBV3	582	612	0.03%	0.004%
41	6.823	1777	1783	1785	rBV2	396	428	0.02%	0.003%
42	6.897	1801	1806	1808	rBV4	395	317	0.02%	0.002%
43	6.990	1818	1835	1867	rBV	263151	474796	25.02%	2.773%
44	7.190	1894	1897	1898	rBV	682	372	0.02%	0.002%
45	7.322	1926	1938	1957	rBV	939640	1613559	85.04%	9.425%
46	7.624	2022	2032	2061	rVV	177501	311640	16.42%	1.820%
47	8.093	2167	2178	2219	rBV2	486432	949969	50.07%	5.549%
48	8.656	2350	2353	2354	rBV3	415	225	0.01%	0.001%
49	8.682	2360	2361	2365	rVB2	571	303	0.02%	0.002%
50	8.704	2365	2368	2369	rBV2	537	237	0.01%	0.001%
51	8.762	2383	2386	2390	rBV2	535	386	0.02%	0.002%
52	8.794	2394	2396	2403	rBV2	456	479	0.03%	0.003%
53	8.855	2403	2415	2443	rBV	949690	1567875	82.63%	9.158%
54	9.116	2493	2496	2498	rBV2	687	447	0.02%	0.003%
55	9.228	2529	2531	2534	rVB2	583	287	0.02%	0.002%
56	9.248	2534	2537	2538	rBV	671	311	0.02%	0.002%
57	9.321	2558	2560	2563	rBV2	533	270	0.01%	0.002%
58	9.415	2587	2589	2591	rBV	473	282	0.01%	0.002%
59	9.543	2625	2629	2630	rBV2	599	401	0.02%	0.002%
60	9.627	2650	2655	2657	rBV2	572	429	0.02%	0.003%
61	9.765	2696	2698	2701	rVB2	565	323	0.02%	0.002%
62	9.784	2701	2704	2705	rBV3	589	302	0.02%	0.002%
63	9.903	2738	2741	2744	rBV3	685	485	0.03%	0.003%
64	9.936	2749	2751	2753	rBV3	563	366	0.02%	0.002%
65	10.103	2801	2803	2806	rVB3	659	308	0.02%	0.002%
66	10.222	2829	2840	2859	rBV	527287	820098	43.22%	4.790%
67	10.411	2897	2899	2905	rVB3	716	581	0.03%	0.003%
68	10.473	2915	2918	2922	rBV5	821	737	0.04%	0.004%
69	10.534	2933	2937	2940	rVV3	443	401	0.02%	0.002%
70	10.550	2940	2942	2950	rVB5	664	621	0.03%	0.004%
71	10.659	2975	2976	2982	rVB2	732	525	0.03%	0.003%
72	10.691	2982	2986	2988	rBV2	731	451	0.02%	0.003%
73	10.730	2996	2998	3002	rBV3	426	325	0.02%	0.002%
74	10.768	3009	3010	3013	rVV2	418	280	0.01%	0.002%
75	10.797	3017	3019	3022	rBV	429	225	0.01%	0.001%
76	10.855	3031	3037	3039	rBV4	617	527	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020112.D
 Acq On : 21 Jan 2021 16:30
 Operator : SY/MD
 Sample : M1181-01DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E20DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

77	10.900	3048	3051	3053	rBV3	449	273	0.01%	0.002%
78	10.974	3071	3074	3077	rBV2	497	305	0.02%	0.002%
79	11.000	3079	3082	3088	rVB2	462	413	0.02%	0.002%
80	11.154	3127	3130	3131	rBV2	510	313	0.02%	0.002%
81	11.257	3149	3162	3182	rBV	950394	1509010	79.53%	8.815%
82	11.630	3266	3278	3305	rBV	999212	1573650	82.94%	9.192%
83	11.836	3340	3342	3344	rBV	381	234	0.01%	0.001%
84	11.952	3376	3378	3381	rBV2	712	362	0.02%	0.002%
85	12.132	3430	3434	3441	rBV3	420	652	0.03%	0.004%
86	12.321	3489	3493	3494	rBV2	455	271	0.01%	0.002%
87	12.376	3507	3510	3512	rBV	525	360	0.02%	0.002%
88	12.466	3534	3538	3541	rBV3	490	491	0.03%	0.003%
89	12.546	3558	3563	3569	rBV3	446	626	0.03%	0.004%
90	12.659	3591	3598	3607	rVB7	1627	2710	0.14%	0.016%
91	12.749	3624	3626	3629	rVB2	818	412	0.02%	0.002%
92	12.939	3682	3685	3690	rVB2	593	369	0.02%	0.002%
93	13.022	3708	3711	3713	rBV	562	315	0.02%	0.002%
94	13.099	3732	3735	3736	rBV	445	254	0.01%	0.001%
95	13.209	3767	3769	3772	rBV2	376	228	0.01%	0.001%
96	13.273	3786	3789	3796	rVB5	2272	2351	0.12%	0.014%
97	13.521	3859	3866	3874	rBV3	2035	2894	0.15%	0.017%
98	13.755	3933	3939	3945	rBV6	1602	2493	0.13%	0.015%
99	13.797	3950	3952	3956	rVB2	765	465	0.02%	0.003%
100	16.193	4693	4697	4705	rBV	12884	9097	0.48%	0.053%


Sum of corrected areas: 17119448

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020112.D
Acq On : 21 Jan 2021 16:30
Operator : SY/MD
Sample : M1181-01DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E20DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

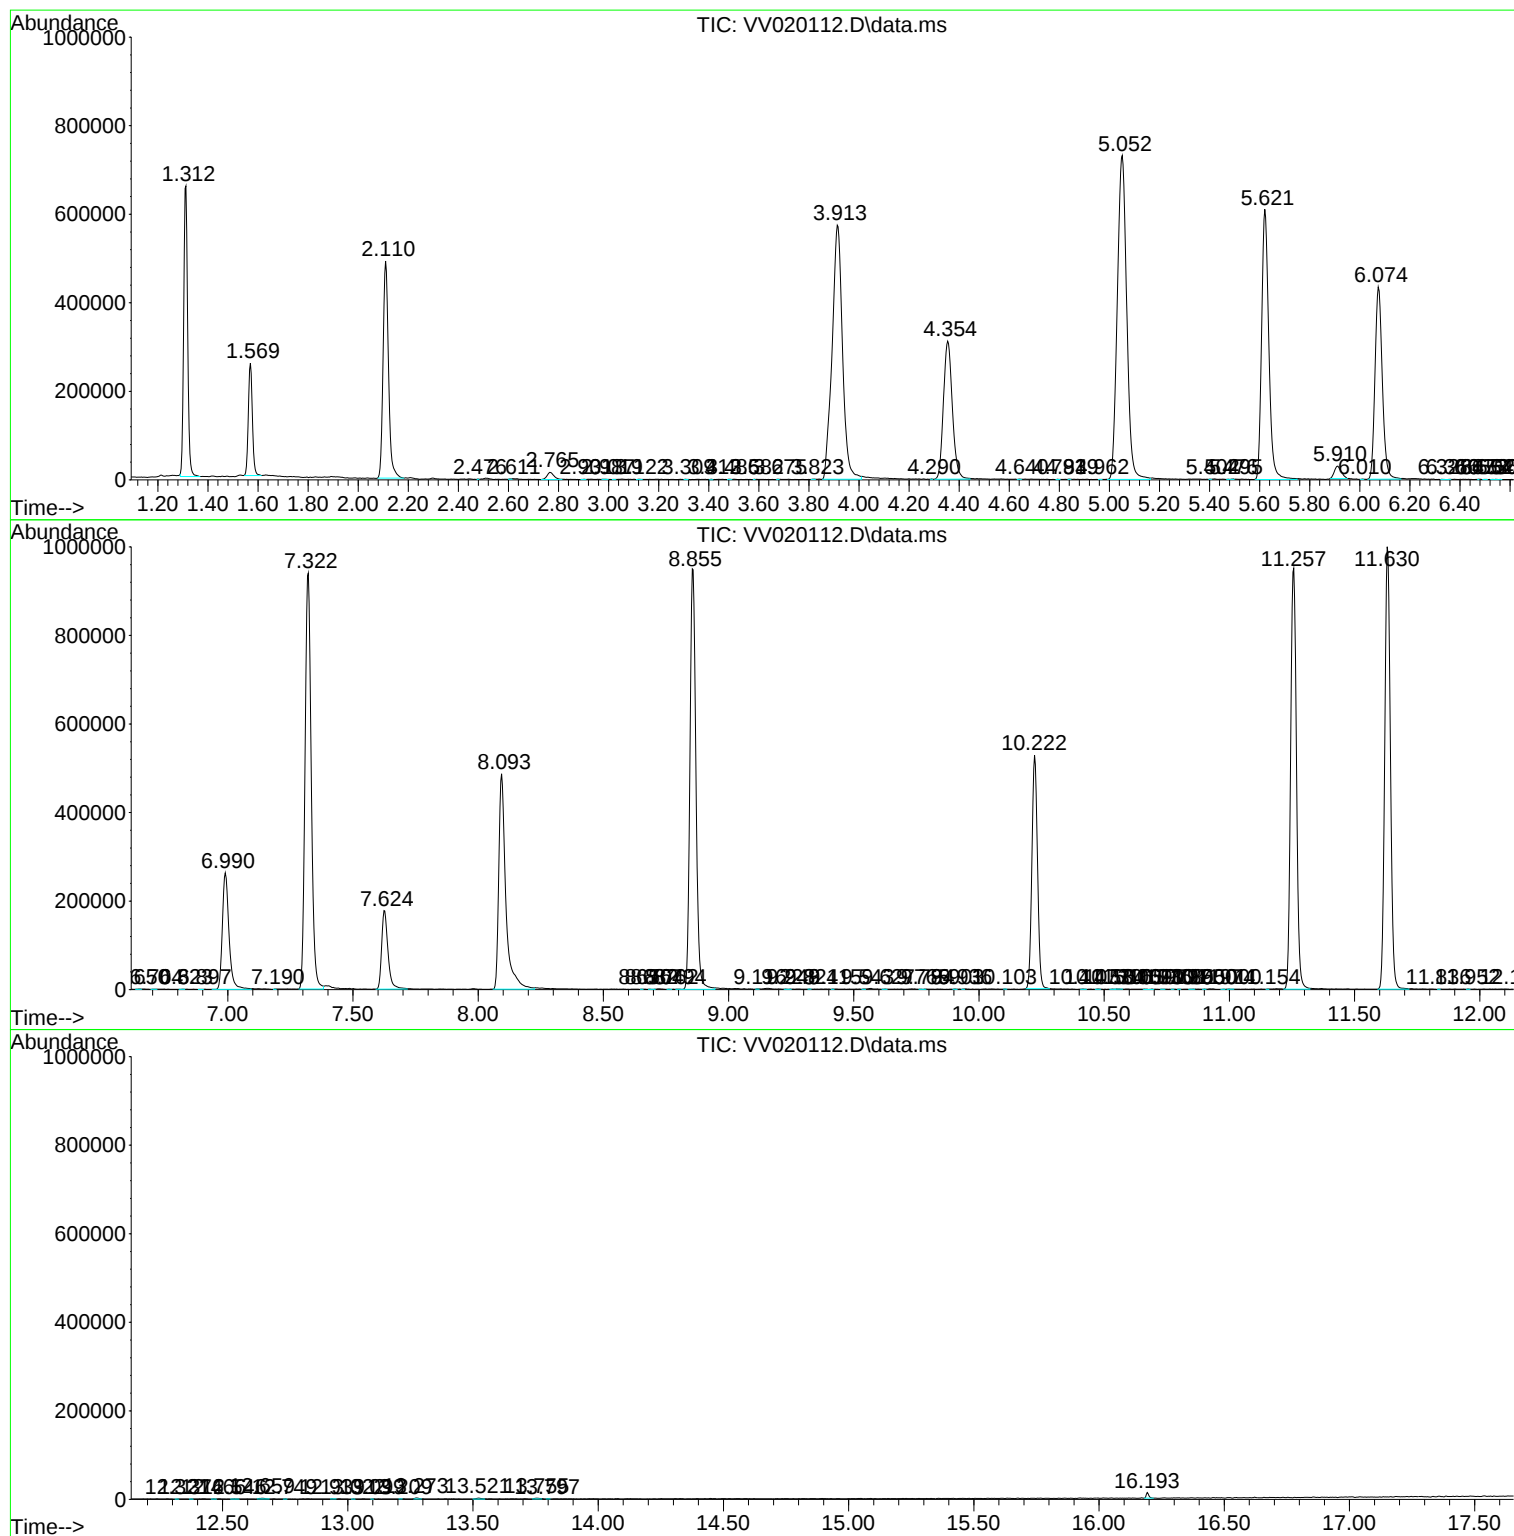

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020112.D
Acq On : 21 Jan 2021 16:30
Operator : SY/MD
Sample : M1181-01DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E20DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020112.D
Acq On : 21 Jan 2021 16:30
Operator : SY/MD
Sample : M1181-01DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E20DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------