

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020113.D
 Acq On : 21 Jan 2021 16:54
 Operator : SY/MD
 Sample : M1181-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E21DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	85	rVB2	477207	516455	28.40%	3.423%
2	1.569	142	149	165	rVB	250910	276166	15.19%	1.830%
3	2.110	306	317	337	rBV	485521	722601	39.73%	4.789%
4	2.296	367	375	384	rBV3	2321	3615	0.20%	0.024%
5	2.676	490	493	494	rBV2	739	326	0.02%	0.002%
6	2.730	506	510	513	rBV2	491	518	0.03%	0.003%
7	2.769	513	522	535	rVV3	7698	14069	0.77%	0.093%
8	2.907	563	565	569	rBV2	408	283	0.02%	0.002%
9	2.965	581	583	585	rBV3	436	238	0.01%	0.002%
10	3.007	593	596	601	rBV5	733	722	0.04%	0.005%
11	3.042	605	607	608	rVV	556	185	0.01%	0.001%
12	3.068	613	615	618	rBV	637	364	0.02%	0.002%
13	3.116	628	630	632	rBV2	426	222	0.01%	0.001%
14	3.135	635	636	640	rVB3	770	228	0.01%	0.002%
15	3.155	640	642	644	rBV2	450	199	0.01%	0.001%
16	3.216	658	661	664	rBV3	475	323	0.02%	0.002%
17	3.235	664	667	669	rBV2	523	289	0.02%	0.002%
18	3.283	679	682	685	rBV4	675	529	0.03%	0.004%
19	3.405	717	720	721	rBV	398	205	0.01%	0.001%
20	3.438	728	730	733	rVB2	360	180	0.01%	0.001%
21	3.467	737	739	742	rBV2	335	217	0.01%	0.001%
22	3.512	746	753	755	rBV3	878	915	0.05%	0.006%
23	3.663	797	800	801	rBV2	526	283	0.02%	0.002%
24	3.749	822	827	828	rBV3	767	579	0.03%	0.004%
25	3.804	841	844	848	rVV4	451	384	0.02%	0.003%
26	3.840	852	855	856	rBV3	385	212	0.01%	0.001%
27	3.913	859	878	906	rBV2	373281	1141351	62.76%	7.564%
28	4.354	1000	1015	1041	rBV	285612	698865	38.43%	4.631%
29	4.663	1108	1111	1112	rBV3	945	504	0.03%	0.003%
30	4.720	1126	1129	1130	rBV2	574	234	0.01%	0.002%
31	4.759	1139	1141	1143	rBV2	468	257	0.01%	0.002%
32	4.913	1185	1189	1191	rBV3	865	627	0.03%	0.004%
33	4.926	1191	1193	1195	rVB3	569	263	0.01%	0.002%
34	4.939	1195	1197	1200	rBV	345	207	0.01%	0.001%
35	5.052	1211	1232	1260	rBV2	694715	1818562	100.00%	12.052%
36	5.373	1328	1332	1335	rBV4	797	724	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020113.D
 Acq On : 21 Jan 2021 16:54
 Operator : SY/MD
 Sample : M1181-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E21DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	5.537	1381	1383	1385	rBV2	315	197	0.01%	0.001%
38	5.621	1395	1409	1439	rBV	555685	1102828	60.64%	7.309%
39	5.910	1490	1499	1516	rVB3	27075	55179	3.03%	0.366%
40	6.026	1533	1535	1536	rBV2	707	283	0.02%	0.002%
41	6.074	1536	1550	1578	rVV	404486	813863	44.75%	5.394%
42	6.441	1659	1664	1665	rBV3	1041	917	0.05%	0.006%
43	6.573	1703	1705	1708	rBV3	403	221	0.01%	0.001%
44	6.807	1773	1778	1780	rBV3	305	307	0.02%	0.002%
45	6.872	1794	1798	1801	rBV4	257	216	0.01%	0.001%
46	6.904	1804	1808	1812	rVB2	641	427	0.02%	0.003%
47	6.926	1812	1815	1817	rBV3	634	273	0.02%	0.002%
48	6.990	1823	1835	1866	rBV	241647	439487	24.17%	2.913%
49	7.322	1925	1938	1963	rBV	922021	1585117	87.16%	10.505%
50	7.627	2021	2033	2053	rBV	158745	278447	15.31%	1.845%
51	7.891	2112	2115	2119	rVV3	335	272	0.01%	0.002%
52	7.984	2138	2144	2150	rBV5	1082	1491	0.08%	0.010%
53	8.039	2158	2161	2163	rBV2	359	239	0.01%	0.002%
54	8.093	2167	2178	2210	rBV2	413382	821834	45.19%	5.446%
55	8.399	2270	2273	2276	rBV3	1026	712	0.04%	0.005%
56	8.486	2296	2300	2302	rBV2	386	287	0.02%	0.002%
57	8.566	2321	2325	2327	rBV2	300	257	0.01%	0.002%
58	8.624	2340	2343	2344	rBV2	413	259	0.01%	0.002%
59	8.691	2362	2364	2365	rBV	480	197	0.01%	0.001%
60	8.749	2380	2382	2388	rBV3	903	977	0.05%	0.006%
61	8.859	2403	2416	2440	rBV	895373	1403672	77.19%	9.302%
62	9.206	2523	2524	2528	rBV3	570	307	0.02%	0.002%
63	9.257	2536	2540	2542	rBV3	654	427	0.02%	0.003%
64	9.341	2563	2566	2569	rBV2	661	513	0.03%	0.003%
65	9.392	2578	2582	2588	rBV6	951	765	0.04%	0.005%
66	9.437	2594	2596	2599	rBV	837	640	0.04%	0.004%
67	9.473	2604	2607	2608	rBV3	498	274	0.02%	0.002%
68	9.585	2640	2642	2644	rBV	489	301	0.02%	0.002%
69	9.672	2666	2669	2675	rVB5	819	942	0.05%	0.006%
70	9.711	2677	2681	2683	rBV3	512	408	0.02%	0.003%
71	9.939	2750	2752	2753	rBV	552	215	0.01%	0.001%
72	10.023	2776	2778	2781	rBV3	633	402	0.02%	0.003%
73	10.141	2813	2815	2819	rBV3	504	350	0.02%	0.002%
74	10.222	2826	2840	2865	rBV	486690	759041	41.74%	5.030%
75	10.379	2886	2889	2891	rBV2	867	434	0.02%	0.003%
76	10.415	2897	2900	2903	rBV2	464	300	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020113.D
 Acq On : 21 Jan 2021 16:54
 Operator : SY/MD
 Sample : M1181-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E21DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

77	10.627	2960	2966	2970	rBV4	696	772	0.04%	0.005%
78	10.704	2985	2990	2996	rBV5	663	946	0.05%	0.006%
79	10.740	2999	3001	3005	rVB3	413	215	0.01%	0.001%
80	10.862	3036	3039	3040	rVV	461	212	0.01%	0.001%
81	10.977	3073	3075	3079	rBV4	379	203	0.01%	0.001%
82	11.074	3102	3105	3107	rBV2	313	186	0.01%	0.001%
83	11.161	3128	3132	3133	rBV3	871	526	0.03%	0.003%
84	11.257	3150	3162	3182	rBV	848283	1311127	72.10%	8.689%
85	11.437	3215	3218	3219	rBV	786	368	0.02%	0.002%
86	11.630	3266	3278	3298	rBV	814478	1291156	71.00%	8.557%
87	11.862	3348	3350	3351	rBV	576	272	0.01%	0.002%
88	11.900	3360	3362	3364	rBV2	574	267	0.01%	0.002%
89	12.039	3403	3405	3407	rBV2	604	346	0.02%	0.002%
90	12.424	3522	3525	3532	rBV4	873	906	0.05%	0.006%
91	12.457	3532	3535	3538	rBV2	531	378	0.02%	0.003%
92	12.662	3591	3599	3602	rBV4	1269	1587	0.09%	0.011%
93	12.714	3612	3615	3622	rBV2	403	401	0.02%	0.003%
94	13.276	3785	3790	3794	rBV6	1680	1683	0.09%	0.011%
95	13.392	3824	3826	3831	rBV3	595	524	0.03%	0.003%
96	13.495	3855	3858	3860	rBV	502	293	0.02%	0.002%
97	13.508	3860	3862	3863	rBV	712	290	0.02%	0.002%
98	13.521	3863	3866	3870	rVB3	1034	848	0.05%	0.006%
99	13.717	3925	3927	3931	rBV2	490	407	0.02%	0.003%
100	14.408	4139	4142	4144	rBV3	687	431	0.02%	0.003%




Sum of corrected areas: 15089523

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020113.D
Acq On : 21 Jan 2021 16:54
Operator : SY/MD
Sample : M1181-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

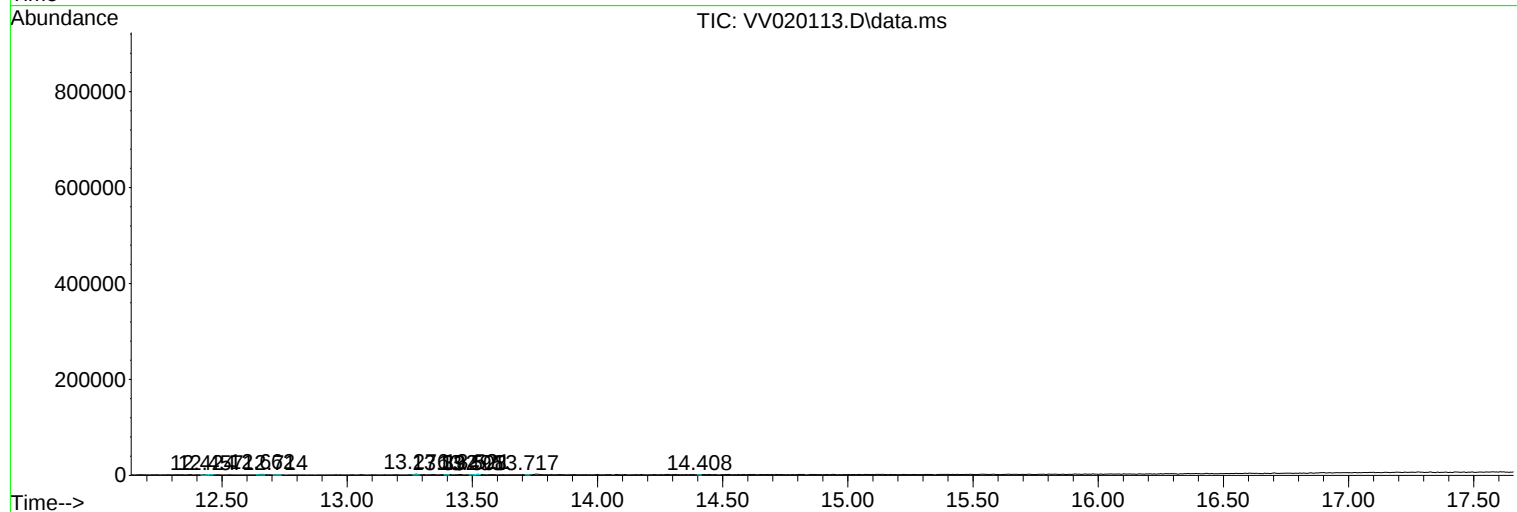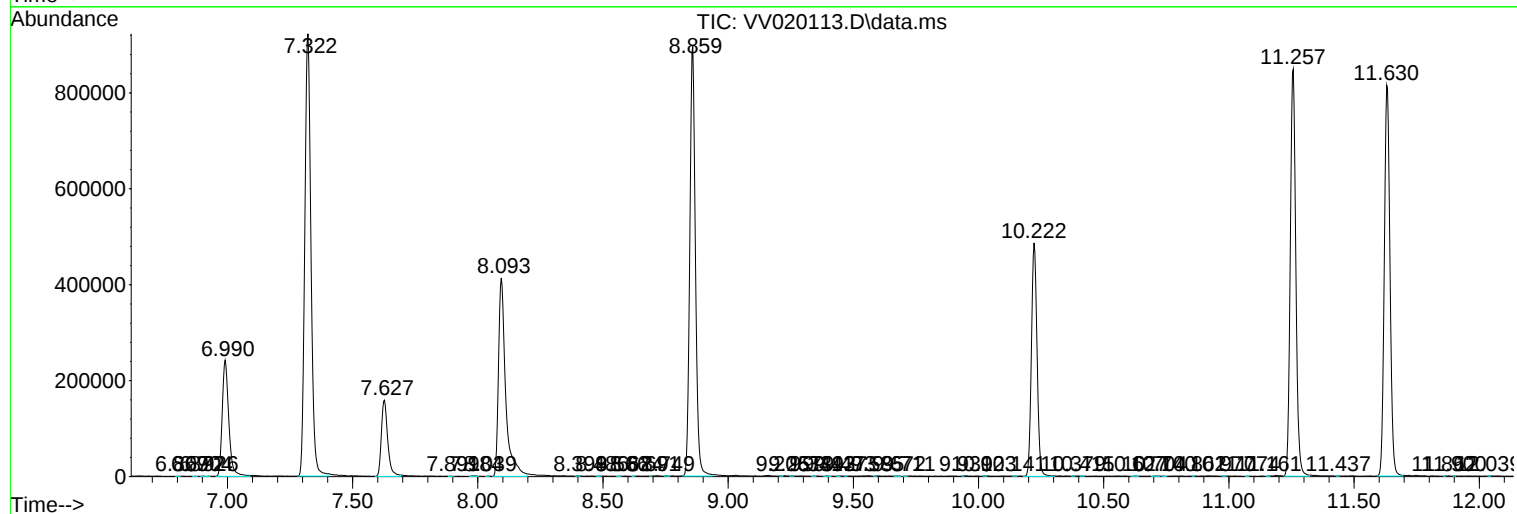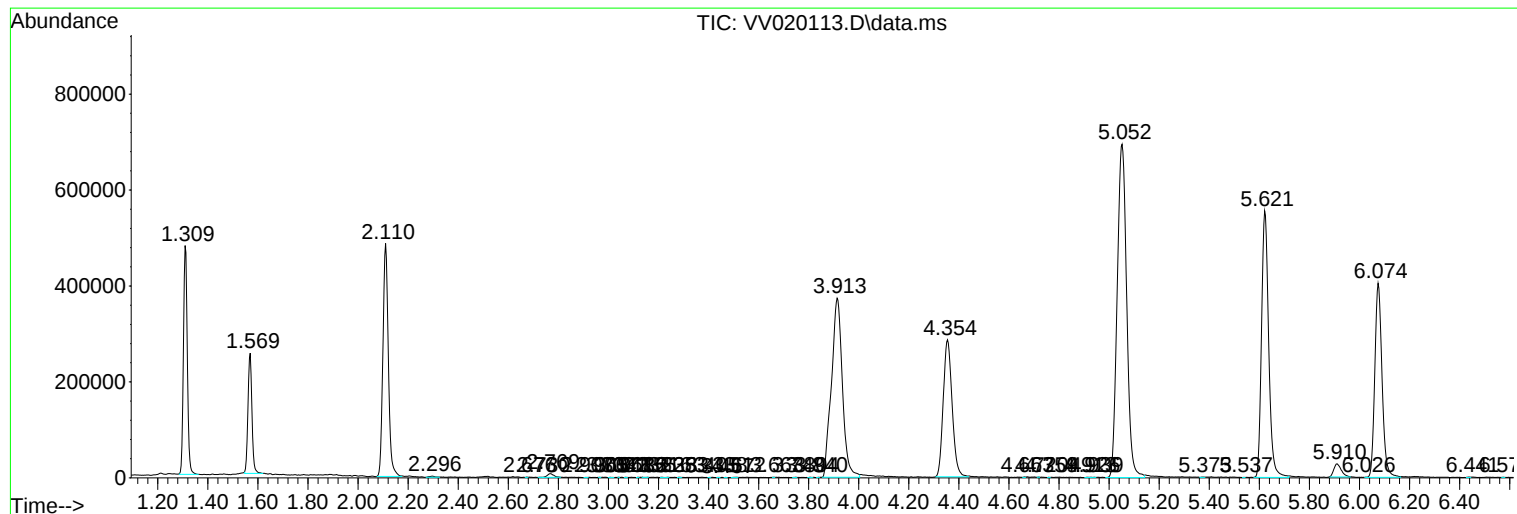

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020113.D
Acq On : 21 Jan 2021 16:54
Operator : SY/MD
Sample : M1181-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020113.D
Acq On : 21 Jan 2021 16:54
Operator : SY/MD
Sample : M1181-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
