

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020114.D
 Acq On : 21 Jan 2021 17:17
 Operator : SY/MD
 Sample : M1181-03DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E22DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	84	rVB	253897	279845	15.65%	1.775%
2	1.569	142	149	161	rBV	221120	257010	14.37%	1.630%
3	2.103	305	315	340	rBV	481583	721738	40.37%	4.578%
4	2.508	432	441	455	rVB3	6312	11902	0.67%	0.075%
5	2.872	550	554	557	rVB3	596	451	0.03%	0.003%
6	2.990	588	591	592	rBV2	481	162	0.01%	0.001%
7	3.010	592	597	599	rBV5	671	671	0.04%	0.004%
8	3.032	599	604	606	rBV4	928	828	0.05%	0.005%
9	3.142	636	638	643	rBV2	496	426	0.02%	0.003%
10	3.161	643	644	648	rBV2	459	355	0.02%	0.002%
11	3.412	720	722	725	rBV2	468	328	0.02%	0.002%
12	3.447	732	733	736	rBV2	387	218	0.01%	0.001%
13	3.563	767	769	772	rBV	571	278	0.02%	0.002%
14	3.582	772	775	779	rVB2	690	339	0.02%	0.002%
15	3.611	779	784	787	rBV4	954	949	0.05%	0.006%
16	3.675	802	804	806	rVB	464	196	0.01%	0.001%
17	3.688	806	808	810	rBV	397	170	0.01%	0.001%
18	3.781	835	837	838	rBV	201	108	0.01%	0.001%
19	3.859	859	861	862	rBV	479	225	0.01%	0.001%
20	3.910	862	877	916	rVV3	347208	1011965	56.60%	6.419%
21	4.351	998	1014	1042	rBV	290877	722955	40.44%	4.586%
22	4.560	1077	1079	1081	rBV2	1147	689	0.04%	0.004%
23	4.785	1147	1149	1153	rBV2	968	643	0.04%	0.004%
24	4.929	1192	1194	1197	rBV3	477	279	0.02%	0.002%
25	4.974	1204	1208	1210	rBV4	470	335	0.02%	0.002%
26	5.048	1214	1231	1256	rBV2	703779	1787910	100.00%	11.342%
27	5.621	1395	1409	1439	rBV	549944	1112808	62.24%	7.059%
28	5.916	1488	1501	1525	rBV3	131458	285130	15.95%	1.809%
29	6.074	1535	1550	1577	rBV	446465	905236	50.63%	5.742%
30	6.315	1624	1625	1626	rVB	429	83	0.00%	0.001%
31	6.370	1639	1642	1644	rBV	379	308	0.02%	0.002%
32	6.408	1651	1654	1657	rBV3	289	216	0.01%	0.001%
33	6.424	1657	1659	1661	rBV2	511	183	0.01%	0.001%
34	6.450	1666	1667	1668	rVB2	189	36	0.00%	0.000%
35	6.482	1670	1677	1680	rBV5	685	963	0.05%	0.006%
36	6.514	1680	1687	1688	rBV4	1075	954	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012121\
 Data File : VW020114.D
 Acq On : 21 Jan 2021 17:17
 Operator : SY/MD
 Sample : M1181-03DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E22DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

37	6.556	1699	1700	1701	rVB4	73	14	0.00%	0.000%
38	6.566	1701	1703	1707	rBV2	424	365	0.02%	0.002%
39	6.608	1712	1716	1718	rBV	328	211	0.01%	0.001%
40	6.630	1718	1723	1726	rBV3	716	706	0.04%	0.004%
41	6.691	1740	1742	1743	rVB	295	98	0.01%	0.001%
42	6.704	1743	1746	1751	rBV3	761	668	0.04%	0.004%
43	6.743	1757	1758	1760	rBV	469	131	0.01%	0.001%
44	6.804	1775	1777	1778	rBV	434	186	0.01%	0.001%
45	6.852	1790	1792	1795	rBV4	517	226	0.01%	0.001%
46	6.897	1804	1806	1808	rBV2	415	242	0.01%	0.002%
47	6.942	1818	1820	1822	rBV	493	170	0.01%	0.001%
48	6.990	1822	1835	1863	rBV	216146	399189	22.33%	2.532%
49	7.318	1926	1937	1959	rBV	823065	1424567	79.68%	9.037%
50	7.627	2022	2033	2055	rBV	155187	275872	15.43%	1.750%
51	7.836	2096	2098	2102	rBV4	1033	769	0.04%	0.005%
52	7.907	2118	2120	2123	rBV3	626	360	0.02%	0.002%
53	7.981	2130	2143	2164	rBV	363452	607084	33.95%	3.851%
54	8.103	2169	2181	2221	rBV2	351973	857529	47.96%	5.440%
55	8.730	2374	2376	2377	rBV2	304	114	0.01%	0.001%
56	8.772	2384	2389	2391	rBV2	523	406	0.02%	0.003%
57	8.858	2403	2416	2441	rBV	911504	1477094	82.62%	9.370%
58	9.116	2493	2496	2499	rBV3	692	454	0.03%	0.003%
59	9.254	2536	2539	2542	rBV2	364	211	0.01%	0.001%
60	9.321	2556	2560	2569	rBV3	538	704	0.04%	0.004%
61	9.373	2574	2576	2578	rBV	370	222	0.01%	0.001%
62	9.418	2587	2590	2594	rVB2	642	433	0.02%	0.003%
63	9.492	2608	2613	2616	rBV2	470	402	0.02%	0.003%
64	9.553	2627	2632	2637	rBV5	2083	2999	0.17%	0.019%
65	9.627	2651	2655	2659	rBV3	658	553	0.03%	0.004%
66	9.656	2662	2664	2668	rVB2	338	231	0.01%	0.001%
67	9.678	2669	2671	2675	rBV	162	123	0.01%	0.001%
68	9.707	2678	2680	2682	rBV2	416	180	0.01%	0.001%
69	9.804	2705	2710	2713	rBV3	442	445	0.02%	0.003%
70	9.836	2719	2720	2722	rBV	355	157	0.01%	0.001%
71	10.019	2774	2777	2778	rBV	460	207	0.01%	0.001%
72	10.106	2803	2804	2805	rBV	448	130	0.01%	0.001%
73	10.177	2824	2826	2829	rVB2	634	320	0.02%	0.002%
74	10.225	2829	2841	2859	rBV	551078	899880	50.33%	5.708%
75	10.550	2936	2942	2948	rBV3	2269	2812	0.16%	0.018%
76	10.752	3003	3005	3010	rBV	415	273	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020114.D
 Acq On : 21 Jan 2021 17:17
 Operator : SY/MD
 Sample : M1181-03DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E22DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

77	11.148	3126	3128	3130	rBV	438	200	0.01%	0.001%
78	11.193	3134	3142	3151	rBV7	3670	5424	0.30%	0.034%
79	11.257	3151	3162	3186	rVV	869228	1330279	74.40%	8.439%
80	11.427	3211	3215	3217	rBV2	821	729	0.04%	0.005%
81	11.540	3248	3250	3251	rBV	504	244	0.01%	0.002%
82	11.633	3266	3279	3297	rBV	866770	1352540	75.65%	8.580%
83	12.099	3422	3424	3429	rBV4	444	366	0.02%	0.002%
84	12.325	3492	3494	3499	rVB3	641	276	0.02%	0.002%
85	12.415	3520	3522	3524	rBV2	647	411	0.02%	0.003%
86	12.662	3592	3599	3607	rVB5	3236	4338	0.24%	0.028%
87	12.926	3679	3681	3684	rVB2	721	340	0.02%	0.002%
88	12.942	3684	3686	3689	rBV2	446	188	0.01%	0.001%
89	13.276	3785	3790	3795	rBV4	2253	2233	0.12%	0.014%
90	13.759	3935	3940	3950	rVB6	1971	2890	0.16%	0.018%
91	13.813	3955	3957	3960	rBV	371	202	0.01%	0.001%




Sum of corrected areas: 15764289

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020114.D
Acq On : 21 Jan 2021 17:17
Operator : SY/MD
Sample : M1181-03DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E22DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

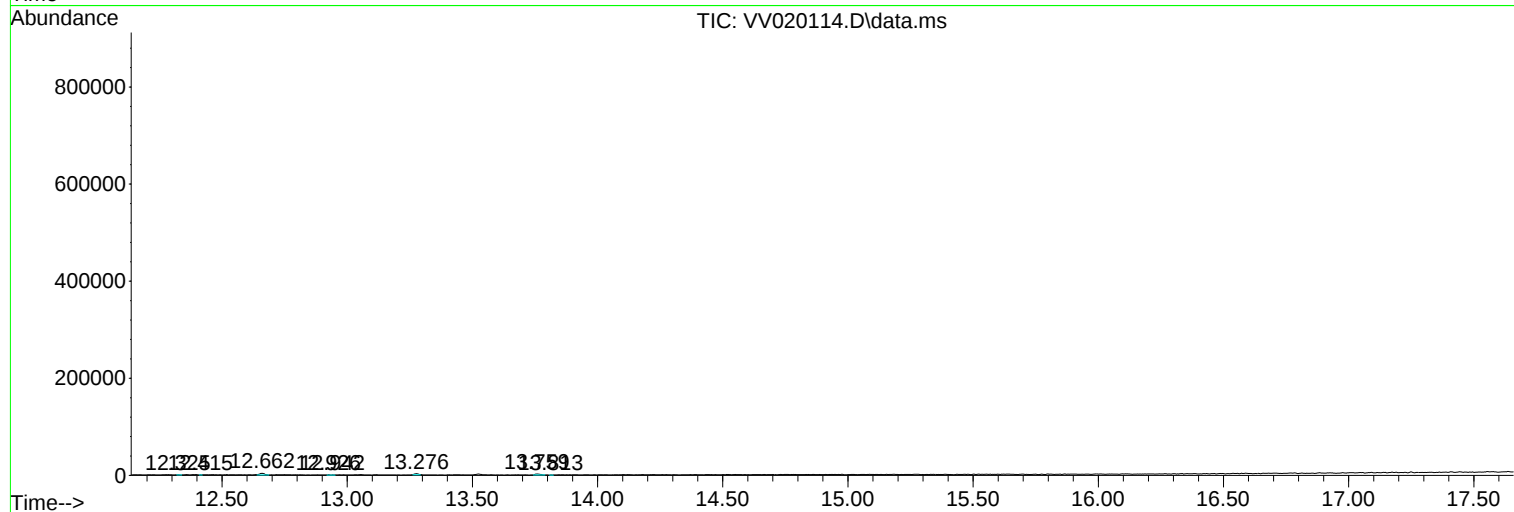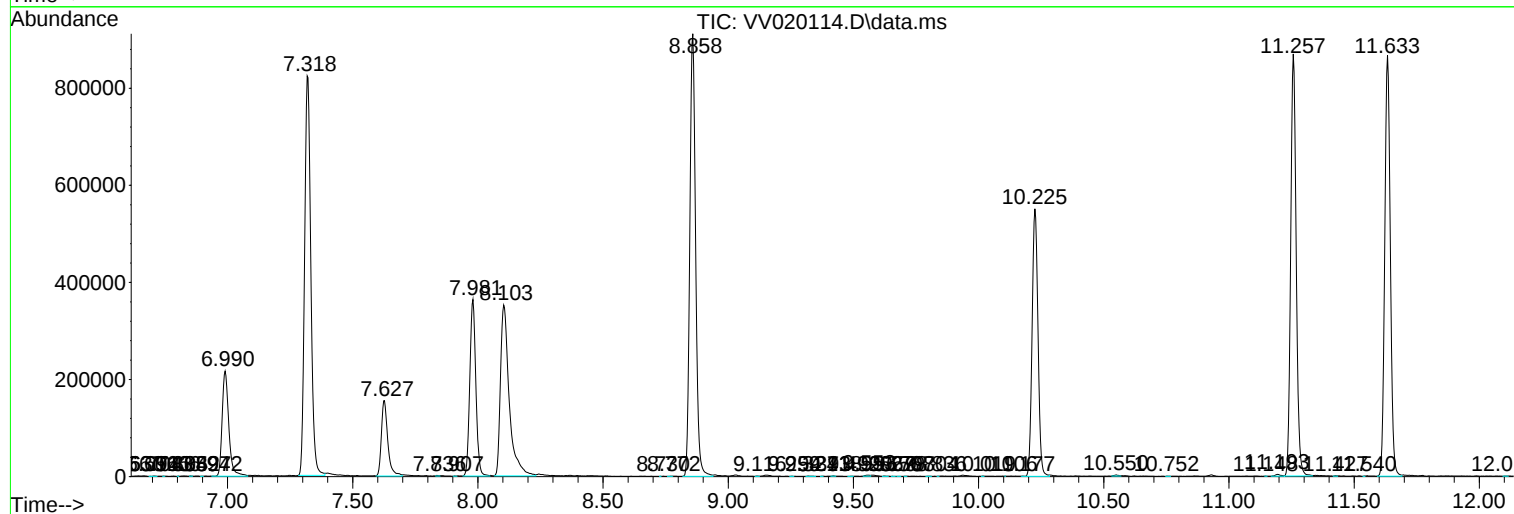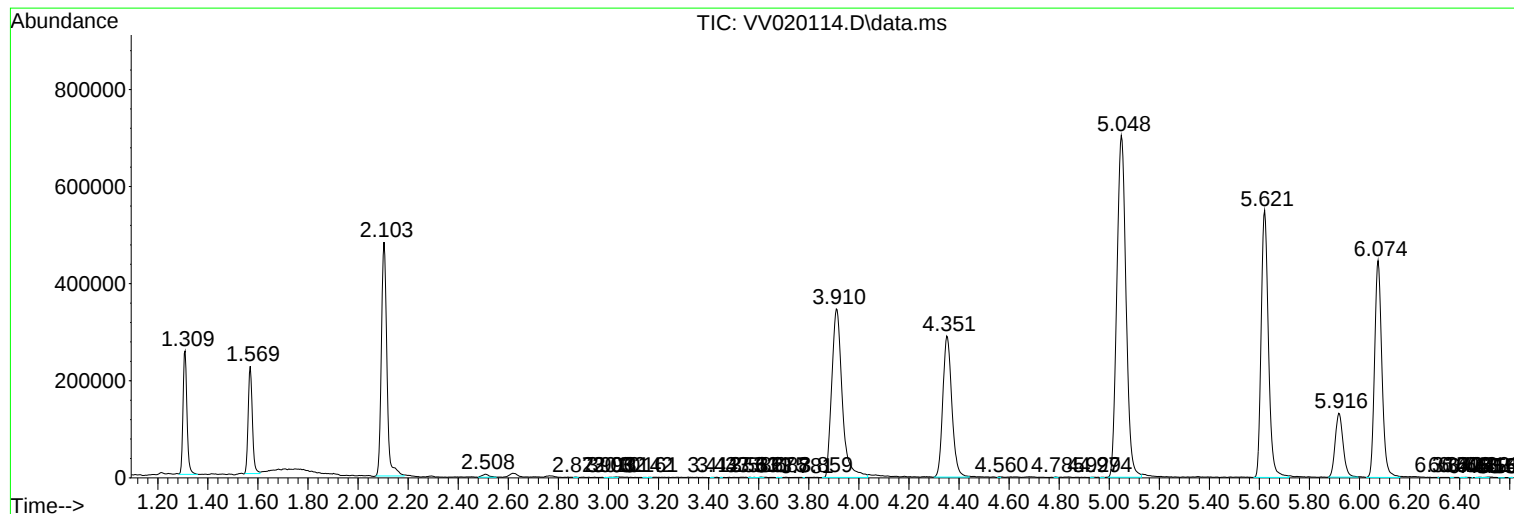

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020114.D
Acq On : 21 Jan 2021 17:17
Operator : SY/MD
Sample : M1181-03DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E22DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020114.D
Acq On : 21 Jan 2021 17:17
Operator : SY/MD
Sample : M1181-03DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E22DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
