

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020116.D
 Acq On : 21 Jan 2021 20:04
 Operator : SY/MD
 Sample : VIBLK36
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	82	rVB	257878	265706	15.81%	1.980%
2	1.569	142	149	165	rVB	218633	247554	14.73%	1.845%
3	2.110	307	317	347	rVB	462929	705537	41.97%	5.257%
4	2.450	421	423	426	rBV3	627	333	0.02%	0.002%
5	2.749	512	516	522	rVB4	767	751	0.04%	0.006%
6	2.833	539	542	546	rVB2	847	675	0.04%	0.005%
7	2.894	558	561	565	rVB3	571	432	0.03%	0.003%
8	2.920	565	569	570	rBV2	428	320	0.02%	0.002%
9	3.087	619	621	624	rBV4	476	315	0.02%	0.002%
10	3.138	635	637	639	rVB3	565	191	0.01%	0.001%
11	3.251	666	672	673	rBV	670	581	0.03%	0.004%
12	3.302	684	688	689	rBV2	328	220	0.01%	0.002%
13	3.370	708	709	716	rVB3	464	323	0.02%	0.002%
14	3.499	747	749	753	rBV2	517	238	0.01%	0.002%
15	3.566	765	770	772	rBV2	441	349	0.02%	0.003%
16	3.627	787	789	792	rVB	489	265	0.02%	0.002%
17	3.708	811	814	817	rBV3	442	303	0.02%	0.002%
18	3.807	843	845	848	rVB3	660	324	0.02%	0.002%
19	3.823	848	850	852	rVB	420	198	0.01%	0.001%
20	3.836	852	854	856	rBV	469	227	0.01%	0.002%
21	3.894	861	872	909	rBV	110641	347563	20.67%	2.590%
22	4.354	999	1015	1043	rBV	274884	683017	40.63%	5.089%
23	4.781	1146	1148	1149	rBV2	470	221	0.01%	0.002%
24	4.926	1189	1193	1194	rBV3	459	286	0.02%	0.002%
25	5.052	1213	1232	1258	rBV2	651491	1681103	100.00%	12.527%
26	5.482	1363	1366	1369	rBV2	485	403	0.02%	0.003%
27	5.495	1369	1370	1373	rVB3	671	234	0.01%	0.002%
28	5.534	1379	1382	1384	rBV2	408	351	0.02%	0.003%
29	5.556	1387	1389	1391	rVB2	580	225	0.01%	0.002%
30	5.576	1391	1395	1396	rBV3	751	458	0.03%	0.003%
31	5.621	1396	1409	1440	rBV	496176	1001435	59.57%	7.462%
32	5.910	1489	1499	1518	rVB2	40031	81533	4.85%	0.608%
33	6.074	1535	1550	1579	rBV	390267	793073	47.18%	5.910%
34	6.338	1628	1632	1633	rBV2	581	464	0.03%	0.003%
35	6.428	1658	1660	1666	rVB3	743	632	0.04%	0.005%
36	6.540	1692	1695	1697	rVB	492	271	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020116.D
 Acq On : 21 Jan 2021 20:04
 Operator : SY/MD
 Sample : VIBLK36
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	6.572	1702	1705	1708	rBV5	733	549	0.03%	0.004%
38	6.640	1722	1726	1729	rBV3	627	572	0.03%	0.004%
39	6.653	1729	1730	1732	rBV2	417	183	0.01%	0.001%
40	6.720	1746	1751	1754	rVB5	714	503	0.03%	0.004%
41	6.736	1754	1756	1758	rBV3	489	336	0.02%	0.003%
42	6.868	1794	1797	1799	rBV3	434	305	0.02%	0.002%
43	6.990	1821	1835	1854	rBV	220527	403081	23.98%	3.004%
44	7.322	1926	1938	1969	rBV	870144	1508121	89.71%	11.238%
45	7.582	2016	2019	2022	rBV3	359	252	0.01%	0.002%
46	7.624	2022	2032	2052	rBV	158740	279388	16.62%	2.082%
47	7.900	2116	2118	2120	rBV2	313	171	0.01%	0.001%
48	7.913	2120	2122	2125	rVB2	479	257	0.02%	0.002%
49	7.949	2130	2133	2134	rVB2	472	210	0.01%	0.002%
50	7.987	2136	2145	2155	rBV6	4098	6537	0.39%	0.049%
51	8.093	2168	2178	2215	rBV2	418918	854111	50.81%	6.364%
52	8.518	2307	2310	2313	rBV4	1146	964	0.06%	0.007%
53	8.675	2357	2359	2362	rBV2	412	251	0.01%	0.002%
54	8.698	2364	2366	2368	rBV3	402	184	0.01%	0.001%
55	8.752	2380	2383	2385	rBV	349	198	0.01%	0.001%
56	8.813	2399	2402	2403	rBV3	363	209	0.01%	0.002%
57	8.855	2403	2415	2441	rBV	805881	1325402	78.84%	9.876%
58	9.228	2528	2531	2534	rBV2	398	254	0.02%	0.002%
59	9.260	2538	2541	2544	rBV2	488	405	0.02%	0.003%
60	9.273	2544	2545	2548	rVB2	527	206	0.01%	0.002%
61	9.318	2557	2559	2563	rVB2	354	209	0.01%	0.002%
62	9.386	2570	2580	2584	rBV7	693	1087	0.06%	0.008%
63	9.440	2592	2597	2599	rBV3	323	332	0.02%	0.002%
64	9.521	2618	2622	2623	rBV3	419	225	0.01%	0.002%
65	9.633	2654	2657	2659	rBV2	481	294	0.02%	0.002%
66	9.797	2704	2708	2709	rBV	331	217	0.01%	0.002%
67	9.846	2719	2723	2727	rBV2	589	450	0.03%	0.003%
68	9.868	2728	2730	2735	rVB2	430	244	0.01%	0.002%
69	9.939	2747	2752	2756	rBV3	378	428	0.03%	0.003%
70	9.987	2763	2767	2769	rBV2	423	272	0.02%	0.002%
71	9.997	2769	2770	2774	rVB	356	185	0.01%	0.001%
72	10.016	2774	2776	2777	rBV	525	209	0.01%	0.002%
73	10.061	2787	2790	2792	rBV3	485	340	0.02%	0.003%
74	10.083	2792	2797	2801	rVB3	613	505	0.03%	0.004%
75	10.116	2804	2807	2809	rBV4	322	229	0.01%	0.002%
76	10.222	2828	2840	2859	rBV	447738	703498	41.85%	5.242%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020116.D
 Acq On : 21 Jan 2021 20:04
 Operator : SY/MD
 Sample : VIBLK36
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

77	10.608	2957	2960	2965	rVB3	564	421	0.03%	0.003%
78	10.685	2982	2984	2985	rBV	668	240	0.01%	0.002%
79	10.739	2997	3001	3004	rVB4	493	441	0.03%	0.003%
80	10.759	3004	3007	3009	rBV2	525	333	0.02%	0.002%
81	10.987	3076	3078	3082	rVB3	641	355	0.02%	0.003%
82	11.022	3088	3089	3093	rBV2	435	308	0.02%	0.002%
83	11.109	3114	3116	3118	rBV3	426	272	0.02%	0.002%
84	11.151	3126	3129	3130	rBV2	539	327	0.02%	0.002%
85	11.257	3150	3162	3184	rBV	830679	1269999	75.55%	9.463%
86	11.511	3239	3241	3243	rBV	858	406	0.02%	0.003%
87	11.633	3266	3279	3302	rBV	772629	1232431	73.31%	9.183%
88	11.804	3330	3332	3333	rBV	894	334	0.02%	0.002%
89	11.964	3378	3382	3383	rBV	760	464	0.03%	0.003%
90	12.045	3405	3407	3411	rBV3	526	429	0.03%	0.003%
91	12.122	3429	3431	3434	rBV3	365	203	0.01%	0.002%
92	12.472	3535	3540	3543	rBV3	562	506	0.03%	0.004%
93	12.530	3555	3558	3562	rBV3	794	812	0.05%	0.006%
94	12.653	3592	3596	3597	rBV2	774	507	0.03%	0.004%
95	12.710	3612	3614	3618	rBV2	435	370	0.02%	0.003%
96	13.267	3782	3787	3788	rBV	683	480	0.03%	0.004%
97	13.276	3788	3790	3797	rVB3	1074	1026	0.06%	0.008%
98	13.640	3900	3903	3905	rBV	396	188	0.01%	0.001%
99	13.759	3936	3940	3946	rVB6	1007	1092	0.06%	0.008%
100	14.836	4269	4275	4276	rBV4	818	791	0.05%	0.006%




Sum of corrected areas: 13420219

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020116.D
Acq On : 21 Jan 2021 20:04
Operator : SY/MD
Sample : VIBLK36
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VIBLK36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

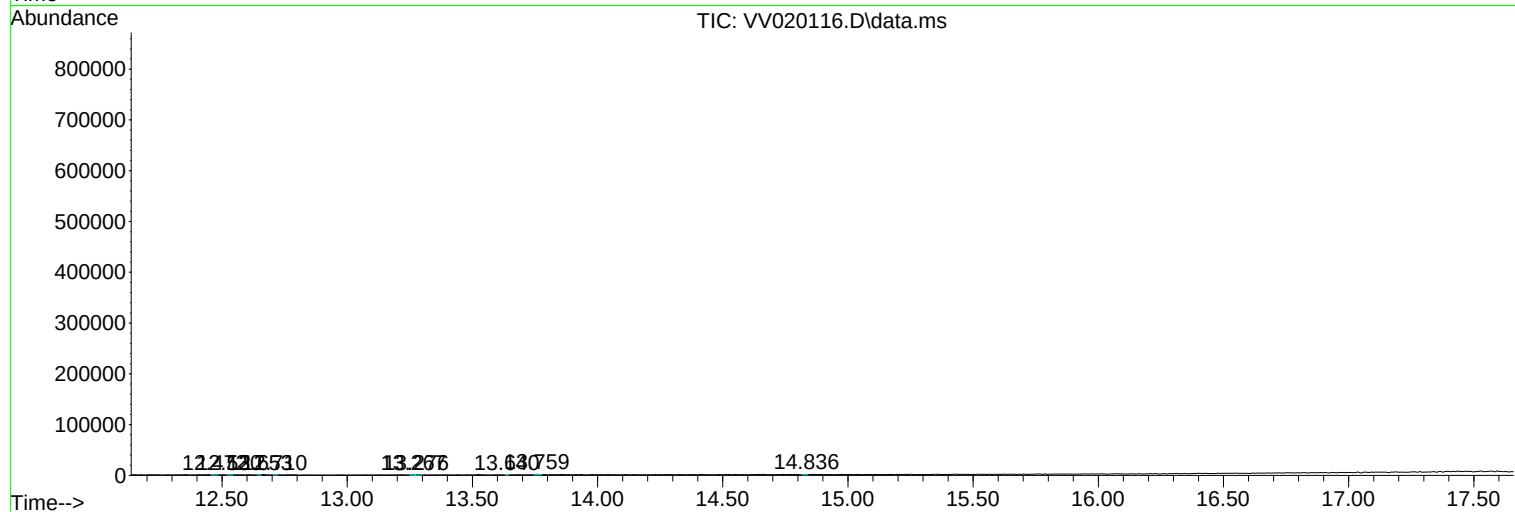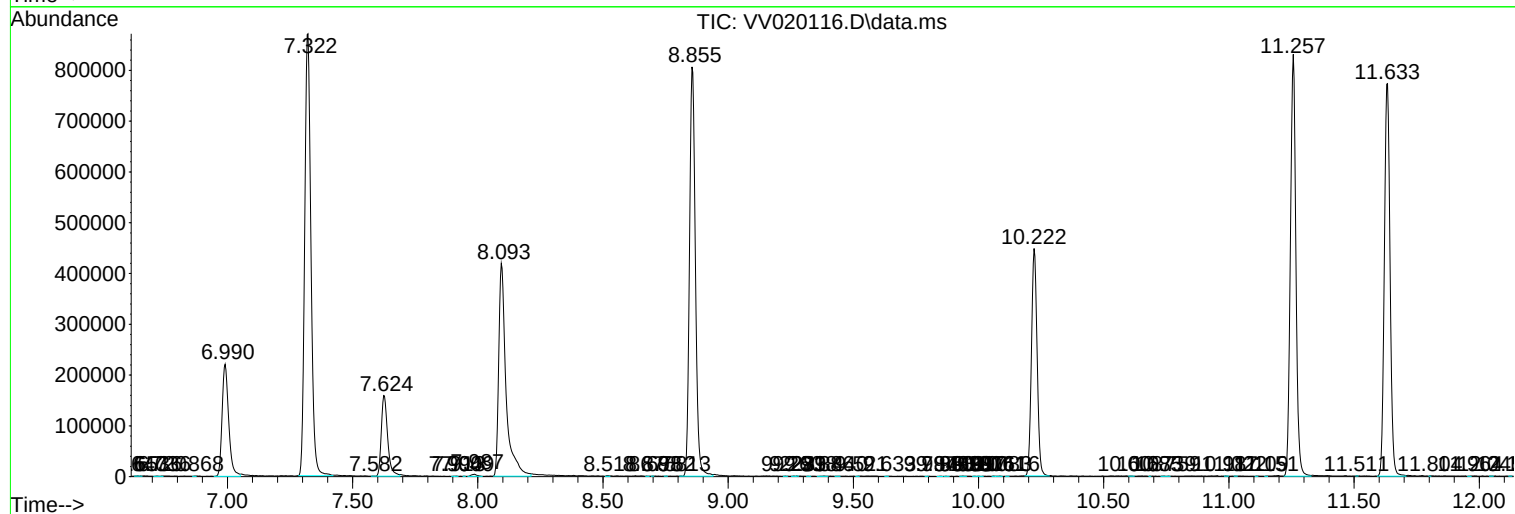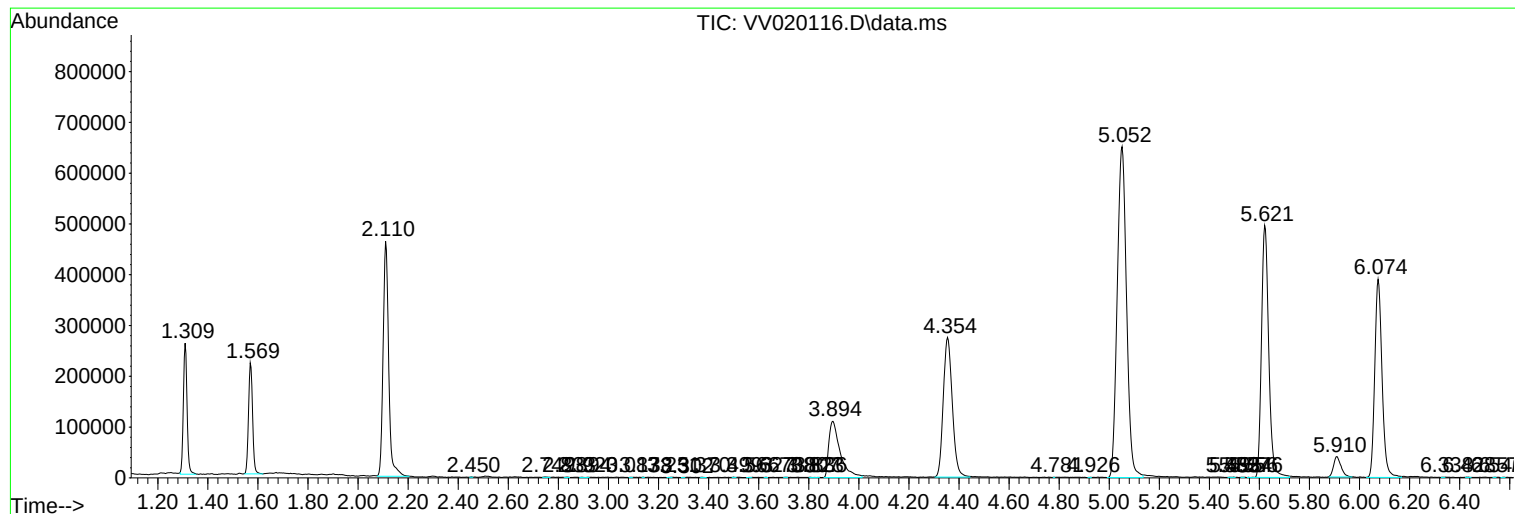

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020116.D
Acq On : 21 Jan 2021 20:04
Operator : SY/MD
Sample : VIBLK36
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020116.D
Acq On : 21 Jan 2021 20:04
Operator : SY/MD
Sample : VIBLK36
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
