

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020117.D
 Acq On : 21 Jan 2021 20:27
 Operator : SY/MD
 Sample : M1199-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020117.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	83	rVB	255679	263816	15.59%	1.954%
2	1.569	142	149	164	rVB	217911	245781	14.52%	1.820%
3	2.110	307	317	346	rVB	472412	709631	41.92%	5.255%
4	2.765	519	521	525	rBV3	538	292	0.02%	0.002%
5	2.859	546	550	551	rBV3	437	299	0.02%	0.002%
6	2.872	552	554	557	rVV2	937	455	0.03%	0.003%
7	2.913	566	567	569	rBV2	575	286	0.02%	0.002%
8	2.946	575	577	578	rBV	382	103	0.01%	0.001%
9	2.962	578	582	584	rVV3	683	381	0.02%	0.003%
10	3.074	615	617	620	rBV3	393	282	0.02%	0.002%
11	3.251	669	672	673	rBV2	460	243	0.01%	0.002%
12	3.351	700	703	704	rBV2	471	284	0.02%	0.002%
13	3.460	736	737	738	rBV	443	107	0.01%	0.001%
14	3.534	756	760	767	rVB5	666	884	0.05%	0.007%
15	3.569	768	771	772	rBV3	358	187	0.01%	0.001%
16	3.637	791	792	794	rVB3	389	88	0.01%	0.001%
17	3.656	796	798	800	rBV2	663	390	0.02%	0.003%
18	3.765	830	832	833	rBV2	226	85	0.01%	0.001%
19	3.897	862	873	909	rBV	110214	342707	20.25%	2.538%
20	4.354	999	1015	1037	rBV	271701	669944	39.58%	4.961%
21	4.679	1114	1116	1118	rBV3	812	348	0.02%	0.003%
22	4.830	1161	1163	1165	rBV3	791	442	0.03%	0.003%
23	4.862	1170	1173	1176	rBV4	1307	902	0.05%	0.007%
24	4.884	1179	1180	1183	rBV2	394	233	0.01%	0.002%
25	5.052	1212	1232	1261	rBV2	653654	1692751	100.00%	12.536%
26	5.482	1363	1366	1368	rBV4	1328	817	0.05%	0.006%
27	5.543	1383	1385	1387	rBV2	618	310	0.02%	0.002%
28	5.621	1397	1409	1436	rBV	513641	1027112	60.68%	7.607%
29	5.907	1486	1498	1514	rBV2	54558	111794	6.60%	0.828%
30	6.074	1537	1550	1583	rBV2	381247	785107	46.38%	5.814%
31	6.334	1629	1631	1634	rBV3	436	254	0.02%	0.002%
32	6.351	1634	1636	1639	rVB	593	278	0.02%	0.002%
33	6.367	1639	1641	1645	rBV2	324	271	0.02%	0.002%
34	6.386	1645	1647	1649	rBV2	396	207	0.01%	0.002%
35	6.437	1661	1663	1667	rVB3	516	268	0.02%	0.002%
36	6.460	1667	1670	1672	rBV2	669	420	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012121\
 Data File : VW020117.D
 Acq On : 21 Jan 2021 20:27
 Operator : SY/MD
 Sample : M1199-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	6.492	1678	1680	1682	rBV2	473	255	0.02%	0.002%
38	6.547	1695	1697	1699	rBV	400	185	0.01%	0.001%
39	6.556	1699	1700	1703	rVB	578	185	0.01%	0.001%
40	6.576	1703	1706	1708	rBV	492	279	0.02%	0.002%
41	6.588	1708	1710	1711	rBV	217	62	0.00%	0.000%
42	6.698	1742	1744	1746	rBV2	220	123	0.01%	0.001%
43	6.746	1756	1759	1765	rVB2	144	108	0.01%	0.001%
44	6.781	1767	1770	1773	rBV2	246	158	0.01%	0.001%
45	6.836	1780	1787	1789	rBV2	206	183	0.01%	0.001%
46	6.859	1792	1794	1795	rVV2	103	25	0.00%	0.000%
47	6.907	1807	1809	1811	rVB2	175	73	0.00%	0.001%
48	6.923	1812	1814	1820	rVB2	234	168	0.01%	0.001%
49	6.990	1824	1835	1861	rBV	215769	389023	22.98%	2.881%
50	7.277	1920	1924	1925	rBV2	361	234	0.01%	0.002%
51	7.322	1925	1938	1963	rBV	871654	1509554	89.18%	11.179%
52	7.588	2019	2021	2022	rBV	462	229	0.01%	0.002%
53	7.627	2022	2033	2064	rVV	155699	276605	16.34%	2.048%
54	7.894	2114	2116	2119	rBV2	357	169	0.01%	0.001%
55	7.936	2127	2129	2135	rVB4	548	411	0.02%	0.003%
56	7.984	2137	2144	2151	rBV6	2406	3705	0.22%	0.027%
57	8.042	2158	2162	2167	rBV4	682	560	0.03%	0.004%
58	8.096	2167	2179	2217	rBV2	374112	797707	47.12%	5.908%
59	8.588	2329	2332	2335	rBV5	923	721	0.04%	0.005%
60	8.649	2349	2351	2354	rBV	603	360	0.02%	0.003%
61	8.768	2386	2388	2390	rBV2	622	314	0.02%	0.002%
62	8.858	2404	2416	2438	rBV	783725	1278936	75.55%	9.472%
63	9.219	2526	2528	2531	rVB	748	346	0.02%	0.003%
64	9.257	2538	2540	2545	rBV4	686	538	0.03%	0.004%
65	9.289	2549	2550	2552	rVB	846	202	0.01%	0.001%
66	9.305	2552	2555	2559	rBV4	762	611	0.04%	0.005%
67	9.354	2567	2570	2573	rVB2	616	345	0.02%	0.003%
68	9.370	2573	2575	2577	rBV2	312	114	0.01%	0.001%
69	9.379	2577	2578	2581	rVB2	321	146	0.01%	0.001%
70	9.440	2593	2597	2600	rBV3	464	441	0.03%	0.003%
71	9.479	2607	2609	2611	rVB2	279	101	0.01%	0.001%
72	9.592	2640	2644	2645	rBV	390	237	0.01%	0.002%
73	9.601	2645	2647	2652	rVB	404	253	0.01%	0.002%
74	9.704	2677	2679	2682	rVB3	472	153	0.01%	0.001%
75	9.778	2698	2702	2703	rBV	603	387	0.02%	0.003%
76	9.865	2726	2729	2732	rBV2	419	370	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020117.D
 Acq On : 21 Jan 2021 20:27
 Operator : SY/MD
 Sample : M1199-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E77

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

77	9.907	2740	2742	2746	rBV4	444	334	0.02%	0.002%
78	10.032	2779	2781	2782	rBV2	532	238	0.01%	0.002%
79	10.064	2788	2791	2793	rBV2	680	383	0.02%	0.003%
80	10.222	2828	2840	2857	rBV	424292	667682	39.44%	4.945%
81	10.579	2949	2951	2956	rBV3	527	527	0.03%	0.004%
82	10.727	2995	2997	2998	rBV	492	157	0.01%	0.001%
83	10.887	3046	3047	3048	rBV	259	76	0.00%	0.001%
84	10.952	3065	3067	3070	rBV2	502	282	0.02%	0.002%
85	11.122	3118	3120	3125	rBV4	397	330	0.02%	0.002%
86	11.257	3149	3162	3182	rBV	834054	1302151	76.93%	9.644%
87	11.473	3225	3229	3230	rBV	198	124	0.01%	0.001%
88	11.630	3266	3278	3307	rBV	899469	1407305	83.14%	10.422%
89	12.559	3565	3567	3568	rBV	412	139	0.01%	0.001%
90	13.759	3937	3940	3943	rBV5	1340	818	0.05%	0.006%




Sum of corrected areas: 13502881

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020117.D
Acq On : 21 Jan 2021 20:27
Operator : SY/MD
Sample : M1199-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

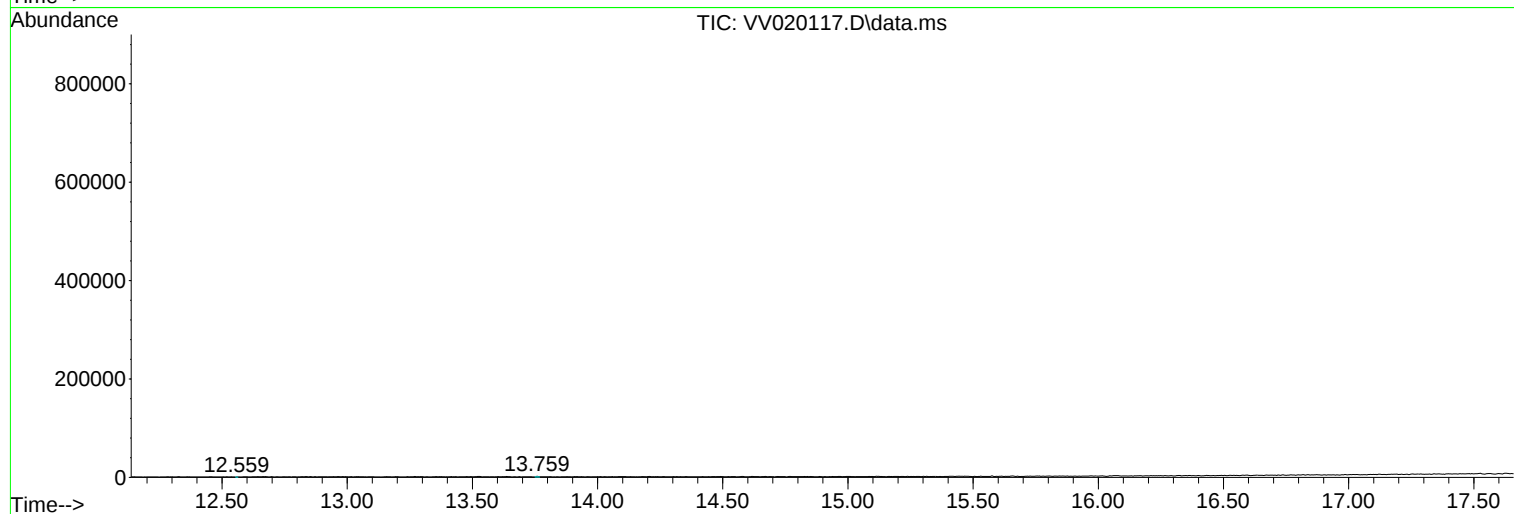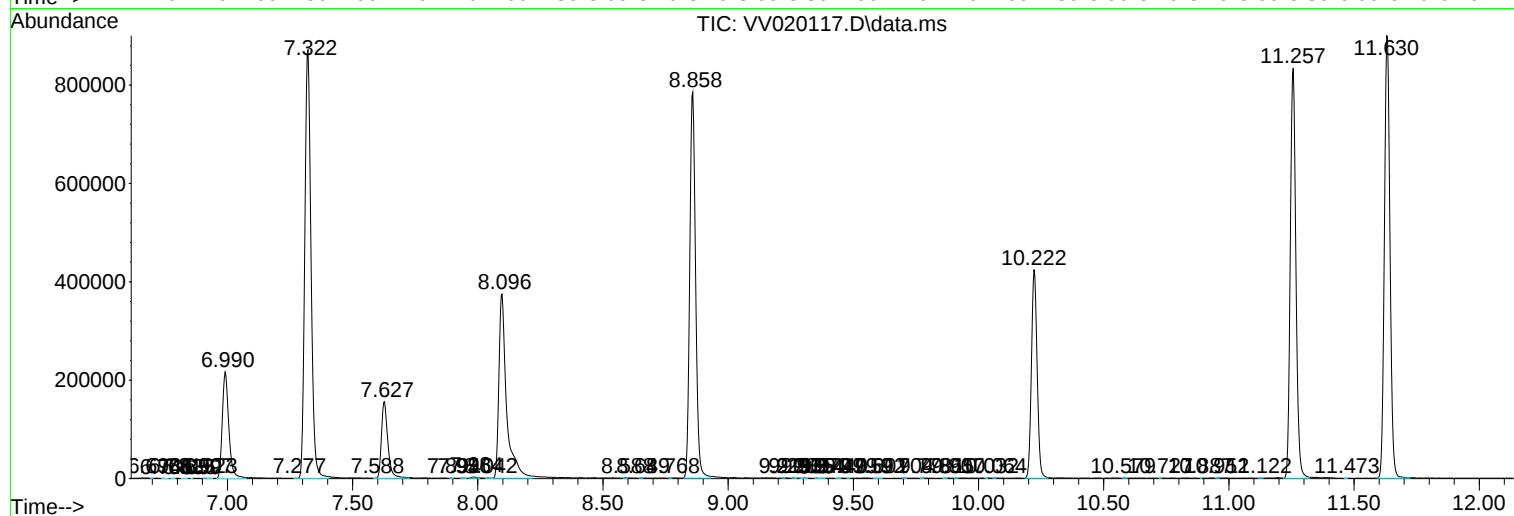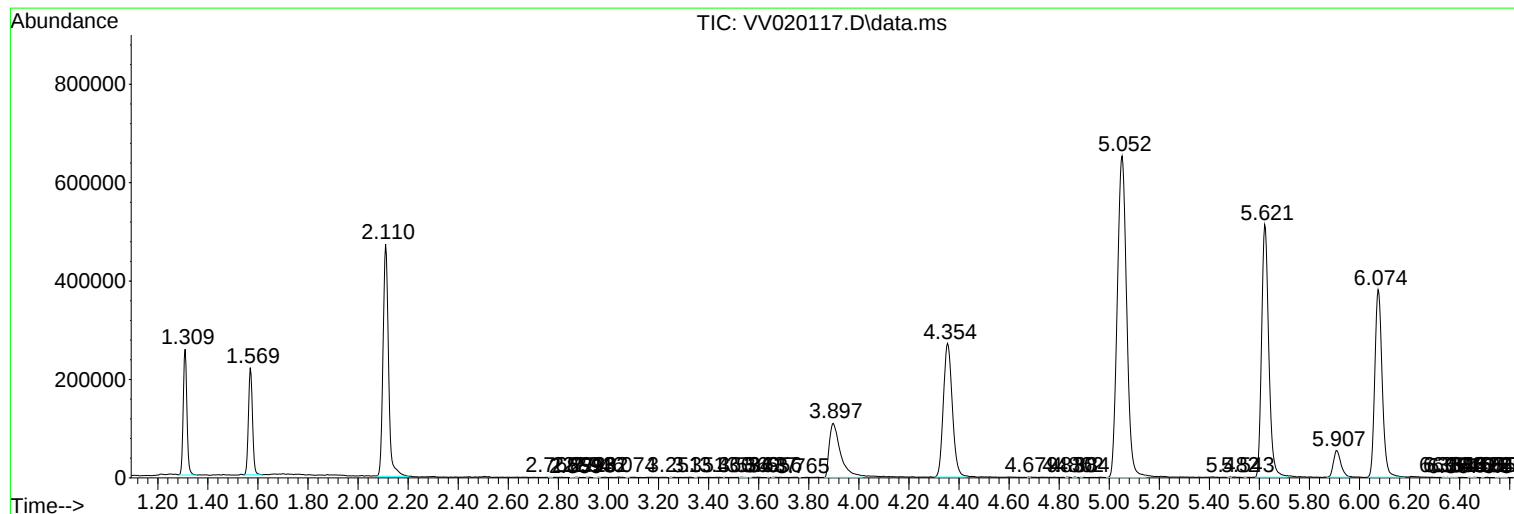

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020117.D
Acq On : 21 Jan 2021 20:27
Operator : SY/MD
Sample : M1199-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020117.D
Acq On : 21 Jan 2021 20:27
Operator : SY/MD
Sample : M1199-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
