

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020118.D
 Acq On : 21 Jan 2021 20:51
 Operator : SY/MD
 Sample : M1199-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	80	rVB	247390	251263	13.47%	1.775%
2	1.570	142	149	161	rVB	193119	220493	11.82%	1.557%
3	2.110	307	317	347	rVB	415092	624852	33.50%	4.414%
4	2.656	482	487	488	rBV2	285	198	0.01%	0.001%
5	2.717	501	506	515	rBV4	485	697	0.04%	0.005%
6	2.759	515	519	522	rBV4	528	457	0.02%	0.003%
7	2.804	529	533	540	rBV2	383	471	0.03%	0.003%
8	2.836	541	543	544	rBV2	166	53	0.00%	0.000%
9	2.888	556	559	561	rBV2	329	175	0.01%	0.001%
10	2.962	580	582	583	rVB2	207	61	0.00%	0.000%
11	3.052	605	610	615	rBV3	272	340	0.02%	0.002%
12	3.071	615	616	617	rVV3	165	41	0.00%	0.000%
13	3.081	617	619	621	rVV	254	163	0.01%	0.001%
14	3.103	623	626	629	rVV2	295	202	0.01%	0.001%
15	3.119	629	631	635	rVV	253	138	0.01%	0.001%
16	3.190	650	653	657	rVB3	378	226	0.01%	0.002%
17	3.373	708	710	712	rBV2	153	43	0.00%	0.000%
18	3.399	712	718	719	rBV2	280	213	0.01%	0.002%
19	3.428	725	727	730	rBV	304	156	0.01%	0.001%
20	3.492	744	747	751	rBV	311	252	0.01%	0.002%
21	3.528	756	758	761	rVB	297	150	0.01%	0.001%
22	3.602	777	781	783	rBV2	286	205	0.01%	0.001%
23	3.614	783	785	788	rVB	434	237	0.01%	0.002%
24	3.647	793	795	798	rBV	169	110	0.01%	0.001%
25	3.701	807	812	815	rBV3	229	209	0.01%	0.001%
26	3.798	840	842	846	rBV	198	72	0.00%	0.001%
27	3.849	856	858	861	rBV	191	131	0.01%	0.001%
28	3.894	861	872	912	rBV	120618	368783	19.77%	2.605%
29	4.354	998	1015	1051	rBV	300425	737092	39.52%	5.206%
30	4.856	1169	1171	1173	rBV	232	132	0.01%	0.001%
31	5.052	1214	1232	1271	rBV2	725382	1864998	100.00%	13.173%
32	5.370	1328	1331	1336	rBV3	539	598	0.03%	0.004%
33	5.425	1345	1348	1349	rBV2	350	158	0.01%	0.001%
34	5.438	1349	1352	1357	rVB4	581	417	0.02%	0.003%
35	5.463	1357	1360	1363	rBV2	335	253	0.01%	0.002%
36	5.499	1368	1371	1374	rBV3	1078	844	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020118.D
 Acq On : 21 Jan 2021 20:51
 Operator : SY/MD
 Sample : M1199-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	5.534	1380	1382	1383	rBV3	161	54	0.00%	0.000%
38	5.544	1383	1385	1387	rVB2	265	130	0.01%	0.001%
39	5.621	1396	1409	1441	rBV	574615	1151402	61.74%	8.133%
40	5.852	1478	1481	1485	rBV3	623	430	0.02%	0.003%
41	5.910	1487	1499	1519	rVV	55234	115520	6.19%	0.816%
42	6.074	1535	1550	1578	rBV	420667	846814	45.41%	5.981%
43	6.251	1603	1605	1608	rBV4	668	354	0.02%	0.003%
44	6.370	1639	1642	1646	rBV2	441	293	0.02%	0.002%
45	6.611	1711	1717	1719	rBV	283	292	0.02%	0.002%
46	6.646	1723	1728	1733	rBV6	723	999	0.05%	0.007%
47	6.753	1759	1761	1764	rVB2	452	208	0.01%	0.001%
48	6.772	1764	1767	1770	rVB	282	193	0.01%	0.001%
49	6.817	1779	1781	1783	rVB	262	79	0.00%	0.001%
50	6.939	1816	1819	1823	rBV2	308	244	0.01%	0.002%
51	6.990	1823	1835	1866	rBV	221533	406155	21.78%	2.869%
52	7.318	1925	1937	1954	rBV	864560	1493470	80.08%	10.549%
53	7.627	2022	2033	2054	rBV	151044	264488	14.18%	1.868%
54	7.836	2096	2098	2100	rBV	340	149	0.01%	0.001%
55	7.891	2112	2115	2116	rBV	340	199	0.01%	0.001%
56	7.984	2139	2144	2152	rVB5	2067	2467	0.13%	0.017%
57	8.045	2159	2163	2167	rBV3	266	353	0.02%	0.002%
58	8.093	2168	2178	2210	rBV2	385697	820525	44.00%	5.796%
59	8.717	2369	2372	2373	rBV2	421	181	0.01%	0.001%
60	8.775	2388	2390	2393	rBV	425	277	0.01%	0.002%
61	8.855	2403	2415	2435	rBV	874169	1424960	76.41%	10.065%
62	9.116	2493	2496	2497	rBV2	552	321	0.02%	0.002%
63	9.158	2501	2509	2514	rBV3	2078	2687	0.14%	0.019%
64	9.412	2586	2588	2590	rBV2	285	139	0.01%	0.001%
65	9.460	2601	2603	2609	rVB2	478	327	0.02%	0.002%
66	9.502	2611	2616	2617	rBV	424	339	0.02%	0.002%
67	9.560	2629	2634	2635	rBV4	1363	936	0.05%	0.007%
68	9.836	2718	2720	2723	rBV	422	270	0.01%	0.002%
69	9.884	2732	2735	2738	rBV	324	229	0.01%	0.002%
70	10.013	2773	2775	2777	rBV	214	111	0.01%	0.001%
71	10.138	2810	2814	2818	rBV2	288	291	0.02%	0.002%
72	10.222	2827	2840	2863	rBV	477020	758147	40.65%	5.355%
73	10.386	2888	2891	2893	rBV2	622	477	0.03%	0.003%
74	10.849	3031	3035	3038	rBV2	413	358	0.02%	0.003%
75	11.029	3086	3091	3094	rBV2	528	472	0.03%	0.003%
76	11.257	3150	3162	3180	rBV	890922	1377718	73.87%	9.731%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020118.D
Acq On : 21 Jan 2021 20:51
Operator : SY/MD
Sample : M1199-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E90

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Title : VOC Analysis

77	11.633	3266	3279	3299	rBV	886076	1406702	75.43%	9.936%
78	12.074	3413	3416	3419	rBV3	446	292	0.02%	0.002%
79	12.244	3465	3469	3472	rBV3	635	534	0.03%	0.004%
80	13.116	3737	3740	3747	rBV3	1134	968	0.05%	0.007%
81	15.180	4379	4382	4389	rBV4	1259	1282	0.07%	0.009%




Sum of corrected areas: 14157719

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020118.D
Acq On : 21 Jan 2021 20:51
Operator : SY/MD
Sample : M1199-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

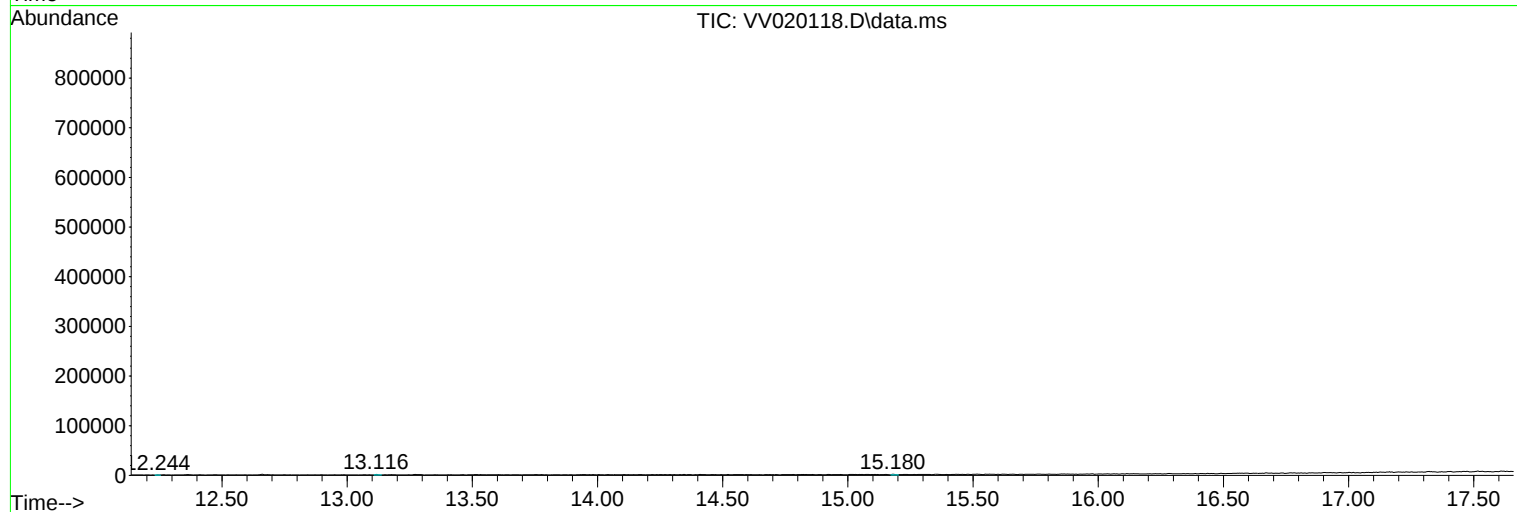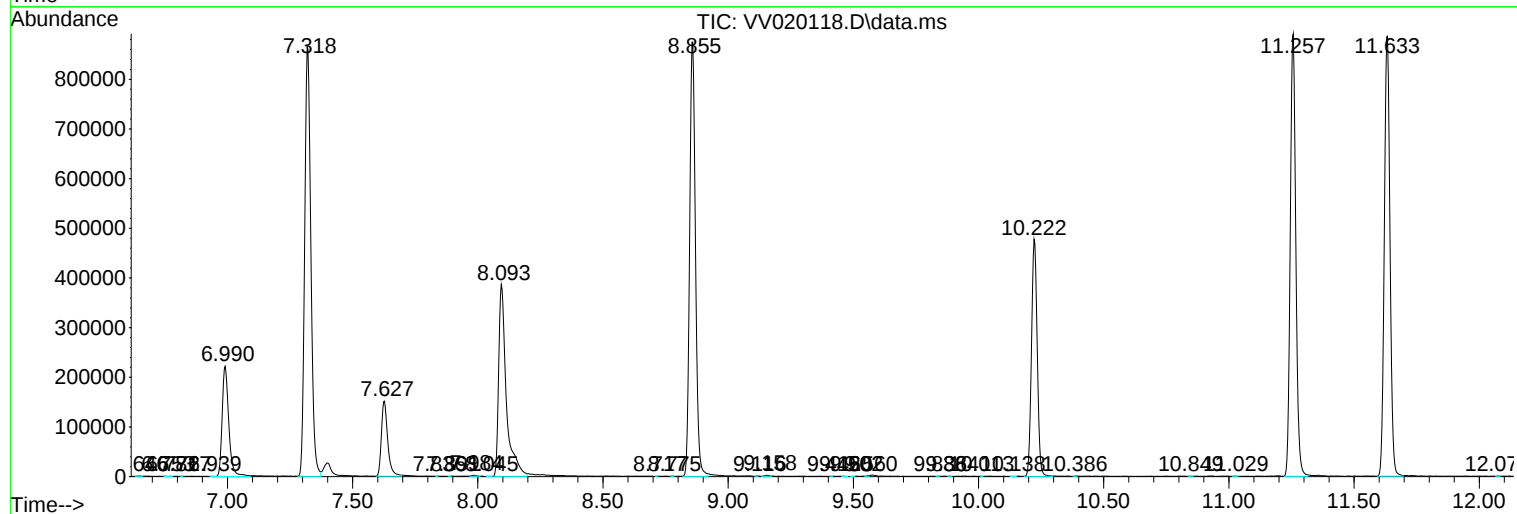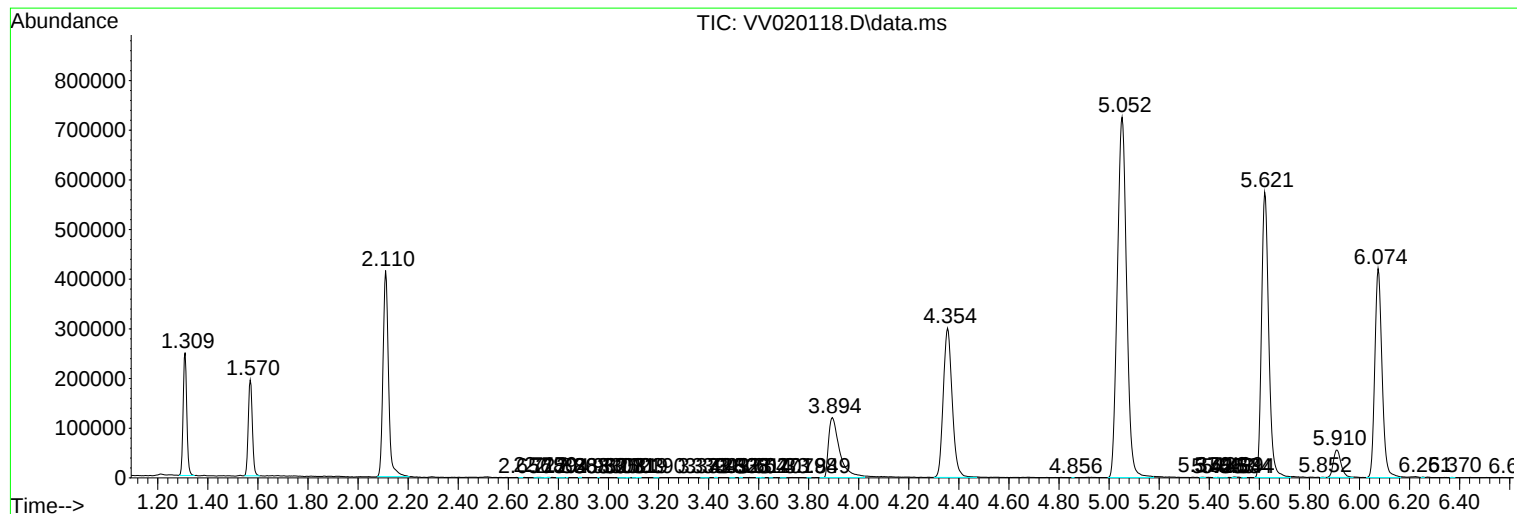

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020118.D
Acq On : 21 Jan 2021 20:51
Operator : SY/MD
Sample : M1199-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020118.D
Acq On : 21 Jan 2021 20:51
Operator : SY/MD
Sample : M1199-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
