

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020121.D
 Acq On : 21 Jan 2021 22:02
 Operator : SY/MD
 Sample : M1181-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020121.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	61	69	86	rBV	2884904	2901460	2.46%	1.641%
2	1.570	142	149	161	rVB	219196	245031	0.21%	0.139%
3	2.110	307	317	344	rVB2	479666	768580	0.65%	0.435%
4	2.666	488	490	494	rBV2	799	505	0.00%	0.000%
5	2.766	508	521	549	rBV2	341208	633431	0.54%	0.358%
6	2.965	580	583	585	rBV4	524	334	0.00%	0.000%
7	3.116	628	630	631	rBV	343	154	0.00%	0.000%
8	3.132	631	635	638	rVB3	511	413	0.00%	0.000%
9	3.190	645	653	655	rBV6	4684	5663	0.00%	0.003%
10	3.325	692	695	700	rVB3	694	475	0.00%	0.000%
11	3.357	704	705	708	rVV2	357	140	0.00%	0.000%
12	3.373	708	710	717	rVB3	859	671	0.00%	0.000%
13	3.409	717	721	722	rBV2	460	354	0.00%	0.000%
14	3.438	728	730	733	rBV2	604	334	0.00%	0.000%
15	3.486	742	745	747	rBV2	493	270	0.00%	0.000%
16	3.541	759	762	766	rVB2	653	609	0.00%	0.000%
17	3.563	766	769	770	rBV	436	183	0.00%	0.000%
18	3.586	773	776	778	rBV3	431	262	0.00%	0.000%
19	3.627	787	789	795	rVB4	966	871	0.00%	0.000%
20	3.659	797	799	802	rBV	487	234	0.00%	0.000%
21	3.676	802	804	805	rBV	373	175	0.00%	0.000%
22	3.692	805	809	813	rVB3	806	577	0.00%	0.000%
23	3.711	813	815	817	rBV3	566	229	0.00%	0.000%
24	3.743	824	825	828	rBV3	539	316	0.00%	0.000%
25	3.766	829	832	834	rBV4	1001	683	0.00%	0.000%
26	3.920	858	880	953	rBV3	46762773	117739142	100.00%	66.602%
27	4.354	1003	1015	1039	rVB	268453	659306	0.56%	0.373%
28	5.052	1214	1232	1268	rBV2	697659	1889317	1.60%	1.069%
29	5.441	1350	1353	1355	rBV2	872	559	0.00%	0.000%
30	5.524	1377	1379	1382	rVB3	796	384	0.00%	0.000%
31	5.621	1395	1409	1437	rBV	504807	1026693	0.87%	0.581%
32	5.920	1485	1502	1534	rBV	11002750	20258801	17.21%	11.460%
33	6.074	1540	1550	1577	rVB	402925	796533	0.68%	0.451%
34	6.621	1718	1720	1721	rBV	546	239	0.00%	0.000%
35	6.875	1797	1799	1803	rBV3	623	315	0.00%	0.000%
36	6.913	1808	1811	1812	rBV2	406	191	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012121\
 Data File : VW020121.D
 Acq On : 21 Jan 2021 22:02
 Operator : SY/MD
 Sample : M1181-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

37	6.991	1823	1835	1855	rBV	232871	417491	0.35%	0.236%
38	7.318	1926	1937	1953	rBV	866097	1488445	1.26%	0.842%
39	7.624	2022	2032	2055	rBV	162064	279432	0.24%	0.158%
40	7.855	2096	2104	2110	rBV7	2022	3278	0.00%	0.002%
41	7.981	2127	2143	2167	rBV	13478721	22221036	18.87%	12.570%
42	8.093	2169	2178	2215	rVB2	440093	848602	0.72%	0.480%
43	8.855	2404	2415	2441	rBV	872366	1434405	1.22%	0.811%
44	9.286	2547	2549	2551	rVB3	903	335	0.00%	0.000%
45	9.309	2553	2556	2561	rBV3	815	729	0.00%	0.000%
46	9.524	2620	2623	2625	rBV2	527	332	0.00%	0.000%
47	9.746	2689	2692	2694	rBV3	604	441	0.00%	0.000%
48	9.997	2767	2770	2774	rVB5	759	530	0.00%	0.000%
49	10.084	2791	2797	2801	rBV6	1018	1402	0.00%	0.001%
50	10.135	2811	2813	2814	rBV2	319	131	0.00%	0.000%
51	10.222	2828	2840	2856	rBV	474221	741159	0.63%	0.419%
52	10.347	2877	2879	2881	rBV2	998	485	0.00%	0.000%
53	10.460	2912	2914	2916	rVB	564	223	0.00%	0.000%
54	10.498	2920	2926	2928	rBV4	627	571	0.00%	0.000%
55	10.543	2938	2940	2942	rBV	615	344	0.00%	0.000%
56	10.646	2969	2972	2975	rBV3	935	552	0.00%	0.000%
57	10.720	2993	2995	2997	rBV	676	275	0.00%	0.000%
58	10.942	3063	3064	3067	rBV3	432	136	0.00%	0.000%
59	11.000	3079	3082	3083	rBV3	604	305	0.00%	0.000%
60	11.042	3091	3095	3097	rBV5	687	522	0.00%	0.000%
61	11.135	3122	3124	3126	rVB2	688	251	0.00%	0.000%
62	11.254	3150	3161	3183	rBV	770617	1190667	1.01%	0.674%
63	11.630	3266	3278	3300	rBV	763673	1211670	1.03%	0.685%
64	11.830	3338	3340	3343	rBV2	588	310	0.00%	0.000%
65	12.003	3391	3394	3400	rBV4	851	899	0.00%	0.001%
66	12.141	3434	3437	3439	rBV2	601	441	0.00%	0.000%
67	12.621	3585	3586	3587	rBV2	358	110	0.00%	0.000%
68	12.643	3591	3593	3594	rBV2	692	319	0.00%	0.000%
69	13.267	3784	3787	3788	rBV3	777	507	0.00%	0.000%
70	13.354	3810	3814	3817	rBV3	863	914	0.00%	0.001%
71	13.649	3904	3906	3908	rBV2	476	189	0.00%	0.000%
72	14.067	4032	4036	4038	rBV3	861	609	0.00%	0.000%




Sum of corrected areas: 176781481

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020121.D
Acq On : 21 Jan 2021 22:02
Operator : SY/MD
Sample : M1181-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

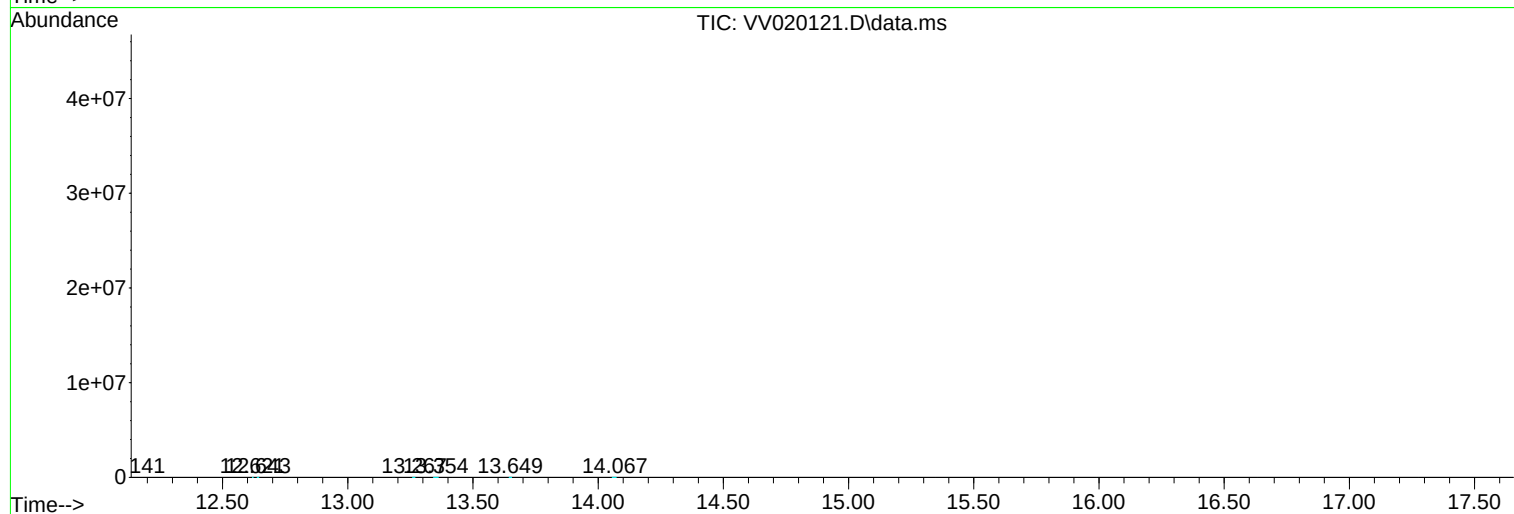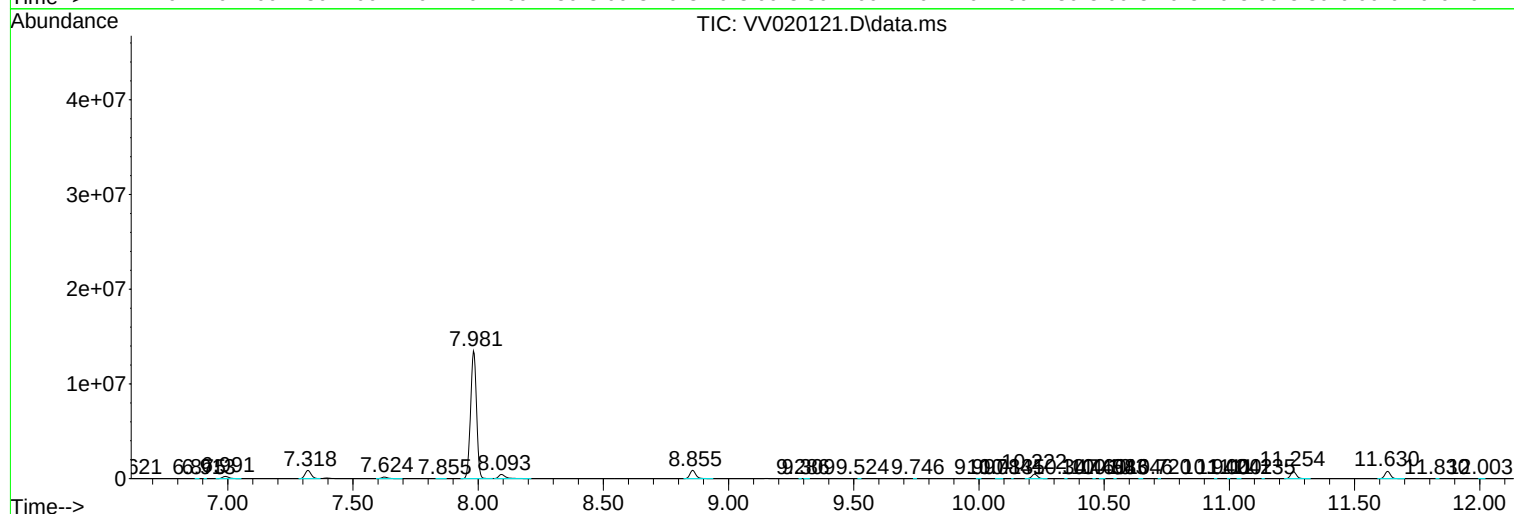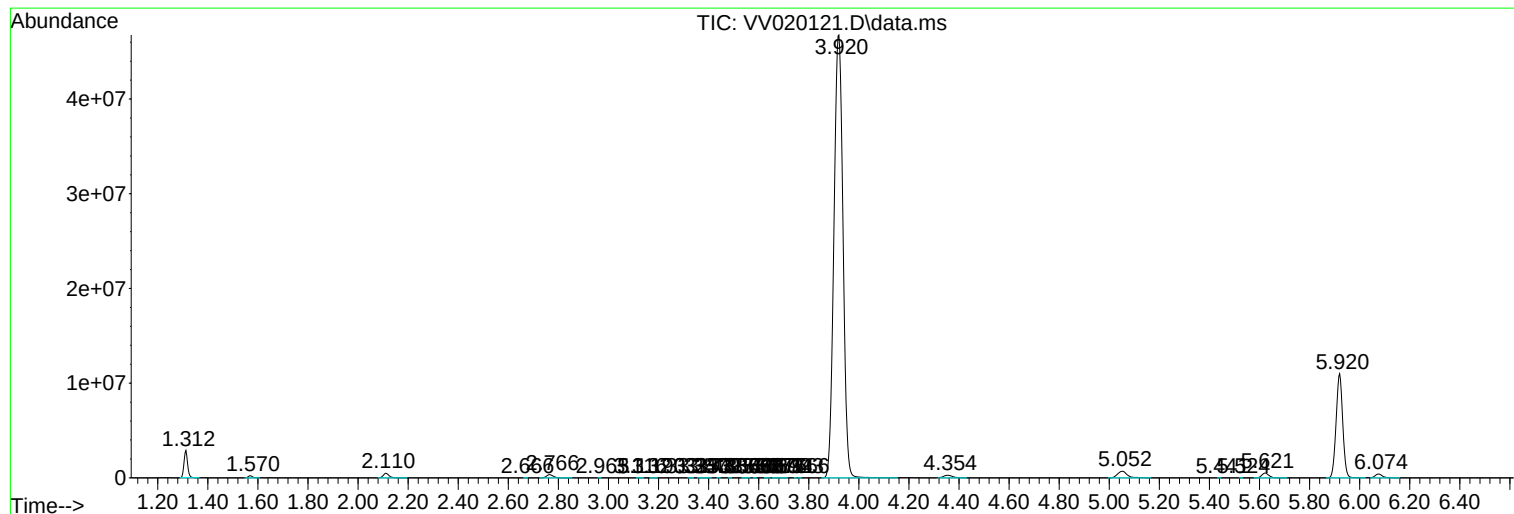

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020121.D
Acq On : 21 Jan 2021 22:02
Operator : SY/MD
Sample : M1181-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020121.D
Acq On : 21 Jan 2021 22:02
Operator : SY/MD
Sample : M1181-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
