

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020122.D
 Acq On : 21 Jan 2021 22:25
 Operator : SY/MD
 Sample : M1181-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020122.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	81	rVB	270164	280545	16.67%	1.911%
2	1.569	142	149	160	rBV	226244	251297	14.93%	1.712%
3	2.110	307	317	357	rVB	463861	714476	42.45%	4.867%
4	2.772	512	523	524	rBV5	3443	4691	0.28%	0.032%
5	2.836	540	543	548	rVB4	820	613	0.04%	0.004%
6	2.939	570	575	578	rBV4	550	525	0.03%	0.004%
7	2.997	590	593	594	rBV2	490	336	0.02%	0.002%
8	3.167	643	646	647	rBV2	518	314	0.02%	0.002%
9	3.212	658	660	664	rVB3	481	304	0.02%	0.002%
10	3.232	664	666	669	rBV2	619	372	0.02%	0.003%
11	3.328	695	696	699	rBV3	527	255	0.02%	0.002%
12	3.431	726	728	733	rVB2	699	466	0.03%	0.003%
13	3.460	733	737	738	rBV3	712	494	0.03%	0.003%
14	3.518	753	755	758	rVB2	903	501	0.03%	0.003%
15	3.547	758	764	766	rBV4	782	818	0.05%	0.006%
16	3.650	794	796	799	rVB4	576	293	0.02%	0.002%
17	3.663	799	800	806	rVB3	397	275	0.02%	0.002%
18	3.910	861	877	906	rBV3	189519	620040	36.84%	4.224%
19	4.354	1000	1015	1046	rVB	272395	678719	40.33%	4.624%
20	4.505	1060	1062	1066	rBV4	582	459	0.03%	0.003%
21	4.759	1140	1141	1146	rVB3	568	333	0.02%	0.002%
22	4.910	1185	1188	1191	rBV3	691	474	0.03%	0.003%
23	4.949	1198	1200	1203	rVB2	641	344	0.02%	0.002%
24	4.965	1203	1205	1206	rBV2	571	291	0.02%	0.002%
25	5.052	1214	1232	1258	rBV2	655355	1683043	100.00%	11.466%
26	5.454	1355	1357	1361	rVB3	604	311	0.02%	0.002%
27	5.489	1366	1368	1370	rBV2	763	471	0.03%	0.003%
28	5.518	1375	1377	1380	rBV3	784	428	0.03%	0.003%
29	5.544	1381	1385	1388	rBV4	505	470	0.03%	0.003%
30	5.621	1397	1409	1438	rBV	499888	998655	59.34%	6.803%
31	5.849	1478	1480	1481	rBV2	867	420	0.02%	0.003%
32	5.920	1489	1502	1520	rBV4	89768	197440	11.73%	1.345%
33	6.074	1536	1550	1577	rBV	375905	767278	45.59%	5.227%
34	6.354	1635	1637	1640	rBV3	592	447	0.03%	0.003%
35	6.453	1666	1668	1670	rBV3	544	348	0.02%	0.002%
36	6.521	1686	1689	1693	rVV3	549	500	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020122.D
 Acq On : 21 Jan 2021 22:25
 Operator : SY/MD
 Sample : M1181-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	6.543	1693	1696	1699	rVV	672	414	0.02%	0.003%
38	6.572	1702	1705	1707	rVV2	588	273	0.02%	0.002%
39	6.798	1771	1775	1777	rBV2	665	438	0.03%	0.003%
40	6.830	1782	1785	1787	rBV3	391	272	0.02%	0.002%
41	6.881	1799	1801	1803	rVB	694	308	0.02%	0.002%
42	6.904	1803	1808	1813	rBV3	606	634	0.04%	0.004%
43	6.990	1822	1835	1855	rBV	201976	364678	21.67%	2.484%
44	7.322	1925	1938	1958	rBV	760457	1315224	78.15%	8.960%
45	7.627	2023	2033	2058	rBV	141051	246526	14.65%	1.679%
46	7.894	2114	2116	2119	rBV5	499	343	0.02%	0.002%
47	7.981	2130	2143	2165	rBV	839749	1409998	83.78%	9.606%
48	8.093	2168	2178	2211	rVV2	366105	716726	42.59%	4.883%
49	8.441	2284	2286	2289	rVB3	989	505	0.03%	0.003%
50	8.457	2289	2291	2297	rVB5	1034	767	0.05%	0.005%
51	8.495	2297	2303	2305	rBV5	909	933	0.06%	0.006%
52	8.627	2342	2344	2348	rBV3	500	364	0.02%	0.002%
53	8.675	2357	2359	2362	rVB4	489	293	0.02%	0.002%
54	8.717	2367	2372	2375	rBV4	524	489	0.03%	0.003%
55	8.804	2396	2399	2402	rBV3	626	486	0.03%	0.003%
56	8.859	2404	2416	2435	rBV	762793	1247953	74.15%	8.502%
57	9.100	2489	2491	2498	rVB7	684	773	0.05%	0.005%
58	9.212	2524	2526	2528	rBV3	620	257	0.02%	0.002%
59	9.286	2547	2549	2552	rBV3	516	324	0.02%	0.002%
60	9.479	2606	2609	2610	rBV2	822	345	0.02%	0.002%
61	9.521	2619	2622	2623	rBV	463	250	0.01%	0.002%
62	9.604	2644	2648	2651	rBV3	557	517	0.03%	0.004%
63	9.649	2659	2662	2664	rBV	452	297	0.02%	0.002%
64	9.801	2704	2709	2710	rBV2	437	358	0.02%	0.002%
65	9.894	2735	2738	2741	rBV4	572	374	0.02%	0.003%
66	9.920	2743	2746	2747	rBV	678	444	0.03%	0.003%
67	10.071	2790	2793	2799	rVB5	918	800	0.05%	0.005%
68	10.164	2817	2822	2823	rBV3	372	272	0.02%	0.002%
69	10.222	2828	2840	2866	rVV	450552	712122	42.31%	4.851%
70	10.312	2866	2868	2872	rVB3	731	360	0.02%	0.002%
71	10.357	2880	2882	2884	rVB3	816	263	0.02%	0.002%
72	10.392	2888	2893	2897	rBV4	935	1187	0.07%	0.008%
73	10.485	2918	2922	2924	rBV	678	564	0.03%	0.004%
74	10.547	2938	2941	2943	rBV3	791	464	0.03%	0.003%
75	10.714	2992	2993	2996	rBV	614	346	0.02%	0.002%
76	10.968	3070	3072	3077	rVB4	832	413	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020122.D
 Acq On : 21 Jan 2021 22:25
 Operator : SY/MD
 Sample : M1181-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

77	11.119	3117	3119	3124	rVB3	670	407	0.02%	0.003%
78	11.167	3132	3134	3139	rBV3	516	375	0.02%	0.003%
79	11.257	3150	3162	3183	rBV	792372	1228415	72.99%	8.369%
80	11.547	3250	3252	3253	rBV	631	251	0.01%	0.002%
81	11.633	3266	3279	3295	rBV	771707	1204775	71.58%	8.208%
82	11.781	3322	3325	3326	rBV2	489	322	0.02%	0.002%
83	12.074	3412	3416	3418	rBV4	995	641	0.04%	0.004%
84	12.251	3469	3471	3473	rVB2	582	253	0.02%	0.002%
85	12.267	3473	3476	3480	rBV2	395	356	0.02%	0.002%
86	12.350	3500	3502	3503	rBV	534	250	0.01%	0.002%
87	12.630	3584	3589	3594	rBV5	757	837	0.05%	0.006%
88	12.653	3594	3596	3597	rVV	880	274	0.02%	0.002%
89	12.736	3620	3622	3626	rBV4	653	536	0.03%	0.004%
90	12.804	3640	3643	3647	rBV4	568	469	0.03%	0.003%
91	12.826	3647	3650	3653	rVV4	1094	806	0.05%	0.005%
92	12.855	3657	3659	3662	rBV	701	334	0.02%	0.002%
93	13.196	3763	3765	3770	rVB4	857	396	0.02%	0.003%
94	13.395	3823	3827	3830	rBV3	788	652	0.04%	0.004%
95	13.431	3836	3838	3842	rVB3	997	603	0.04%	0.004%
96	13.672	3910	3913	3916	rBV3	591	488	0.03%	0.003%
97	13.688	3916	3918	3920	rVB2	1259	495	0.03%	0.003%
98	13.701	3920	3922	3924	rBV2	593	364	0.02%	0.002%
99	13.752	3936	3938	3940	rBV3	706	409	0.02%	0.003%
100	13.871	3970	3975	3978	rBV2	825	711	0.04%	0.005%




Sum of corrected areas: 14678819

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020121\
Data File : VV020122.D
Acq On : 21 Jan 2021 22:25
Operator : SY/MD
Sample : M1181-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

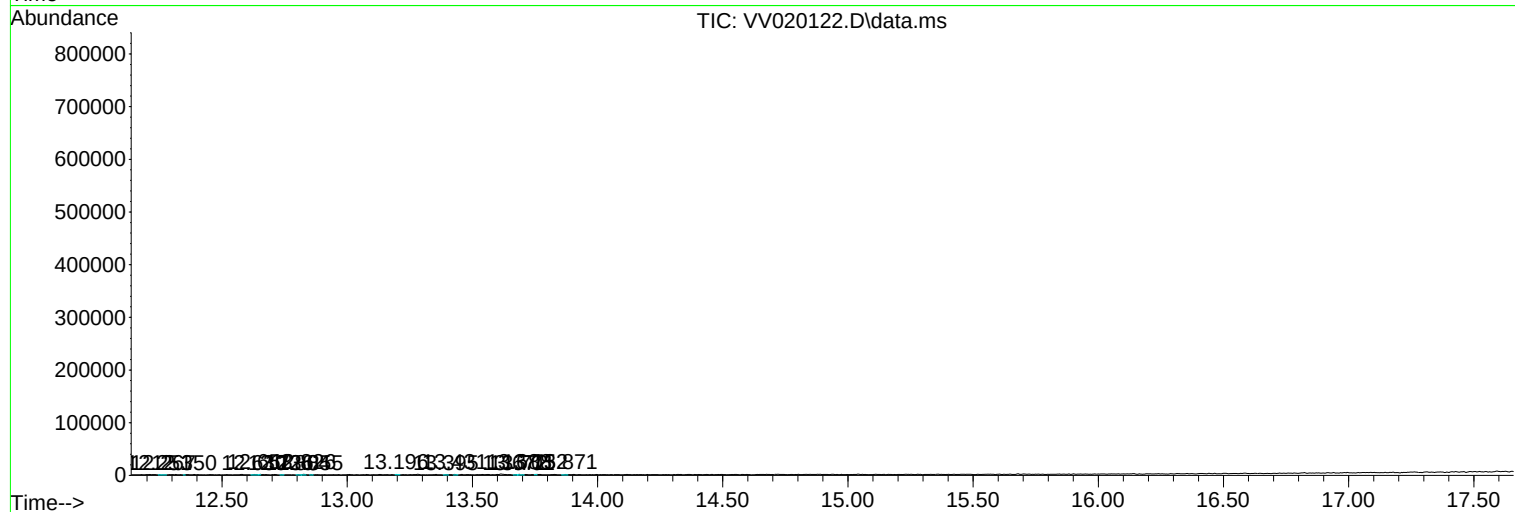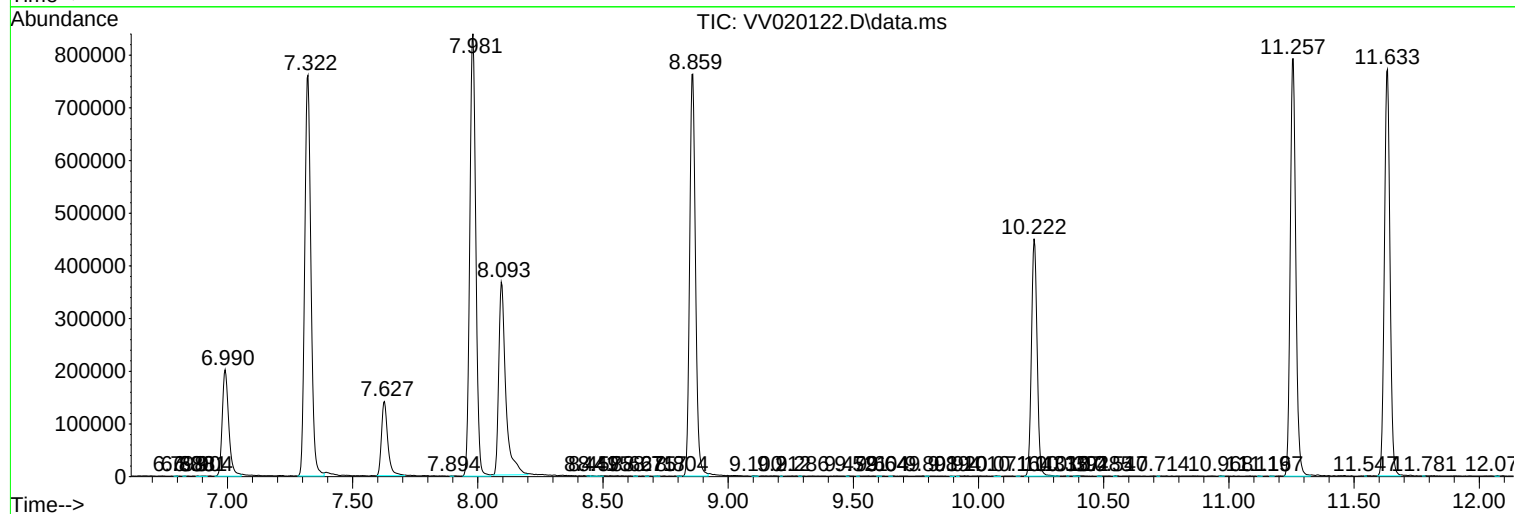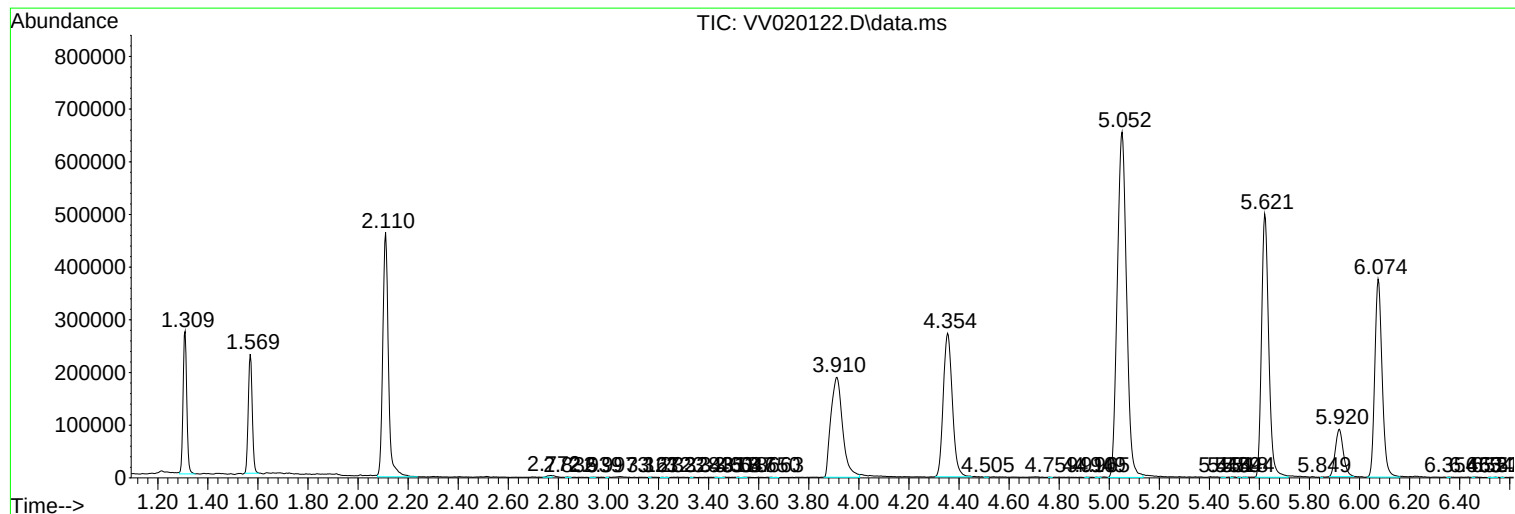

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020122.D
Acq On : 21 Jan 2021 22:25
Operator : SY/MD
Sample : M1181-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020122.D
Acq On : 21 Jan 2021 22:25
Operator : SY/MD
Sample : M1181-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------