

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020124.D
 Acq On : 21 Jan 2021 23:12
 Operator : SY/MD
 Sample : M1181-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	84	rVB	263160	260179	15.70%	1.875%
2	1.569	142	149	168	rBV	223514	251243	15.16%	1.811%
3	2.110	306	317	353	rBV	422376	646710	39.02%	4.661%
4	2.762	516	520	522	rBV4	1785	1483	0.09%	0.011%
5	3.093	621	623	625	rBV3	473	211	0.01%	0.002%
6	3.132	633	635	639	rVB4	523	238	0.01%	0.002%
7	3.232	664	666	668	rBV2	361	198	0.01%	0.001%
8	3.264	673	676	677	rBV2	718	317	0.02%	0.002%
9	3.273	677	679	683	rBV3	606	432	0.03%	0.003%
10	3.360	702	706	710	rVB4	768	670	0.04%	0.005%
11	3.386	712	714	717	rVV2	559	308	0.02%	0.002%
12	3.402	717	719	723	rVB3	748	342	0.02%	0.002%
13	3.470	738	740	742	rBV	340	188	0.01%	0.001%
14	3.605	779	782	785	rVB2	800	389	0.02%	0.003%
15	3.621	785	787	788	rBV	405	192	0.01%	0.001%
16	3.682	803	806	811	rBV3	625	512	0.03%	0.004%
17	3.711	811	815	818	rBV2	509	390	0.02%	0.003%
18	3.740	820	824	826	rBV2	501	266	0.02%	0.002%
19	3.833	849	853	855	rBV2	742	471	0.03%	0.003%
20	3.897	861	873	914	rBV3	118275	409784	24.72%	2.954%
21	4.354	1000	1015	1040	rBV	270290	664767	40.11%	4.792%
22	4.608	1092	1094	1098	rVB4	666	336	0.02%	0.002%
23	4.634	1100	1102	1105	rBV3	458	279	0.02%	0.002%
24	4.646	1105	1106	1107	rBV	542	112	0.01%	0.001%
25	4.682	1115	1117	1118	rBV	630	229	0.01%	0.002%
26	4.736	1132	1134	1138	rBV3	593	331	0.02%	0.002%
27	4.781	1146	1148	1150	rBV3	543	210	0.01%	0.002%
28	4.801	1151	1154	1157	rVB4	1129	617	0.04%	0.004%
29	4.817	1157	1159	1160	rBV2	803	357	0.02%	0.003%
30	4.897	1182	1184	1187	rVV4	491	281	0.02%	0.002%
31	5.052	1213	1232	1261	rBV2	646845	1657457	100.00%	11.947%
32	5.621	1397	1409	1433	rBV	475594	972533	58.68%	7.010%
33	5.916	1489	1501	1528	rVB6	54336	127105	7.67%	0.916%
34	6.074	1535	1550	1571	rBV	374241	764652	46.13%	5.512%
35	6.379	1641	1645	1647	rBV4	684	510	0.03%	0.004%
36	6.428	1658	1660	1664	rBV2	458	351	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020124.D
 Acq On : 21 Jan 2021 23:12
 Operator : SY/MD
 Sample : M1181-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	6.444	1664	1665	1668	rVV2	597	346	0.02%	0.002%
38	6.460	1668	1670	1672	rVV2	560	307	0.02%	0.002%
39	6.473	1672	1674	1681	rVB6	1168	1101	0.07%	0.008%
40	6.505	1681	1684	1688	rBV3	666	416	0.03%	0.003%
41	6.540	1693	1695	1696	rBV	375	146	0.01%	0.001%
42	6.592	1709	1711	1712	rBV	337	108	0.01%	0.001%
43	6.601	1712	1714	1716	rVB	426	148	0.01%	0.001%
44	6.617	1716	1719	1721	rBV2	597	421	0.03%	0.003%
45	6.717	1748	1750	1753	rVB3	702	215	0.01%	0.002%
46	6.756	1757	1762	1765	rVB3	847	549	0.03%	0.004%
47	6.923	1810	1814	1816	rBV2	659	444	0.03%	0.003%
48	6.990	1824	1835	1862	rBV	202688	369943	22.32%	2.667%
49	7.322	1925	1938	1968	rBV	837461	1448921	87.42%	10.444%
50	7.588	2020	2021	2022	rBV	554	195	0.01%	0.001%
51	7.627	2022	2033	2054	rVV	134805	241153	14.55%	1.738%
52	7.868	2106	2108	2112	rBV4	527	337	0.02%	0.002%
53	7.981	2126	2143	2158	rBV	449847	759456	45.82%	5.474%
54	8.093	2168	2178	2225	rBV2	373283	755214	45.56%	5.444%
55	8.598	2333	2335	2340	rVB3	750	355	0.02%	0.003%
56	8.630	2343	2345	2348	rVB3	461	162	0.01%	0.001%
57	8.653	2349	2352	2355	rBV2	788	530	0.03%	0.004%
58	8.858	2403	2416	2447	rBV	808007	1317395	79.48%	9.496%
59	9.222	2527	2529	2533	rVB3	848	494	0.03%	0.004%
60	9.238	2533	2534	2536	rBV2	586	259	0.02%	0.002%
61	9.363	2570	2573	2577	rVB4	606	382	0.02%	0.003%
62	9.383	2577	2579	2580	rBV	397	145	0.01%	0.001%
63	9.418	2588	2590	2593	rBV2	583	337	0.02%	0.002%
64	9.482	2608	2610	2614	rVB3	554	290	0.02%	0.002%
65	9.530	2617	2625	2630	rBV6	1022	1312	0.08%	0.009%
66	9.627	2649	2655	2657	rBV2	534	499	0.03%	0.004%
67	9.736	2684	2689	2691	rBV3	358	346	0.02%	0.002%
68	9.772	2697	2700	2702	rBV2	252	114	0.01%	0.001%
69	9.826	2712	2717	2719	rBV	269	266	0.02%	0.002%
70	9.948	2752	2755	2761	rVB2	443	343	0.02%	0.002%
71	9.977	2761	2764	2767	rBV2	268	228	0.01%	0.002%
72	10.010	2772	2774	2776	rBV	221	106	0.01%	0.001%
73	10.022	2776	2778	2781	rVB3	441	245	0.01%	0.002%
74	10.042	2781	2784	2786	rBV2	192	136	0.01%	0.001%
75	10.138	2812	2814	2817	rVB2	227	122	0.01%	0.001%
76	10.154	2817	2819	2824	rVB2	301	179	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020124.D
 Acq On : 21 Jan 2021 23:12
 Operator : SY/MD
 Sample : M1181-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

77	10.222	2826	2840	2863	rBV	498827	779875	47.05%	5.621%
78	10.495	2923	2925	2929	rVB	284	110	0.01%	0.001%
79	10.521	2929	2933	2935	rBV2	252	220	0.01%	0.002%
80	10.556	2942	2944	2948	rBB3	275	181	0.01%	0.001%
81	10.669	2977	2979	2982	rBV	280	188	0.01%	0.001%
82	10.701	2986	2989	2995	rVB2	368	314	0.02%	0.002%
83	10.733	2995	2999	3001	rBV2	476	304	0.02%	0.002%
84	10.807	3019	3022	3023	rBV2	285	146	0.01%	0.001%
85	10.878	3042	3044	3047	rVB2	365	158	0.01%	0.001%
86	11.010	3082	3085	3087	rBV3	380	278	0.02%	0.002%
87	11.038	3091	3094	3096	rBV2	679	450	0.03%	0.003%
88	11.257	3150	3162	3182	rBV	763108	1184364	71.46%	8.537%
89	11.633	3267	3279	3297	rBV	779252	1223248	73.80%	8.817%
90	11.823	3335	3338	3341	rBV	516	408	0.02%	0.003%
91	12.315	3489	3491	3492	rBV	456	151	0.01%	0.001%
92	12.646	3590	3594	3595	rBV2	420	266	0.02%	0.002%
93	12.926	3679	3681	3683	rBV2	757	382	0.02%	0.003%
94	13.029	3712	3713	3716	rBV2	401	150	0.01%	0.001%
95	13.161	3752	3754	3756	rBV	523	186	0.01%	0.001%
96	13.389	3822	3825	3827	rBV2	452	351	0.02%	0.003%
97	13.614	3892	3895	3902	rBV4	1147	995	0.06%	0.007%
98	14.009	4014	4018	4027	rVB	18066	11312	0.68%	0.082%
99	14.308	4109	4111	4112	rBV	578	245	0.01%	0.002%
100	15.614	4513	4517	4519	rBV3	1183	839	0.05%	0.006%


Sum of corrected areas: 13873436

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020124.D
Acq On : 21 Jan 2021 23:12
Operator : SY/MD
Sample : M1181-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

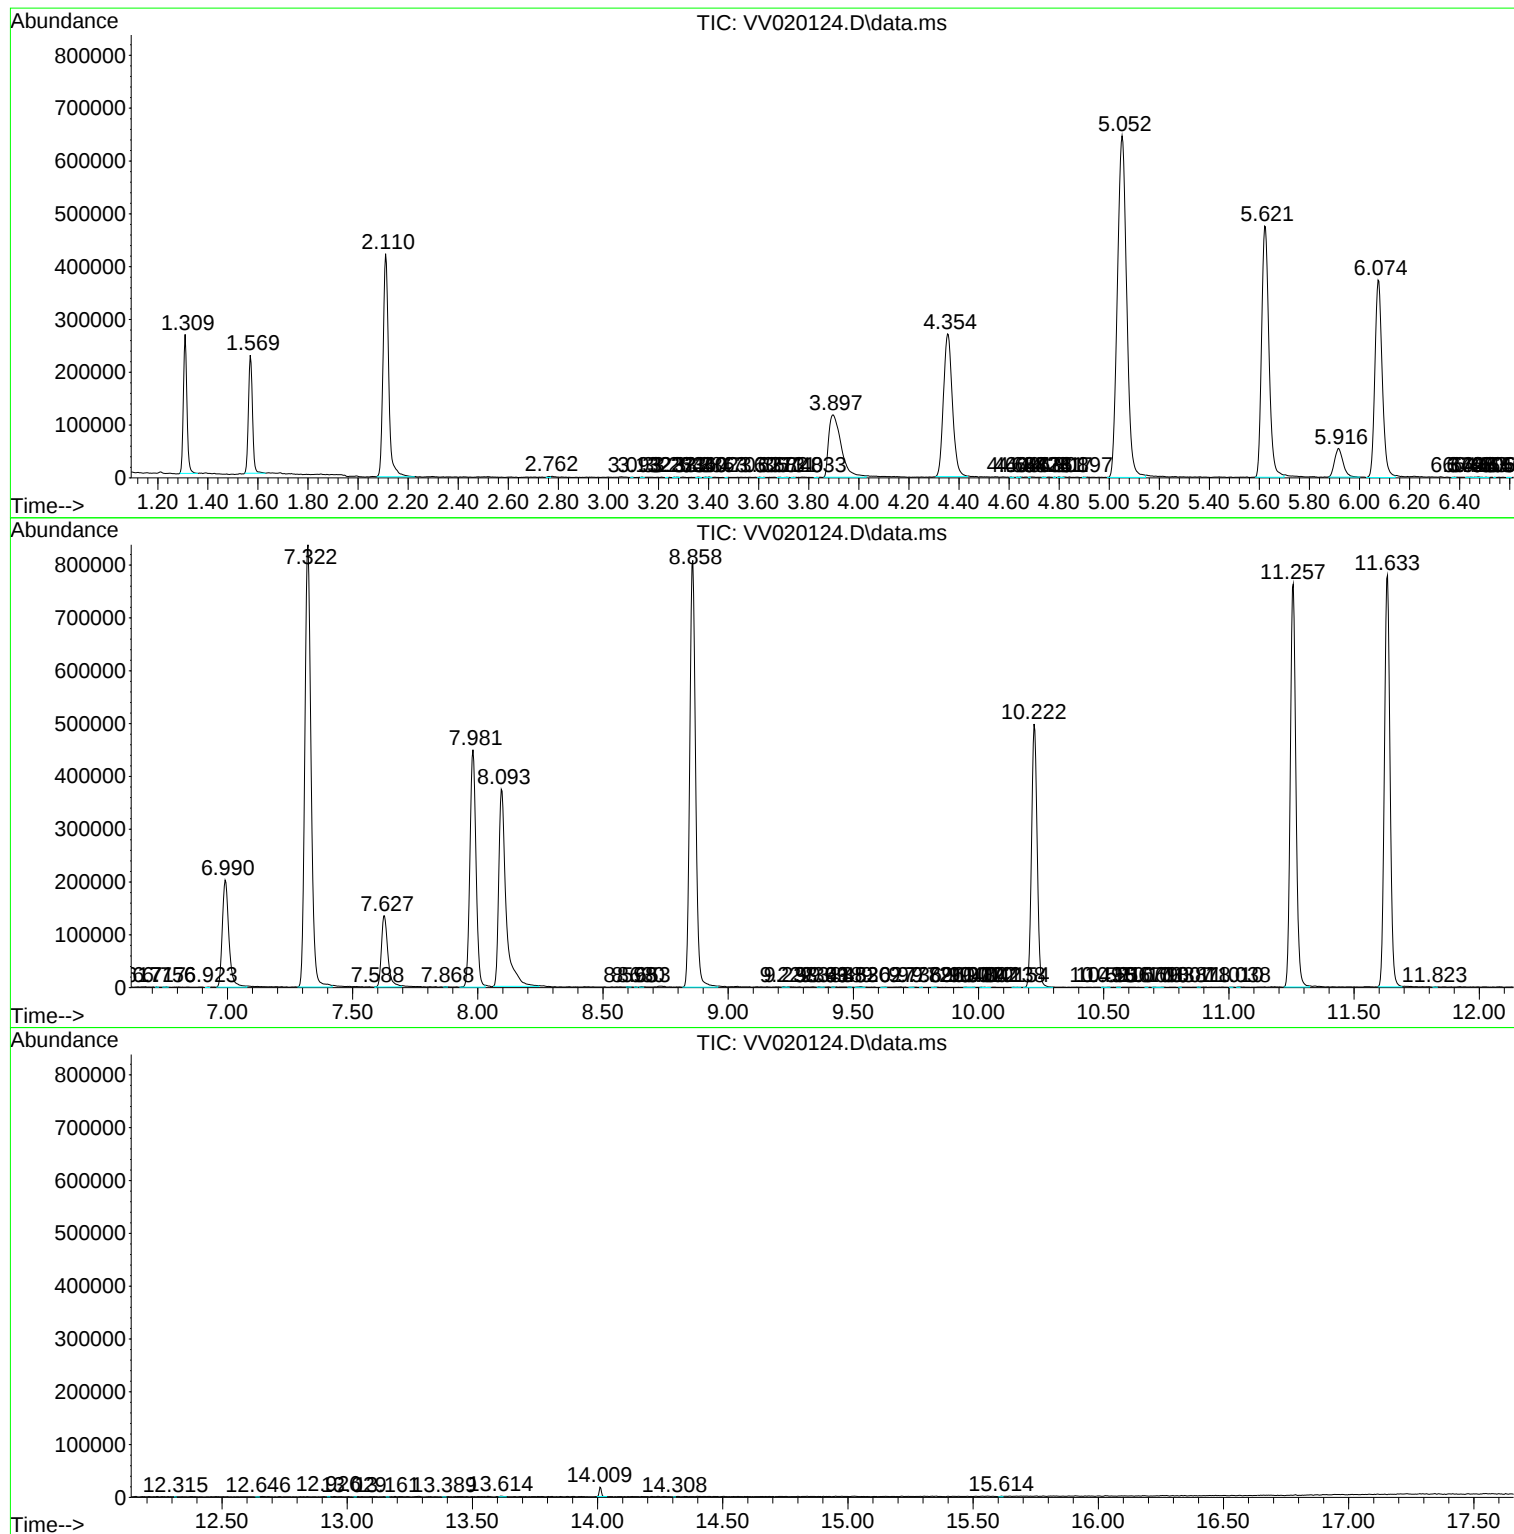

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020124.D
Acq On : 21 Jan 2021 23:12
Operator : SY/MD
Sample : M1181-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020124.D
Acq On : 21 Jan 2021 23:12
Operator : SY/MD
Sample : M1181-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
