

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020126.D
 Acq On : 22 Jan 2021 00:00
 Operator : SY/MD
 Sample : M1181-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E49

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

Signal : TIC: VV020126.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	86	rVB	165850	169649	16.28%	1.855%
2	1.569	143	149	161	rVB	145305	159583	15.31%	1.745%
3	2.110	307	317	339	rBV	240385	363752	34.90%	3.977%
4	2.486	431	434	437	rBV3	1098	523	0.05%	0.006%
5	2.698	496	500	502	rBV3	736	416	0.04%	0.005%
6	2.846	544	546	549	rBV2	645	440	0.04%	0.005%
7	2.862	549	551	554	rVV3	710	336	0.03%	0.004%
8	3.003	593	595	596	rBV	484	181	0.02%	0.002%
9	3.110	625	628	632	rBV4	728	460	0.04%	0.005%
10	3.187	648	652	654	rBV3	844	589	0.06%	0.006%
11	3.412	719	722	723	rBV2	585	266	0.03%	0.003%
12	3.495	743	748	752	rBV4	602	586	0.06%	0.006%
13	3.515	752	754	759	rVV4	418	302	0.03%	0.003%
14	3.557	766	767	772	rBV3	455	367	0.04%	0.004%
15	3.621	783	787	791	rBV4	506	452	0.04%	0.005%
16	3.756	826	829	831	rBV3	970	654	0.06%	0.007%
17	3.788	836	839	841	rVB	672	403	0.04%	0.004%
18	3.894	860	872	912	rBV3	100688	365970	35.11%	4.001%
19	4.354	1000	1015	1045	rBV	170902	420348	40.33%	4.596%
20	4.762	1137	1142	1145	rBV4	804	660	0.06%	0.007%
21	4.923	1189	1192	1193	rBV2	504	273	0.03%	0.003%
22	4.974	1206	1208	1210	rVB2	624	288	0.03%	0.003%
23	4.994	1211	1214	1215	rBV2	1044	496	0.05%	0.005%
24	5.052	1216	1232	1263	rVV2	407563	1042210	100.00%	11.395%
25	5.621	1396	1409	1435	rBV	293495	600661	57.63%	6.567%
26	5.917	1487	1501	1522	rBV6	50792	124444	11.94%	1.361%
27	6.029	1532	1536	1537	rBV4	599	454	0.04%	0.005%
28	6.074	1537	1550	1578	rVV	254897	518535	49.75%	5.670%
29	6.396	1648	1650	1654	rVB3	687	338	0.03%	0.004%
30	6.425	1654	1659	1661	rBV2	660	560	0.05%	0.006%
31	6.470	1671	1673	1675	rBV3	752	491	0.05%	0.005%
32	6.489	1677	1679	1683	rVB3	815	437	0.04%	0.005%
33	6.662	1730	1733	1737	rVB3	465	376	0.04%	0.004%
34	6.701	1742	1745	1746	rBV	128	69	0.01%	0.001%
35	6.708	1746	1747	1749	rVB2	228	72	0.01%	0.001%
36	6.794	1771	1774	1777	rVB2	208	133	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012121\
 Data File : VW020126.D
 Acq On : 22 Jan 2021 00:00
 Operator : SY/MD
 Sample : M1181-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E49

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	6.810	1777	1779	1782	rVB2	278	124	0.01%	0.001%
38	6.833	1782	1786	1789	rBV3	285	173	0.02%	0.002%
39	6.862	1792	1795	1798	rBV	151	137	0.01%	0.001%
40	6.952	1819	1823	1824	rBV2	248	129	0.01%	0.001%
41	6.990	1824	1835	1862	rBV	120818	223304	21.43%	2.442%
42	7.174	1888	1892	1893	rBV2	162	105	0.01%	0.001%
43	7.257	1913	1918	1919	rBV2	367	265	0.03%	0.003%
44	7.322	1925	1938	1957	rBV	496250	853176	81.86%	9.328%
45	7.627	2023	2033	2057	rBV	84189	148432	14.24%	1.623%
46	7.933	2127	2128	2129	rBV	137	35	0.00%	0.000%
47	7.981	2130	2143	2163	rBV	508756	861608	82.67%	9.421%
48	8.093	2168	2178	2213	rBV2	286609	588947	56.51%	6.439%
49	8.331	2249	2252	2256	rBV2	631	540	0.05%	0.006%
50	8.463	2289	2293	2297	rBV2	501	315	0.03%	0.003%
51	8.531	2307	2314	2318	rBV3	531	774	0.07%	0.008%
52	8.560	2318	2323	2324	rBV3	418	366	0.04%	0.004%
53	8.656	2350	2353	2356	rBV3	370	337	0.03%	0.004%
54	8.717	2367	2372	2376	rBV4	778	919	0.09%	0.010%
55	8.807	2398	2400	2401	rBV	309	160	0.02%	0.002%
56	8.859	2404	2416	2446	rVV	522694	860727	82.59%	9.411%
57	9.193	2517	2520	2521	rBV3	660	316	0.03%	0.003%
58	9.421	2589	2591	2596	rBV3	390	270	0.03%	0.003%
59	9.492	2611	2613	2614	rBV	425	172	0.02%	0.002%
60	9.611	2644	2650	2652	rBV3	697	695	0.07%	0.008%
61	10.222	2829	2840	2862	rVB	288248	452547	43.42%	4.948%
62	10.386	2888	2891	2892	rBV2	783	439	0.04%	0.005%
63	11.067	3101	3103	3104	rBV2	704	218	0.02%	0.002%
64	11.132	3119	3123	3126	rBV3	552	424	0.04%	0.005%
65	11.257	3151	3162	3181	rBV	426167	657139	63.05%	7.185%
66	11.633	3267	3279	3300	rBV	453490	713095	68.42%	7.797%
67	12.167	3442	3445	3447	rBV2	674	492	0.05%	0.005%
68	12.270	3474	3477	3480	rBV3	834	592	0.06%	0.006%
69	13.038	3712	3716	3718	rBV2	707	549	0.05%	0.006%
70	13.273	3786	3789	3791	rBV3	947	603	0.06%	0.007%
71	13.408	3829	3831	3834	rBV3	622	267	0.03%	0.003%
72	13.518	3863	3865	3869	rVB2	848	543	0.05%	0.006%
73	13.990	4010	4012	4017	rVB3	890	649	0.06%	0.007%
74	14.286	4101	4104	4109	rBV3	880	617	0.06%	0.007%

Sum of corrected areas: 9145974




Instrument :
MSVOA_V
ClientSampleId :
F1E49

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020126.D
Acq On : 22 Jan 2021 00:00
Operator : SY/MD
Sample : M1181-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

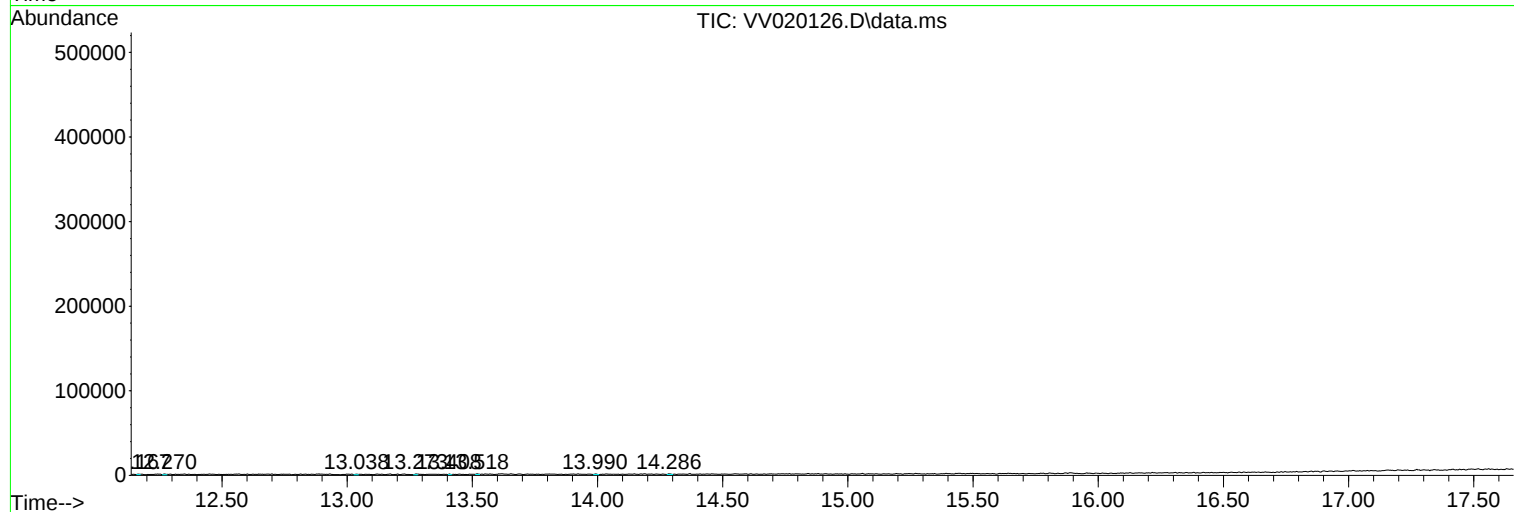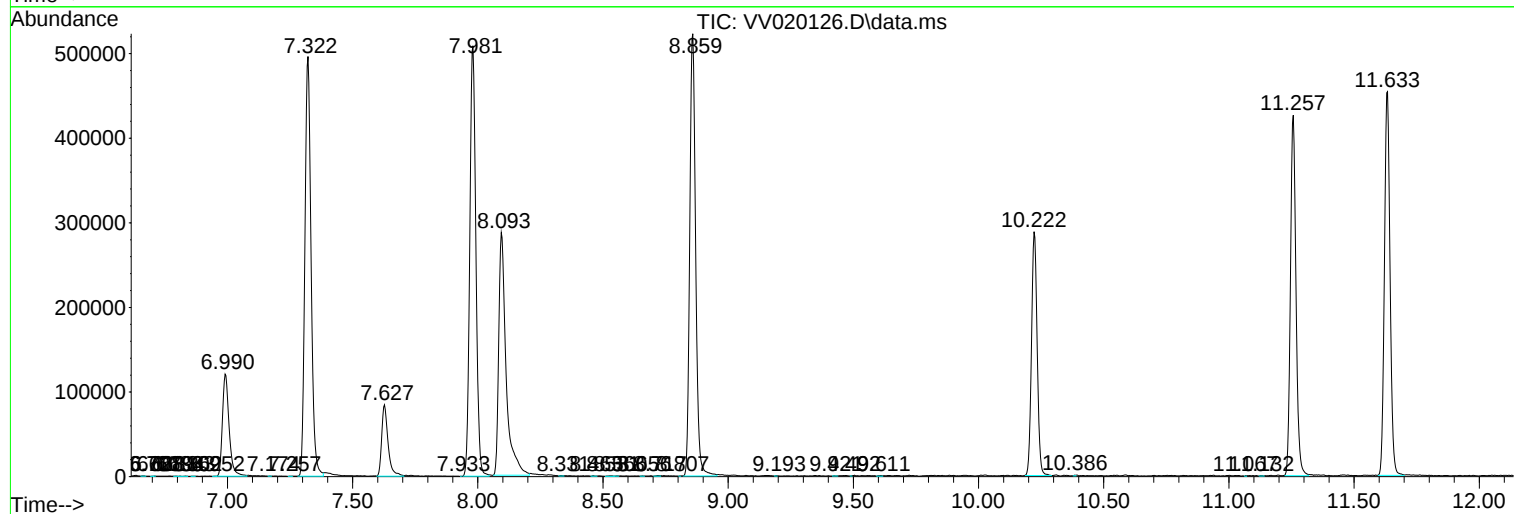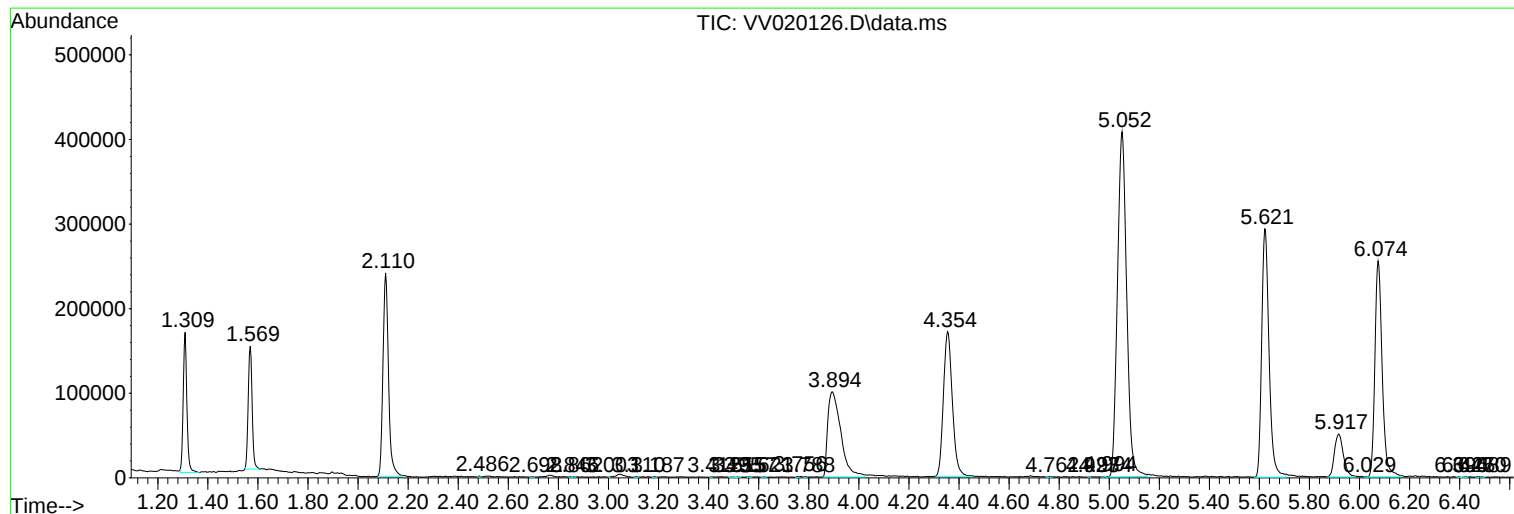

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020126.D
Acq On : 22 Jan 2021 00:00
Operator : SY/MD
Sample : M1181-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020126.D
Acq On : 22 Jan 2021 00:00
Operator : SY/MD
Sample : M1181-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc