

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020127.D
 Acq On : 22 Jan 2021 00:23
 Operator : SY/MD
 Sample : M1181-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020127.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	85	rVB	253057	261474	14.93%	1.791%
2	1.569	142	149	160	rBV	223370	241562	13.80%	1.654%
3	2.110	307	317	356	rVB	422906	656239	37.48%	4.495%
4	2.386	401	403	405	rBV3	682	277	0.02%	0.002%
5	2.438	416	419	421	rBV3	698	455	0.03%	0.003%
6	2.634	477	480	483	rVB4	743	521	0.03%	0.004%
7	2.769	511	522	533	rBV9	3259	6187	0.35%	0.042%
8	2.872	552	554	556	rBV2	493	252	0.01%	0.002%
9	3.010	595	597	599	rBV	339	239	0.01%	0.002%
10	3.126	631	633	636	rBV2	630	354	0.02%	0.002%
11	3.183	649	651	653	rBV2	424	231	0.01%	0.002%
12	3.273	675	679	681	rBV2	367	246	0.01%	0.002%
13	3.389	712	715	717	rBV	420	235	0.01%	0.002%
14	3.466	734	739	745	rBV5	750	1066	0.06%	0.007%
15	3.573	769	772	777	rBV3	483	323	0.02%	0.002%
16	3.695	807	810	815	rBV6	709	693	0.04%	0.005%
17	3.762	827	831	836	rBV3	425	443	0.03%	0.003%
18	3.823	848	850	855	rVB3	592	401	0.02%	0.003%
19	3.849	855	858	859	rBV	424	228	0.01%	0.002%
20	3.904	860	875	906	rBV3	135188	504709	28.83%	3.457%
21	4.354	1000	1015	1043	rBV	279762	684882	39.12%	4.691%
22	4.576	1081	1084	1089	rBV4	689	623	0.04%	0.004%
23	4.679	1114	1116	1118	rBV2	425	226	0.01%	0.002%
24	4.833	1161	1164	1167	rBV2	619	405	0.02%	0.003%
25	4.888	1179	1181	1185	rBV4	683	372	0.02%	0.003%
26	4.929	1191	1194	1197	rBV4	494	414	0.02%	0.003%
27	5.052	1215	1232	1258	rBV2	681811	1750912	100.00%	11.992%
28	5.457	1357	1358	1360	rVB	924	281	0.02%	0.002%
29	5.476	1360	1364	1365	rBV2	934	538	0.03%	0.004%
30	5.531	1379	1381	1385	rVB3	849	506	0.03%	0.003%
31	5.553	1385	1388	1391	rBV4	760	439	0.03%	0.003%
32	5.621	1397	1409	1436	rBV	473531	945072	53.98%	6.473%
33	5.916	1488	1501	1520	rBV5	75941	177451	10.13%	1.215%
34	6.074	1537	1550	1573	rBV	367238	739066	42.21%	5.062%
35	6.389	1646	1648	1651	rBV2	421	326	0.02%	0.002%
36	6.402	1651	1652	1656	rVB3	867	333	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020127.D
 Acq On : 22 Jan 2021 00:23
 Operator : SY/MD
 Sample : M1181-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	6.441	1660	1664	1667	rBV4	587	536	0.03%	0.004%
38	6.453	1667	1668	1671	rBV2	369	248	0.01%	0.002%
39	6.511	1685	1686	1689	rBV	546	327	0.02%	0.002%
40	6.563	1699	1702	1703	rBV3	745	378	0.02%	0.003%
41	6.646	1725	1728	1734	rBV6	924	1085	0.06%	0.007%
42	6.772	1764	1767	1770	rBV4	710	541	0.03%	0.004%
43	6.785	1770	1771	1775	rVB2	691	439	0.03%	0.003%
44	6.920	1810	1813	1819	rVB3	687	694	0.04%	0.005%
45	6.990	1823	1835	1859	rBV2	188084	349601	19.97%	2.394%
46	7.322	1924	1938	1978	rBV	745271	1328498	75.87%	9.099%
47	7.627	2023	2033	2052	rBV	132919	232672	13.29%	1.594%
48	7.884	2110	2113	2116	rBV2	479	265	0.02%	0.002%
49	7.926	2124	2126	2129	rBV2	490	337	0.02%	0.002%
50	7.981	2129	2143	2166	rVV	986544	1657690	94.68%	11.354%
51	8.093	2168	2178	2215	rVV2	424707	834316	47.65%	5.714%
52	8.502	2302	2305	2307	rBV3	903	520	0.03%	0.004%
53	8.621	2339	2342	2343	rBV2	611	248	0.01%	0.002%
54	8.858	2404	2416	2442	rBV	732142	1200840	68.58%	8.225%
55	9.264	2540	2542	2547	rVB2	768	433	0.02%	0.003%
56	9.402	2582	2585	2588	rBV2	469	305	0.02%	0.002%
57	9.418	2588	2590	2592	rBV	612	278	0.02%	0.002%
58	9.495	2610	2614	2617	rBV2	630	521	0.03%	0.004%
59	9.592	2641	2644	2645	rBV	580	267	0.02%	0.002%
60	9.640	2656	2659	2662	rBV2	461	273	0.02%	0.002%
61	9.662	2662	2666	2669	rBV2	400	303	0.02%	0.002%
62	9.678	2669	2671	2675	rVB3	750	542	0.03%	0.004%
63	9.701	2675	2678	2679	rBV	748	459	0.03%	0.003%
64	9.743	2687	2691	2694	rBV3	668	528	0.03%	0.004%
65	9.794	2703	2707	2708	rBV3	743	501	0.03%	0.003%
66	9.810	2710	2712	2714	rVV3	573	245	0.01%	0.002%
67	9.871	2729	2731	2736	rVB5	526	339	0.02%	0.002%
68	9.948	2753	2755	2758	rBV3	491	427	0.02%	0.003%
69	10.064	2788	2791	2792	rBV3	413	213	0.01%	0.001%
70	10.125	2809	2810	2813	rBV2	412	244	0.01%	0.002%
71	10.222	2828	2840	2860	rBV	441805	701362	40.06%	4.804%
72	10.386	2887	2891	2896	rBV4	624	812	0.05%	0.006%
73	10.592	2952	2955	2958	rBV3	983	485	0.03%	0.003%
74	10.678	2980	2982	2984	rVB2	867	342	0.02%	0.002%
75	10.694	2985	2987	2989	rBV2	569	232	0.01%	0.002%
76	10.739	2999	3001	3003	rBV2	884	491	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020127.D
 Acq On : 22 Jan 2021 00:23
 Operator : SY/MD
 Sample : M1181-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

77	10.768	3007	3010	3012	rVV3	510	264	0.02%	0.002%
78	10.823	3025	3027	3031	rVB2	816	483	0.03%	0.003%
79	11.010	3083	3085	3087	rVV	636	311	0.02%	0.002%
80	11.103	3112	3114	3116	rBV2	564	334	0.02%	0.002%
81	11.199	3141	3144	3146	rBV2	485	321	0.02%	0.002%
82	11.254	3150	3161	3181	rVV	712317	1120001	63.97%	7.671%
83	11.482	3231	3232	3234	rVB	796	256	0.01%	0.002%
84	11.527	3244	3246	3249	rBV2	577	388	0.02%	0.003%
85	11.633	3267	3279	3298	rBV	756597	1175479	67.14%	8.051%
86	12.138	3433	3436	3437	rBV2	408	253	0.01%	0.002%
87	12.318	3487	3492	3496	rBV2	557	579	0.03%	0.004%
88	12.620	3584	3586	3588	rBV2	552	276	0.02%	0.002%
89	12.984	3697	3699	3700	rBV	611	215	0.01%	0.001%
90	13.141	3745	3748	3751	rBV3	507	338	0.02%	0.002%
91	13.157	3751	3753	3755	rBV2	683	411	0.02%	0.003%
92	13.209	3766	3769	3774	rBV3	664	589	0.03%	0.004%
93	13.328	3803	3806	3809	rBV2	734	494	0.03%	0.003%
94	13.373	3818	3820	3825	rVB4	496	375	0.02%	0.003%
95	13.527	3866	3868	3871	rBV4	833	361	0.02%	0.002%
96	13.646	3903	3905	3908	rBV	732	367	0.02%	0.003%
97	13.755	3937	3939	3942	rBV3	629	356	0.02%	0.002%
98	13.865	3971	3973	3976	rBV2	816	477	0.03%	0.003%
99	14.048	4029	4030	4033	rBV2	524	362	0.02%	0.002%
100	14.604	4201	4203	4206	rBV2	684	512	0.03%	0.004%




Sum of corrected areas: 14600620

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020127.D
Acq On : 22 Jan 2021 00:23
Operator : SY/MD
Sample : M1181-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

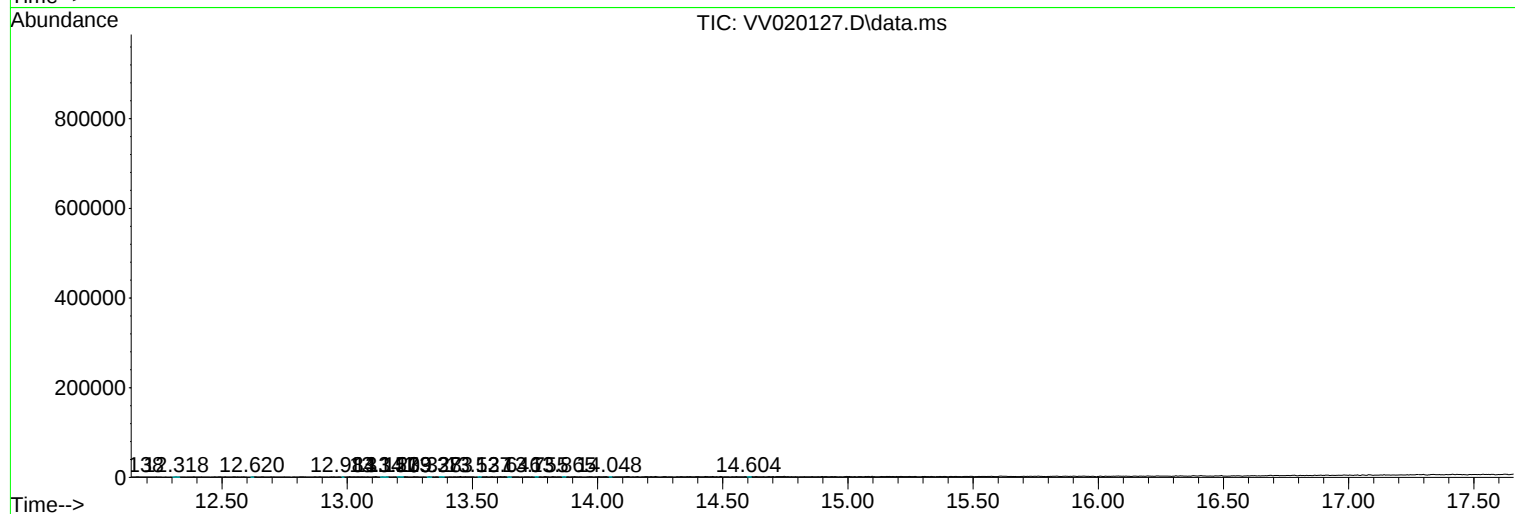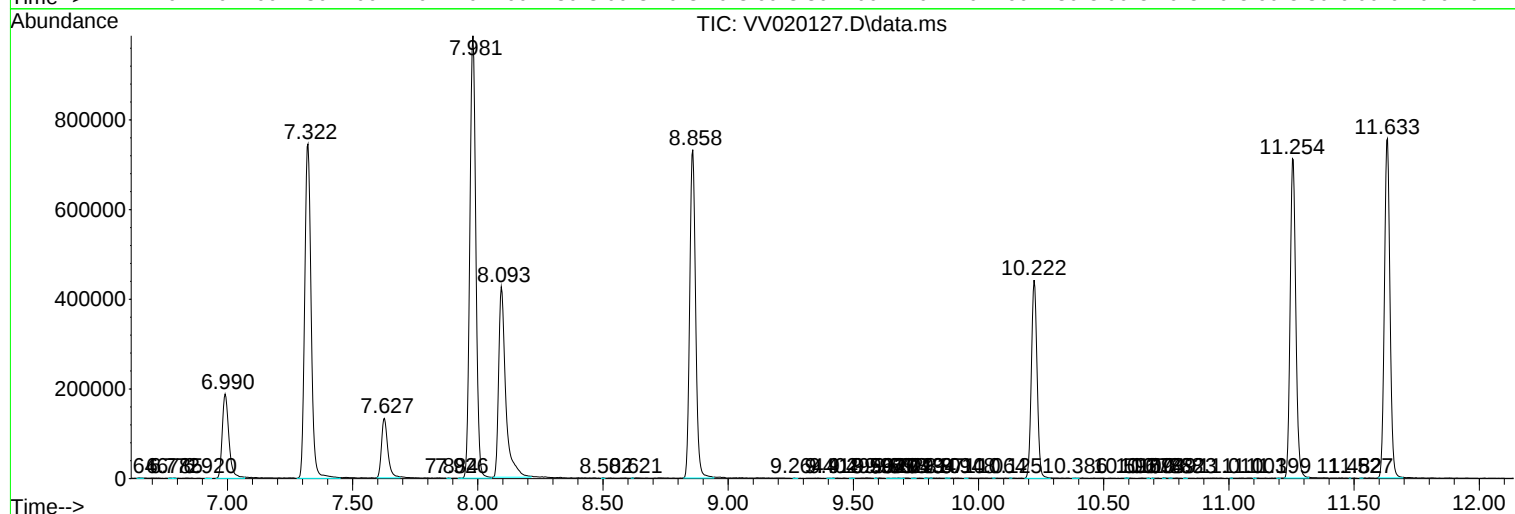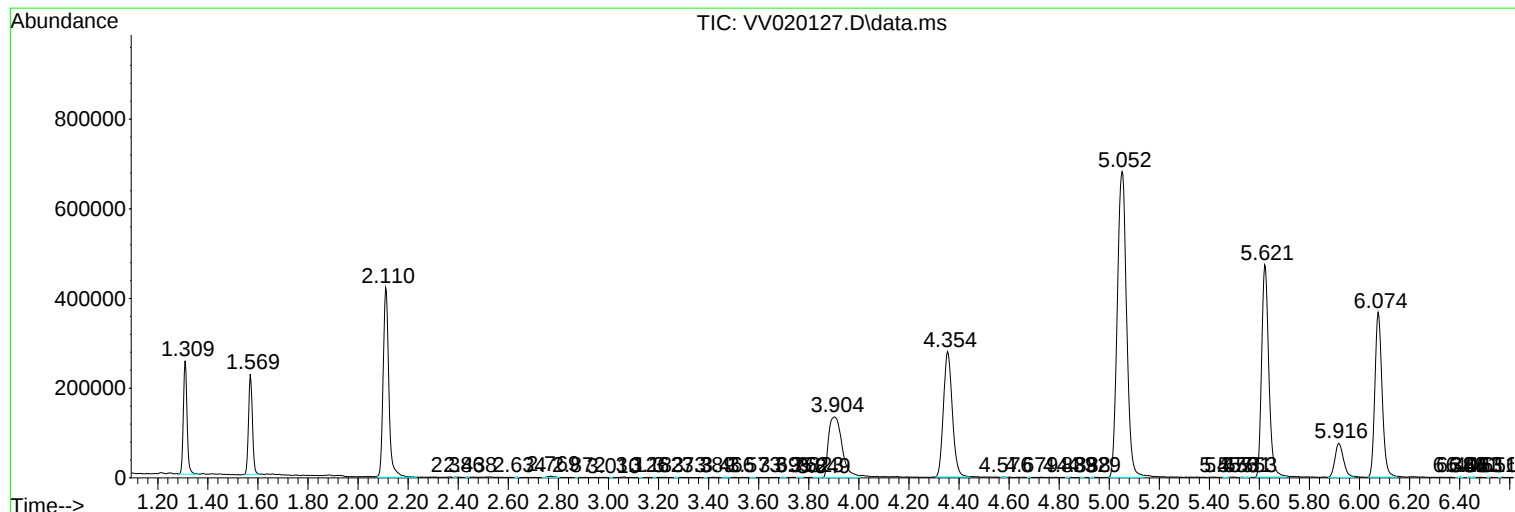

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020127.D
Acq On : 22 Jan 2021 00:23
Operator : SY/MD
Sample : M1181-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020127.D
Acq On : 22 Jan 2021 00:23
Operator : SY/MD
Sample : M1181-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
