

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020129.D
 Acq On : 22 Jan 2021 01:10
 Operator : SY/MD
 Sample : M1201-04 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Z9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020129.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	82	rVB	217985	216259	12.88%	1.638%
2	1.570	142	149	161	rVB	170073	192857	11.49%	1.461%
3	2.110	306	317	356	rVB	347955	529157	31.52%	4.009%
4	2.341	387	389	390	rBV	333	125	0.01%	0.001%
5	2.508	438	441	442	rBV2	1138	635	0.04%	0.005%
6	2.621	467	476	478	rBV3	1341	1844	0.11%	0.014%
7	2.672	487	492	495	rBV2	396	315	0.02%	0.002%
8	2.881	555	557	562	rVB2	343	246	0.01%	0.002%
9	2.904	562	564	570	rBV	313	301	0.02%	0.002%
10	2.984	584	589	592	rBV2	279	240	0.01%	0.002%
11	3.049	599	609	621	rVB4	3779	7412	0.44%	0.056%
12	3.097	621	624	627	rVB	396	188	0.01%	0.001%
13	3.119	628	631	635	rBV2	269	169	0.01%	0.001%
14	3.155	640	642	648	rVB2	444	483	0.03%	0.004%
15	3.187	648	652	654	rBV	260	255	0.02%	0.002%
16	3.219	659	662	664	rBV	158	115	0.01%	0.001%
17	3.267	673	677	680	rBV2	247	228	0.01%	0.002%
18	3.309	685	690	693	rVV	333	220	0.01%	0.002%
19	3.380	710	712	713	rBV	124	30	0.00%	0.000%
20	3.412	720	722	725	rVB	265	118	0.01%	0.001%
21	3.431	725	728	729	rBV	185	122	0.01%	0.001%
22	3.492	743	747	751	rVB2	474	297	0.02%	0.002%
23	3.563	767	769	771	rVB2	129	34	0.00%	0.000%
24	3.579	772	774	776	rVV2	104	58	0.00%	0.000%
25	3.598	778	780	782	rVV2	209	106	0.01%	0.001%
26	3.614	782	785	792	rVB2	362	426	0.03%	0.003%
27	3.643	792	794	796	rBV2	71	34	0.00%	0.000%
28	3.666	796	801	803	rBV2	219	133	0.01%	0.001%
29	3.708	810	814	815	rBV	162	113	0.01%	0.001%
30	3.740	820	824	825	rBV2	564	335	0.02%	0.003%
31	3.772	826	834	843	rVB6	2201	3929	0.23%	0.030%
32	3.830	849	852	855	rBV	189	146	0.01%	0.001%
33	3.843	855	856	859	rVB	331	102	0.01%	0.001%
34	3.859	859	861	862	rBV	265	125	0.01%	0.001%
35	3.897	862	873	905	rBV	112806	363953	21.68%	2.757%
36	4.354	998	1015	1046	rBV	272585	666117	39.67%	5.046%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020129.D
 Acq On : 22 Jan 2021 01:10
 Operator : SY/MD
 Sample : M1201-04 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Z9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	4.621	1096	1098	1100	rBV	234	120	0.01%	0.001%
38	4.679	1115	1116	1117	rBV	119	34	0.00%	0.000%
39	4.698	1117	1122	1123	rVV2	518	296	0.02%	0.002%
40	4.711	1123	1126	1128	rVV	188	118	0.01%	0.001%
41	4.775	1138	1146	1147	rBV3	493	537	0.03%	0.004%
42	4.823	1158	1161	1164	rBV	253	205	0.01%	0.002%
43	4.897	1182	1184	1185	rBV	200	85	0.01%	0.001%
44	4.984	1208	1211	1212	rBV	337	178	0.01%	0.001%
45	5.052	1214	1232	1257	rBV2	655119	1679037	100.00%	12.719%
46	5.396	1337	1339	1340	rBV	191	54	0.00%	0.000%
47	5.405	1340	1342	1344	rBV	250	131	0.01%	0.001%
48	5.486	1365	1367	1370	rBV2	385	250	0.01%	0.002%
49	5.621	1396	1409	1438	rBV	508179	1031286	61.42%	7.812%
50	5.910	1488	1499	1523	rVB3	38957	82562	4.92%	0.625%
51	6.074	1537	1550	1577	rBV	376891	764808	45.55%	5.794%
52	6.302	1618	1621	1625	rVB	323	277	0.02%	0.002%
53	6.325	1625	1628	1631	rBV2	263	201	0.01%	0.002%
54	6.357	1636	1638	1641	rVV	265	134	0.01%	0.001%
55	6.376	1641	1644	1646	rVV	365	179	0.01%	0.001%
56	6.392	1646	1649	1653	rVB2	289	202	0.01%	0.002%
57	6.434	1659	1662	1664	rBV	252	111	0.01%	0.001%
58	6.460	1668	1670	1671	rBV	154	45	0.00%	0.000%
59	6.518	1685	1688	1690	rBV	160	90	0.01%	0.001%
60	6.576	1705	1706	1707	rBV	118	33	0.00%	0.000%
61	6.643	1724	1727	1729	rBV	470	343	0.02%	0.003%
62	6.855	1792	1793	1794	rVB	119	23	0.00%	0.000%
63	6.865	1794	1796	1797	rBV	318	87	0.01%	0.001%
64	6.990	1824	1835	1857	rBV	197698	356448	21.23%	2.700%
65	7.322	1924	1938	1967	rBV	771945	1347923	80.28%	10.211%
66	7.627	2022	2033	2052	rBV	142119	245543	14.62%	1.860%
67	7.862	2100	2106	2110	rBV4	549	646	0.04%	0.005%
68	7.984	2137	2144	2153	rVB7	3550	5794	0.35%	0.044%
69	8.019	2153	2155	2158	rBV	255	85	0.01%	0.001%
70	8.093	2167	2178	2218	rBV2	425171	873602	52.03%	6.618%
71	8.605	2334	2337	2338	rBV2	424	224	0.01%	0.002%
72	8.666	2354	2356	2359	rVB2	524	277	0.02%	0.002%
73	8.711	2368	2370	2374	rBV2	371	202	0.01%	0.002%
74	8.859	2404	2416	2444	rBV	835738	1358958	80.94%	10.295%
75	9.370	2569	2575	2576	rBV	544	497	0.03%	0.004%
76	9.572	2635	2638	2639	rBV	435	225	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020129.D
Acq On : 22 Jan 2021 01:10
Operator : SY/MD
Sample : M1201-04 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Title : VOC Analysis

77	9.653	2660	2663	2664	rBV	244	145	0.01%	0.001%
78	10.222	2827	2840	2864	rBV	517453	813083	48.43%	6.159%
79	11.003	3081	3083	3088	rVB2	475	303	0.02%	0.002%
80	11.257	3150	3162	3188	rBV	847397	1299245	77.38%	9.842%
81	11.630	3267	3278	3304	rBV	848446	1348082	80.29%	10.212%
82	13.649	3904	3906	3912	rBV3	592	681	0.04%	0.005%




Sum of corrected areas: 13200616

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020129.D
Acq On : 22 Jan 2021 01:10
Operator : SY/MD
Sample : M1201-04 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

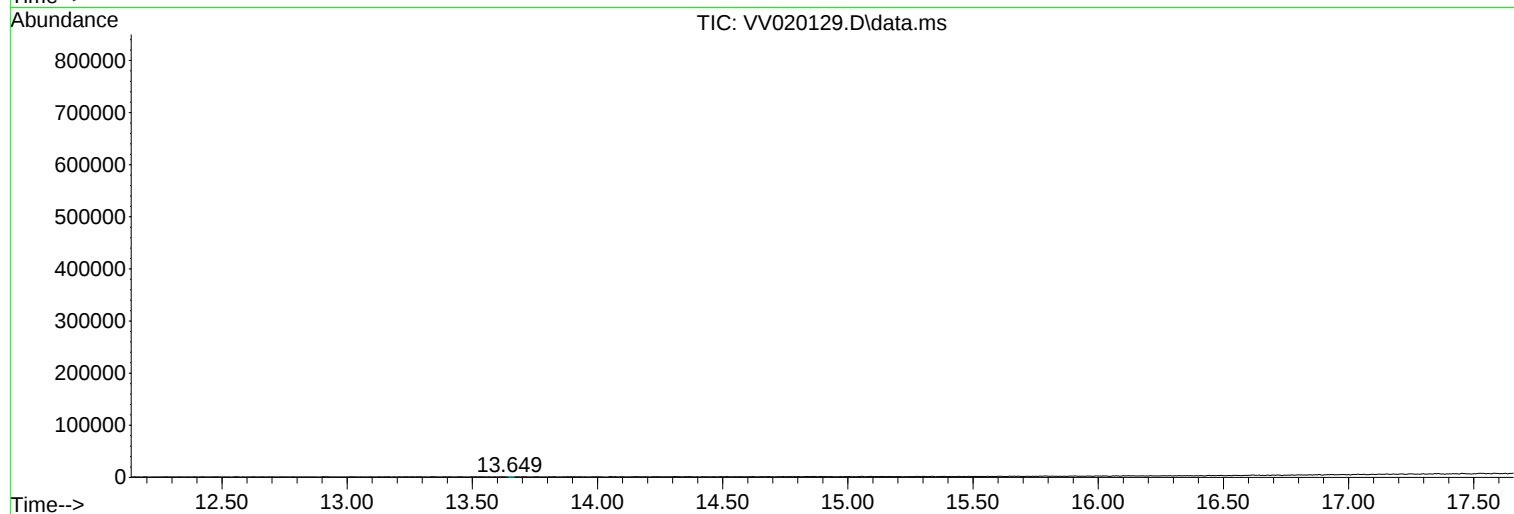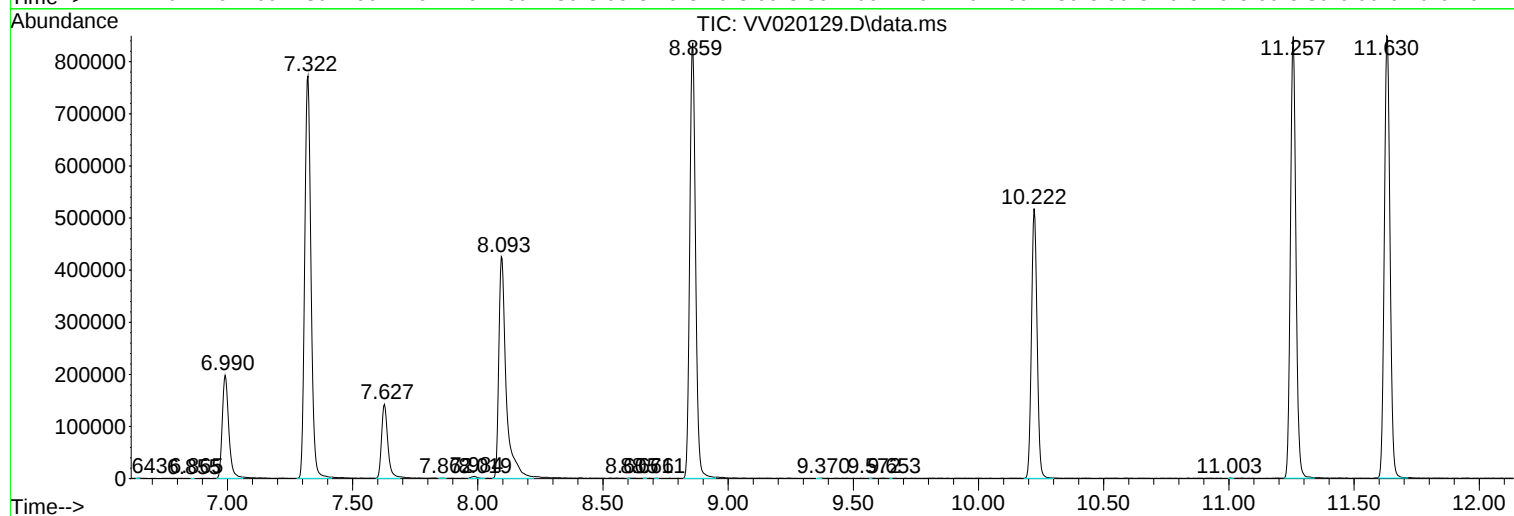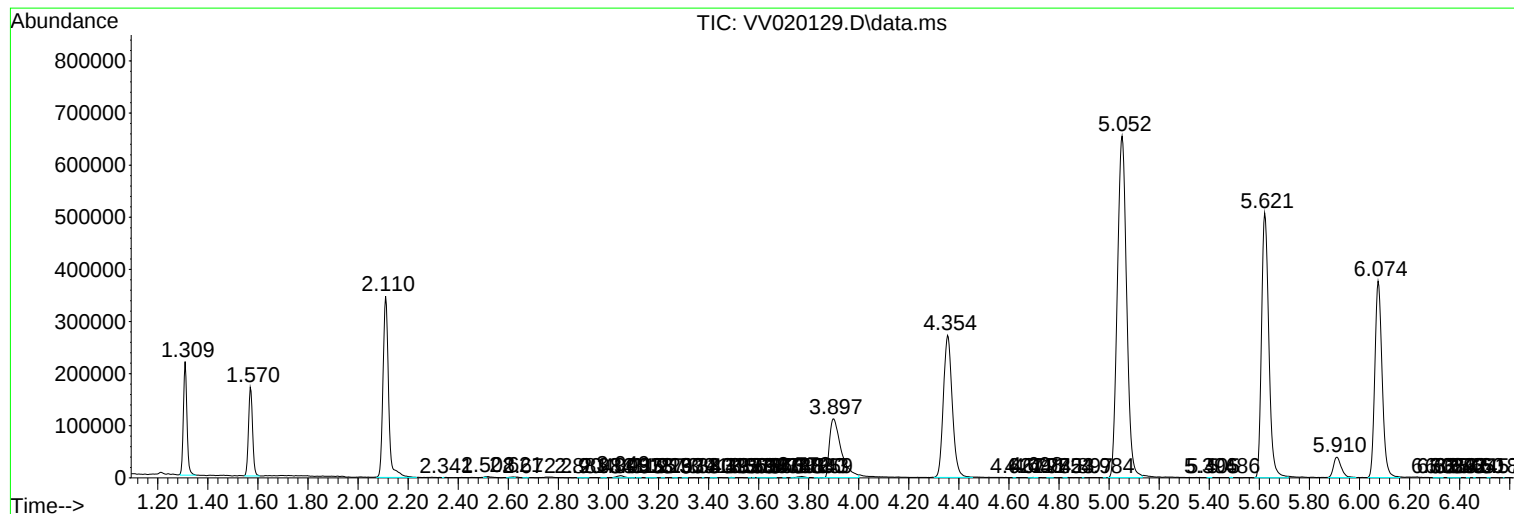

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020129.D
Acq On : 22 Jan 2021 01:10
Operator : SY/MD
Sample : M1201-04 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
Data File : VV020129.D
Acq On : 22 Jan 2021 01:10
Operator : SY/MD
Sample : M1201-04 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Z9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------