
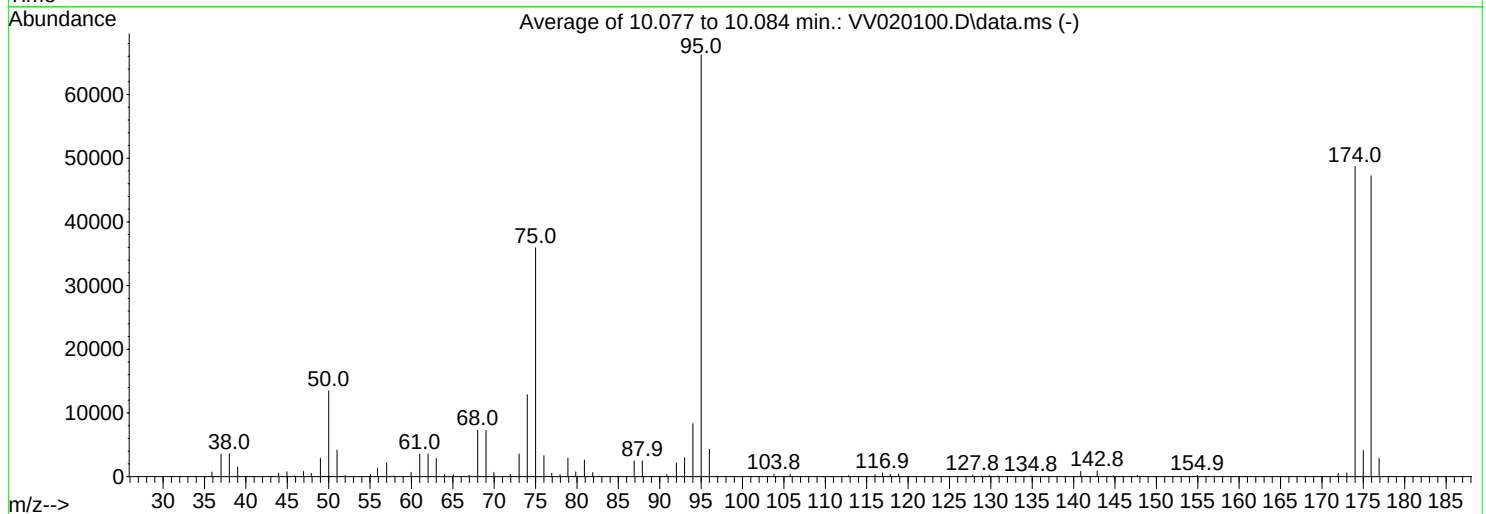


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012121\
 Data File : VV020100.D
 Acq On : 21 Jan 2021 08:59
 Operator : SY/MD
 Sample : BFB85
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB85

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis
 Last Update : Sat Jan 23 00:14:09 2021

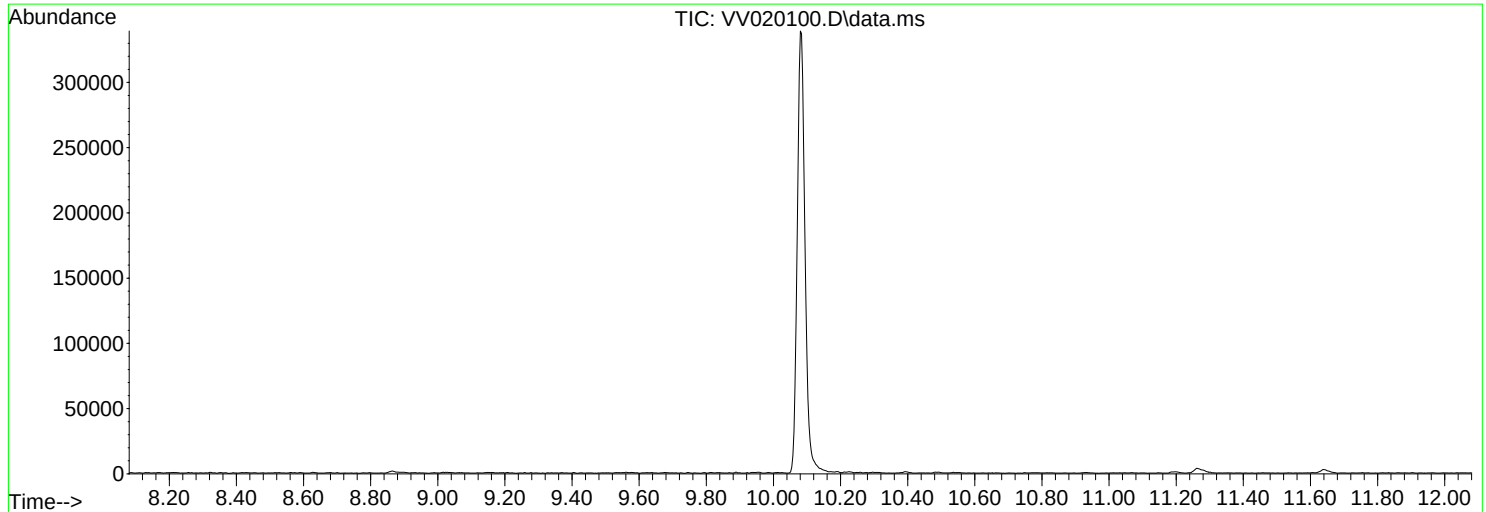

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2785

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	13460	PASS
75	95	30	80	54.3	35936	PASS
95	95	100	100	100.0	66229	PASS
96	95	5	9	6.5	4302	PASS
173	174	0.00	2	1.2	579	PASS
174	95	50	120	73.5	48691	PASS
175	174	5	9	8.5	4135	PASS
176	174	95	101	97.0	47253	PASS
177	176	5	9	6.1	2878	PASS

m/z	Abundance
40.00	230.0
44.00	387.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
35.90	662.0
37.00	3454.0
38.00	3426.0
39.00	1441.0
39.80	205.0
44.00	860.0
44.90	772.0
45.80	130.0
47.00	807.0
47.90	481.0
49.00	2765.0
50.00	12441.0
51.00	4053.0
52.00	161.0
55.00	353.0
55.90	1247.0
57.00	2100.0
57.90	127.0
60.00	579.0
61.00	3160.0
62.00	3509.0
63.00	2604.0
64.00	279.0
65.00	338.0
66.90	237.0
68.00	7123.0
69.00	7076.0
69.90	689.0
71.90	330.0
73.00	3429.0
74.00	12352.0
75.00	33920.0
76.00	3331.0
77.00	472.0
78.00	297.0
78.90	2730.0
79.80	637.0
80.90	2570.0
81.90	592.0
86.90	2384.0
87.90	2235.0
90.80	320.0
92.00	1944.0
93.00	2753.0
94.00	7976.0
95.00	62328.0
96.00	4106.0
103.80	425.0
104.80	105.0
105.70	321.0
110.80	102.0
112.80	108.0
116.00	296.0
116.90	538.0
117.80	336.0
118.90	403.0
127.80	253.0
128.90	116.0
129.90	190.0
130.90	110.0
134.80	108.0
140.90	797.0
142.80	893.0
144.80	132.0
147.70	190.0
155.00	251.0
157.00	154.0
172.00	421.0
173.00	576.0
174.00	44960.0
175.00	3789.0
175.90	43432.0
176.90	2636.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
35.90	745.0
37.00	3743.0
38.00	3798.0
39.00	1569.0
39.90	209.0
44.00	924.0
45.00	824.0
45.80	128.0
46.90	867.0
47.90	540.0
49.00	2977.0
50.00	13836.0
51.00	4344.0
52.00	183.0
53.00	104.0
55.10	335.0
55.90	1395.0
57.00	2265.0
57.90	121.0
59.90	684.0
61.00	3732.0
62.00	3688.0
63.00	2988.0
64.00	350.0
65.00	319.0
66.90	250.0
68.00	7497.0
69.00	7474.0
69.90	707.0
71.90	427.0
73.00	3703.0
74.00	13370.0
75.00	37288.0
76.00	3433.0
76.90	534.0
78.00	351.0
78.90	3026.0
79.80	759.0
80.90	2683.0
81.90	673.0
82.80	105.0
86.00	107.0
86.90	2554.0
87.90	2548.0
90.90	333.0
92.00	2209.0
93.00	3117.0
94.00	8679.0
95.00	68744.0
96.00	4406.0
96.90	124.0
103.80	428.0
105.80	393.0
112.80	149.0
116.00	363.0
116.90	641.0
117.80	365.0
118.90	442.0
127.80	277.0
128.90	126.0
129.70	220.0
130.80	111.0
134.80	123.0
136.50	103.0
140.90	846.0
142.90	900.0
144.80	149.0
146.00	134.0
147.70	229.0
155.00	231.0
157.00	137.0
172.00	562.0
173.00	605.0
174.00	49968.0
175.00	4289.0
175.90	48712.0
176.90	2969.0
178.10	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
35.90	783.0
37.00	3538.0
38.00	3589.0
39.00	1541.0
40.00	242.0
43.90	926.0
45.00	743.0
45.90	150.0
47.00	736.0
47.90	519.0
49.00	2874.0
50.00	14102.0
51.00	4108.0
52.00	180.0
53.00	122.0
55.10	302.0
55.90	1349.0
57.00	2114.0
57.90	102.0
59.90	766.0
61.00	3767.0
62.00	3553.0
63.00	3037.0
64.00	345.0
65.10	287.0
67.00	231.0
68.00	7220.0
69.00	7288.0
70.00	629.0
72.00	428.0
73.00	3566.0
74.00	12861.0
75.00	36600.0
76.00	3111.0
76.90	577.0
77.90	330.0
78.90	2962.0
79.90	881.0
80.90	2594.0
81.90	673.0
82.70	105.0
85.90	151.0
86.90	2442.0
87.90	2633.0
90.90	317.0
92.00	2294.0
93.00	3084.0
94.00	8371.0
95.00	67616.0
96.00	4393.0
96.90	153.0
103.80	378.0
105.80	421.0
109.70	111.0
112.80	170.0
116.00	361.0
116.90	643.0
117.90	338.0
118.80	477.0
127.80	305.0
128.90	115.0
129.80	252.0
130.80	120.0
134.90	123.0
140.80	817.0
141.90	110.0
142.90	828.0
144.80	148.0
146.00	120.0
146.80	113.0
147.70	254.0
154.90	181.0
157.00	115.0
160.70	119.0
171.90	605.0
173.00	555.0
174.00	51144.0
175.00	4327.0
176.00	49616.0
176.90	3029.0
178.10	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85