

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012125\
 Data File : VV038484.D
 Acq On : 21 Jan 2025 15:29
 Operator : SY/MD
 Sample : Q1125-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B08

Quant Time: Jan 22 02:56:22 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 22 02:52:26 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	261786	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	275104	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	107195	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	78319	3.628	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.600%
7) Chloroethane-d5	1.532	69	71592	3.949	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.000%
11) 1,1-Dichloroethene-d2	2.056	65	35735	3.673	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.400%
20) 2-Butanone-d5	3.805	46	171689	37.812	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	75.620%
24) Chloroform-d	4.239	84	158060	3.906	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.200%
26) 1,2-Dichloroethane-d4	4.934	65	69565	3.752	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.000%
32) Benzene-d6	4.950	84	297961	3.932	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.600%
36) 1,2-Dichloropropane-d6	5.979	67	96080	4.172	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.400%
41) Toluene-d8	7.236	98	233257	3.427	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.600%#
43) trans-1,3-Dichloroprop...	7.558	79	28304	3.360	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	67.200%
46) 2-Hexanone-d5	8.024	63	102273	30.771	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	61.540%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	67846	3.716	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	74.400%
66) 1,2-Dichlorobenzene-d4	11.551	152	81757	4.506	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.200%
Target Compounds					Qvalue	
13) Acetone	2.140	43	26709	7.560	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012125\
Data File : VV038484.D
Acq On : 21 Jan 2025 15:29
Operator : SY/MD
Sample : Q1125-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B08

Quant Time: Jan 22 02:56:22 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 22 02:52:26 2025
Response via : Initial Calibration

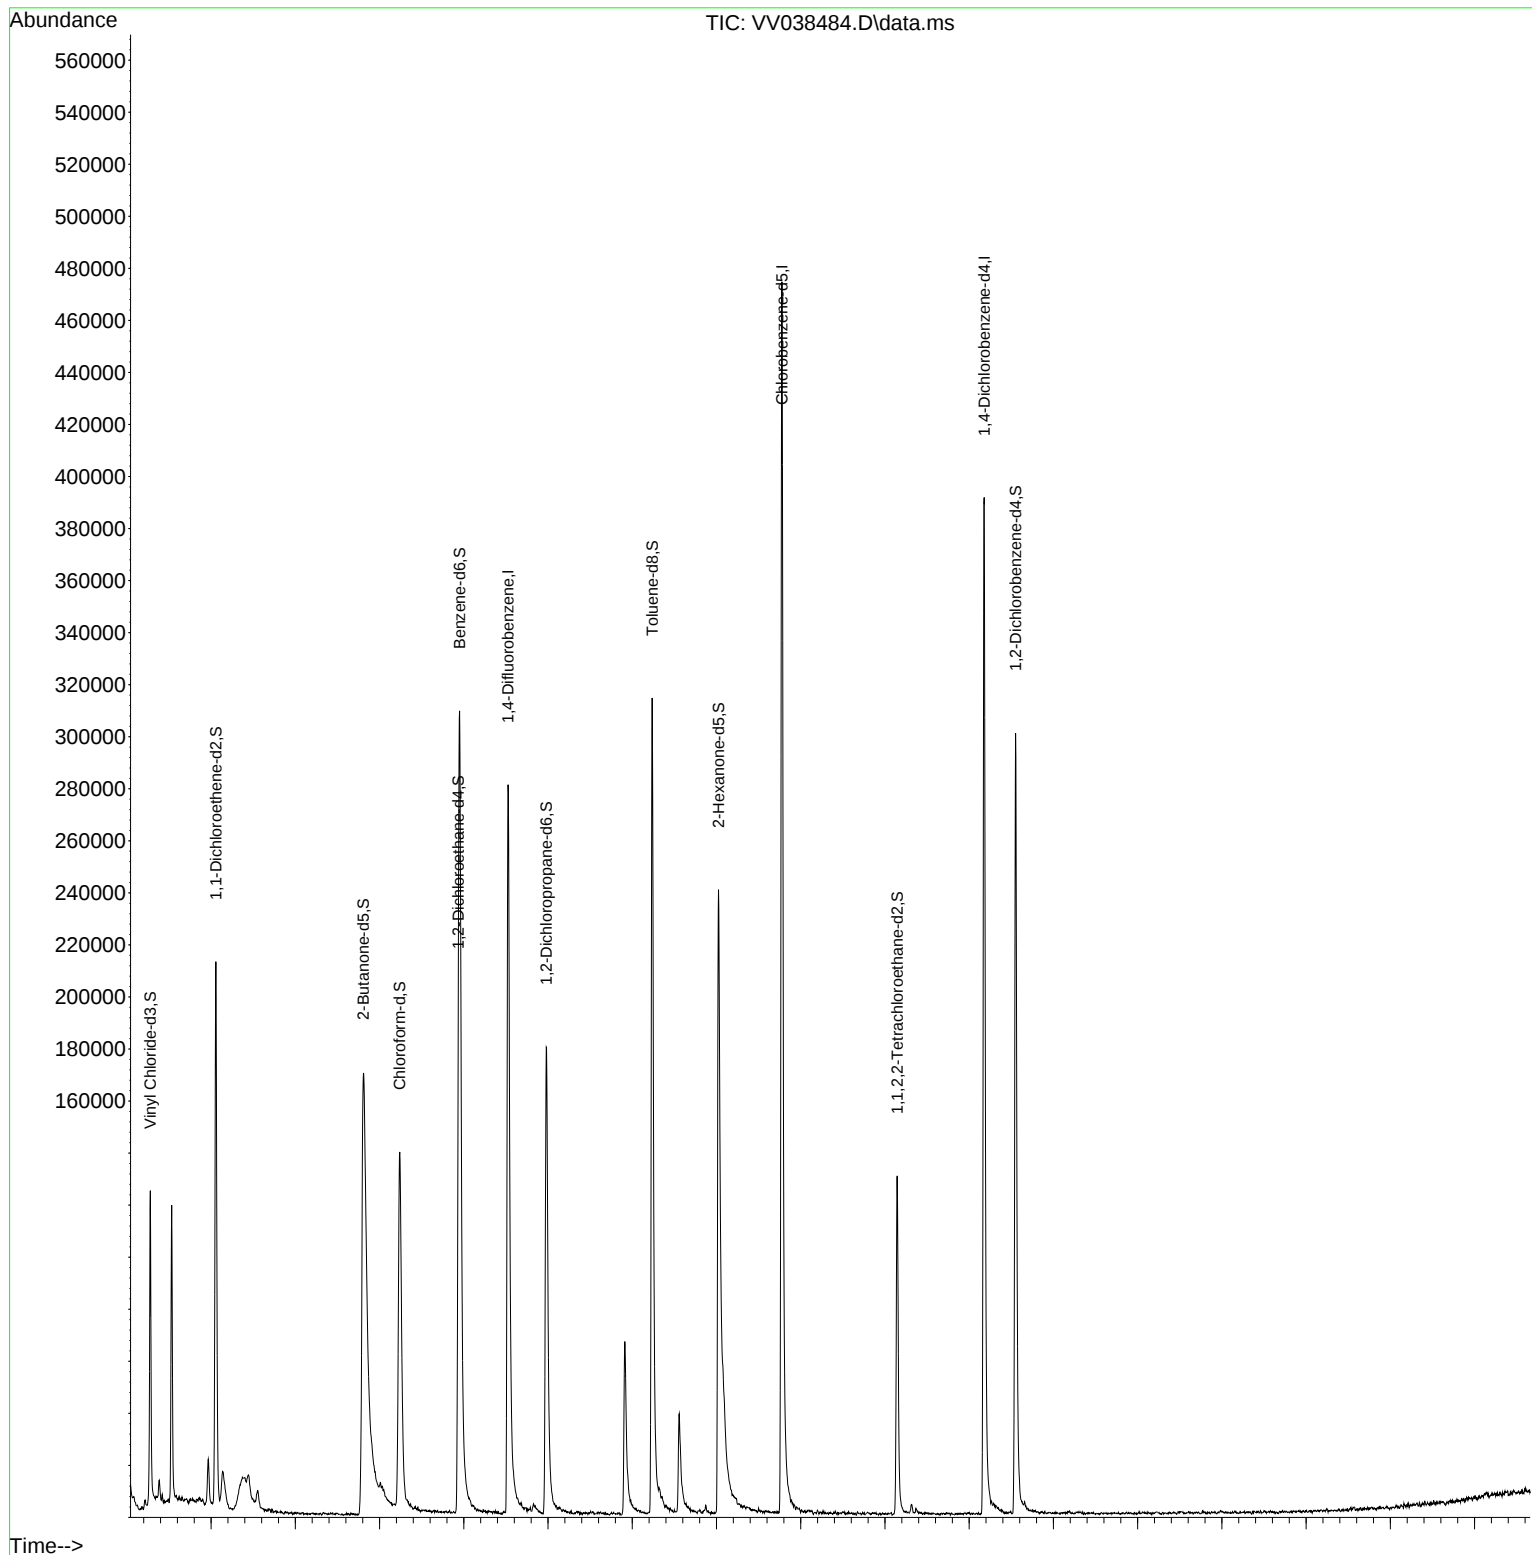

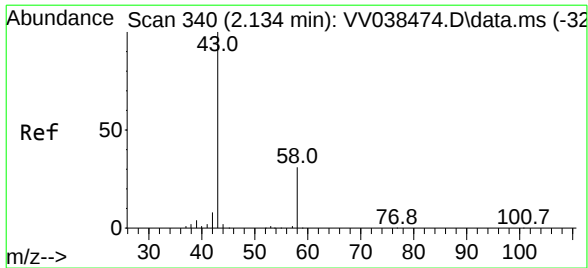

#13
 Acetone
 Concen: 7.560 ug/L
 RT: 2.140 min Scan# 34
 Delta R.T. 0.006 min
 Lab File: VV038484.D
 Acq: 21 Jan 2025 15:29

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B08

Tgt Ion:	43	Resp:	26709
Ion	Ratio	Lower	Upper
43	100		
58	35.5	0.0	67.2

