
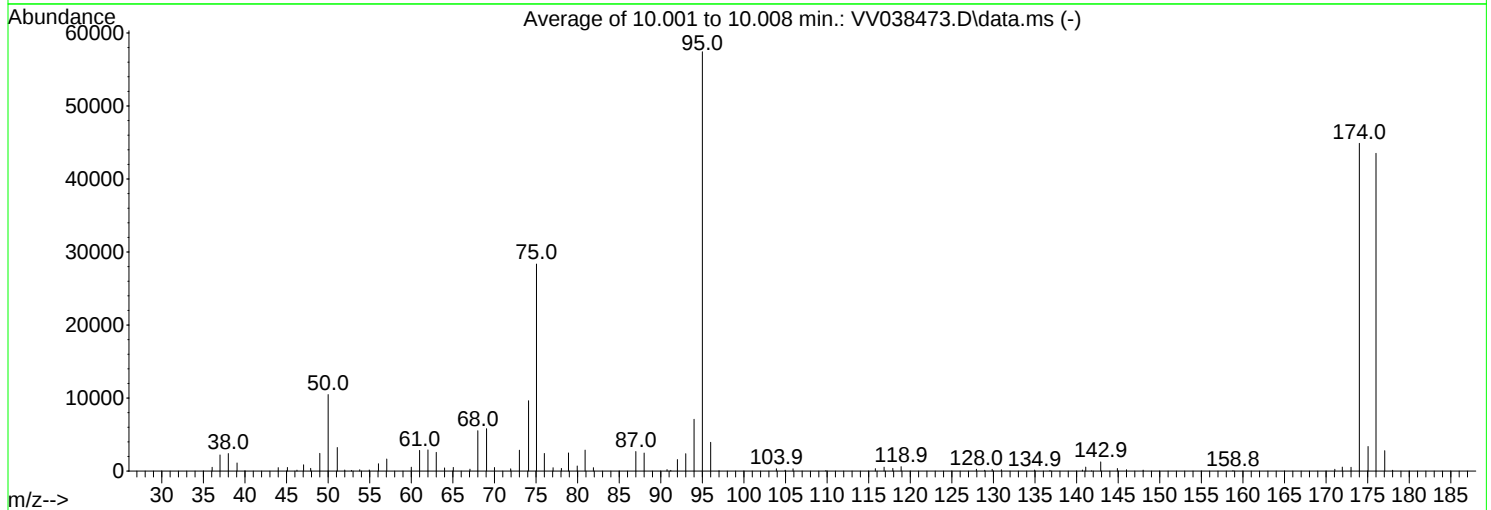


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012125\
Data File : VV038473.D
Acq On : 21 Jan 2025 09:30
Operator : SY/MD
Sample : BFB300
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB300

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Jan 22 02:52:26 2025

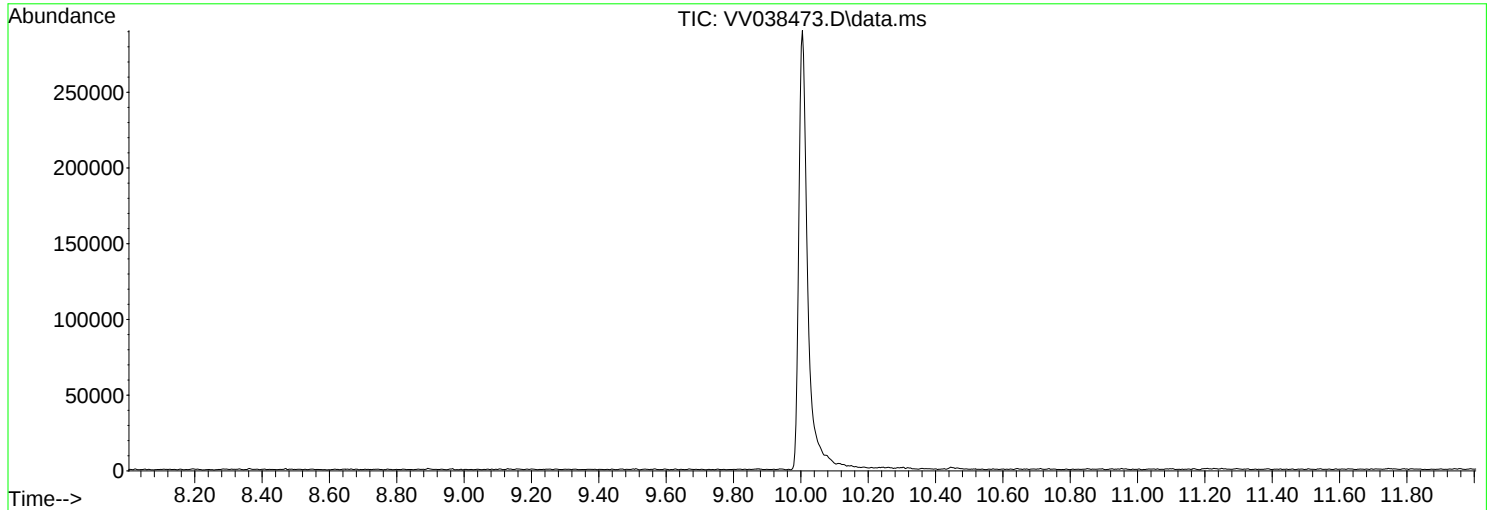

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	10476	PASS
75	95	30	80	49.4	28355	PASS
95	95	100	100	100.0	57429	PASS
96	95	5	9	6.9	3939	PASS
173	174	0.00	2	1.2	521	PASS
174	95	50	120	78.2	44888	PASS
175	174	5	9	7.5	3366	PASS
176	174	95	105	96.9	43517	PASS
177	176	5	10	6.4	2792	PASS

m/z	Abundance
40.00	502.0
43.00	100.0
44.00	272.0
50.00	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB300

m/z	Abundance
36.00	516.0
37.00	2236.0
38.00	2466.0
39.10	1136.0
40.00	567.0
44.00	783.0
45.10	453.0
46.20	154.0
47.10	812.0
47.90	391.0
49.00	2341.0
50.00	10991.0
51.10	3281.0
52.00	135.0
53.80	231.0
54.90	129.0
56.10	1079.0
57.00	1676.0
60.00	522.0
61.00	2941.0
62.00	2815.0
63.00	2766.0
64.00	432.0
65.10	460.0
67.10	258.0
68.00	5638.0
69.00	5746.0
70.00	460.0
72.00	321.0
73.00	2860.0
74.10	10009.0
75.00	28616.0
76.00	2568.0
77.10	455.0
78.00	292.0
78.90	2424.0
79.90	615.0
80.90	2987.0
81.90	470.0
87.00	2565.0
88.00	2538.0
90.80	213.0
92.00	1632.0
93.00	2317.0
94.00	7602.0
95.00	57568.0
96.00	4137.0
97.00	110.0
103.80	298.0
105.10	138.0
105.90	358.0
109.80	109.0
115.80	343.0
116.90	514.0
117.90	365.0
118.90	534.0
128.00	244.0
129.00	106.0
129.90	300.0
130.90	194.0
135.00	153.0
141.10	578.0
142.90	1220.0
144.90	308.0
146.00	209.0
148.00	133.0
171.10	214.0
172.00	516.0
173.00	522.0
174.00	42848.0
175.00	3391.0
176.00	42040.0
177.10	2898.0
178.10	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB300

m/z	Abundance
36.10	541.0
37.00	2242.0
38.00	2438.0
39.00	1161.0
40.00	524.0
44.00	750.0
45.10	508.0
46.20	132.0
47.10	875.0
47.90	409.0
49.00	2540.0
50.00	10969.0
51.10	3331.0
52.00	152.0
52.80	115.0
53.80	197.0
55.00	152.0
56.10	1047.0
57.00	1702.0
60.00	545.0
61.00	2915.0
62.00	3093.0
63.00	2681.0
64.00	443.0
65.00	502.0
67.10	255.0
68.00	5691.0
69.10	5988.0
70.00	491.0
71.90	314.0
73.00	2948.0
74.10	9767.0
75.10	29360.0
76.00	2480.0
77.10	470.0
78.10	356.0
78.90	2594.0
79.90	693.0
80.90	3021.0
81.90	461.0
87.00	2789.0
88.00	2539.0
90.70	208.0
91.20	135.0
92.00	1574.0
93.00	2434.0
94.00	7249.0
95.00	59104.0
96.00	4003.0
103.90	321.0
104.90	117.0
105.90	332.0
109.90	103.0
115.80	360.0
116.90	531.0
117.90	400.0
118.90	649.0
127.90	272.0
128.90	125.0
129.90	222.0
130.90	204.0
135.00	153.0
136.80	128.0
141.10	564.0
142.90	1353.0
144.90	369.0
146.00	199.0
148.00	119.0
158.80	107.0
171.10	282.0
172.00	570.0
173.00	544.0
174.00	46288.0
175.00	3497.0
176.00	45048.0
177.00	2838.0
178.00	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB300

m/z	Abundance
36.10	509.0
37.00	2140.0
38.00	2295.0
39.00	1040.0
40.00	453.0
43.10	127.0
44.00	700.0
45.10	524.0
46.30	120.0
47.00	892.0
47.90	334.0
49.00	2397.0
50.00	9801.0
51.10	3077.0
52.00	145.0
52.80	157.0
53.90	126.0
55.00	168.0
56.00	886.0
57.10	1572.0
60.00	539.0
61.00	2642.0
62.00	2783.0
63.00	2242.0
64.00	427.0
65.00	535.0
67.00	271.0
68.00	5249.0
69.10	5691.0
70.00	514.0
71.90	300.0
73.00	2775.0
74.10	9128.0
75.10	27088.0
76.00	2193.0
77.00	463.0
78.00	456.0
78.90	2441.0
80.00	782.0
80.90	2606.0
81.90	482.0
87.00	2679.0
88.00	2346.0
90.70	201.0
91.20	162.0
92.00	1538.0
93.00	2388.0
94.00	6422.0
95.00	55616.0
96.00	3677.0
104.00	350.0
104.90	132.0
105.90	261.0
115.80	308.0
116.80	566.0
117.90	372.0
118.90	629.0
127.90	250.0
128.90	118.0
129.80	197.0
131.00	150.0
134.90	130.0
136.80	154.0
140.70	429.0
141.10	491.0
141.80	104.0
142.90	1203.0
144.90	397.0
146.00	152.0
148.00	140.0
158.80	108.0
171.00	262.0
171.90	545.0
173.00	498.0
174.00	45528.0
175.10	3210.0
176.00	43464.0
177.00	2640.0
177.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB300