


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV012219\
Data File : VV009228.D
Acq On : 22 Jan 2019 10:41
Operator : SY/MD
Sample : BFB
Misc : 5.00 G/5ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\82V012219S.M
Title : SW846 8260
Last Update : Wed Jan 23 01:54:58 2019

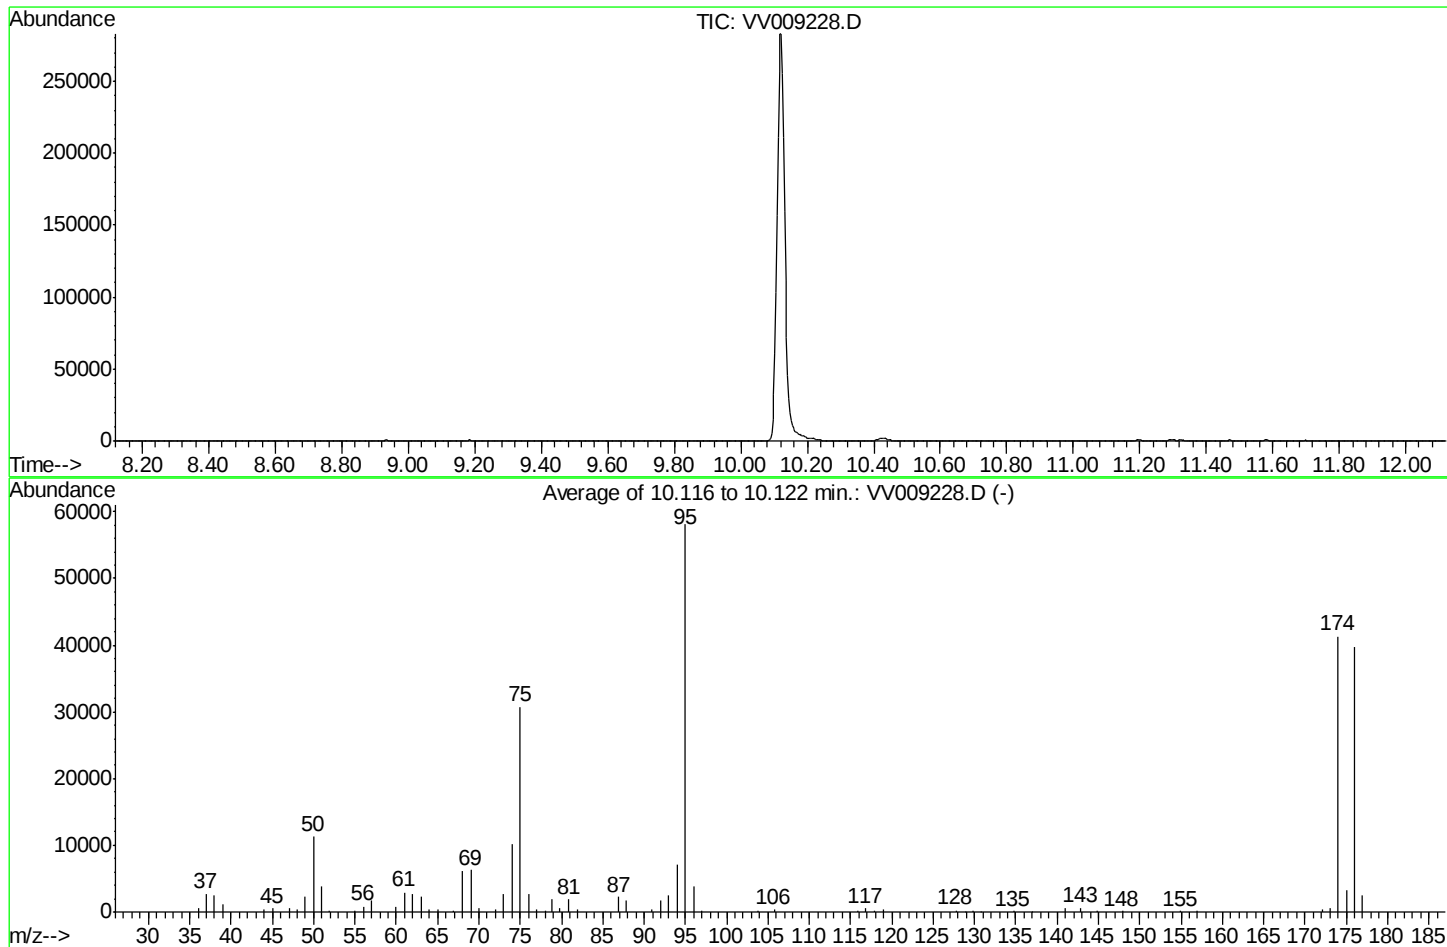

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	11291	PASS
75	95	30	60	52.9	30757	PASS
95	95	100	100	100.0	58109	PASS
96	95	5	9	6.8	3931	PASS
173	174	0.00	2	1.5	601	PASS
174	95	50	100	71.1	41336	PASS
175	174	5	9	7.7	3183	PASS
176	174	95	101	96.2	39773	PASS
177	176	5	9	6.3	2502	PASS