

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020133.D
 Acq On : 22 Jan 2021 13:53
 Operator : SY/MD
 Sample : VV0122WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK87

Quant Time: Jan 23 00:14:45 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jan 23 00:14:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.617	114	372567	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.855	117	352959	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.257	152	224832	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.309	65	157709	57.07	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 114.14%			
7) Chloroethane-d5	1.569	69	131547	56.87	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 113.74%			
11) 1,1-Dichloroethene-d2	2.106	63	239855	43.46	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 86.92%			
21) 2-Butanone-d5	3.891	46	188302	99.36	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 99.36%			
24) Chloroform-d	4.351	84	262783	50.77	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 101.54%			
26) 1,2-Dichloroethane-d4	5.035	65	189350	52.78	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 105.56%			
32) Benzene-d6	5.051	84	499357	51.37	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 102.74%			
36) 1,2-Dichloropropane-d6	6.071	67	183747	59.88	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 119.76%			
41) Toluene-d8	7.318	98	517919	57.27	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 114.54%			
43) trans-1,3-Dichloroprop...	7.624	79	78117	52.03	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 104.06%			
47) 2-Hexanone-d5	8.093	63	104446	81.88	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 81.88%			
57) 1,1,2,2-Tetrachloroeth...	10.222	84	209817	49.95	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 99.90%			
64) 1,2-Dichlorobenzene-d4	11.633	152	224010	53.02	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 106.04%			
Target Compounds					Qvalue	
48) 2-Hexanone	8.148	43	16436	5.11	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020133.D
Acq On : 22 Jan 2021 13:53
Operator : SY/MD
Sample : VV0122WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK87


Quant Time: Jan 23 00:14:45 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jan 23 00:14:09 2021
Response via : Initial Calibration

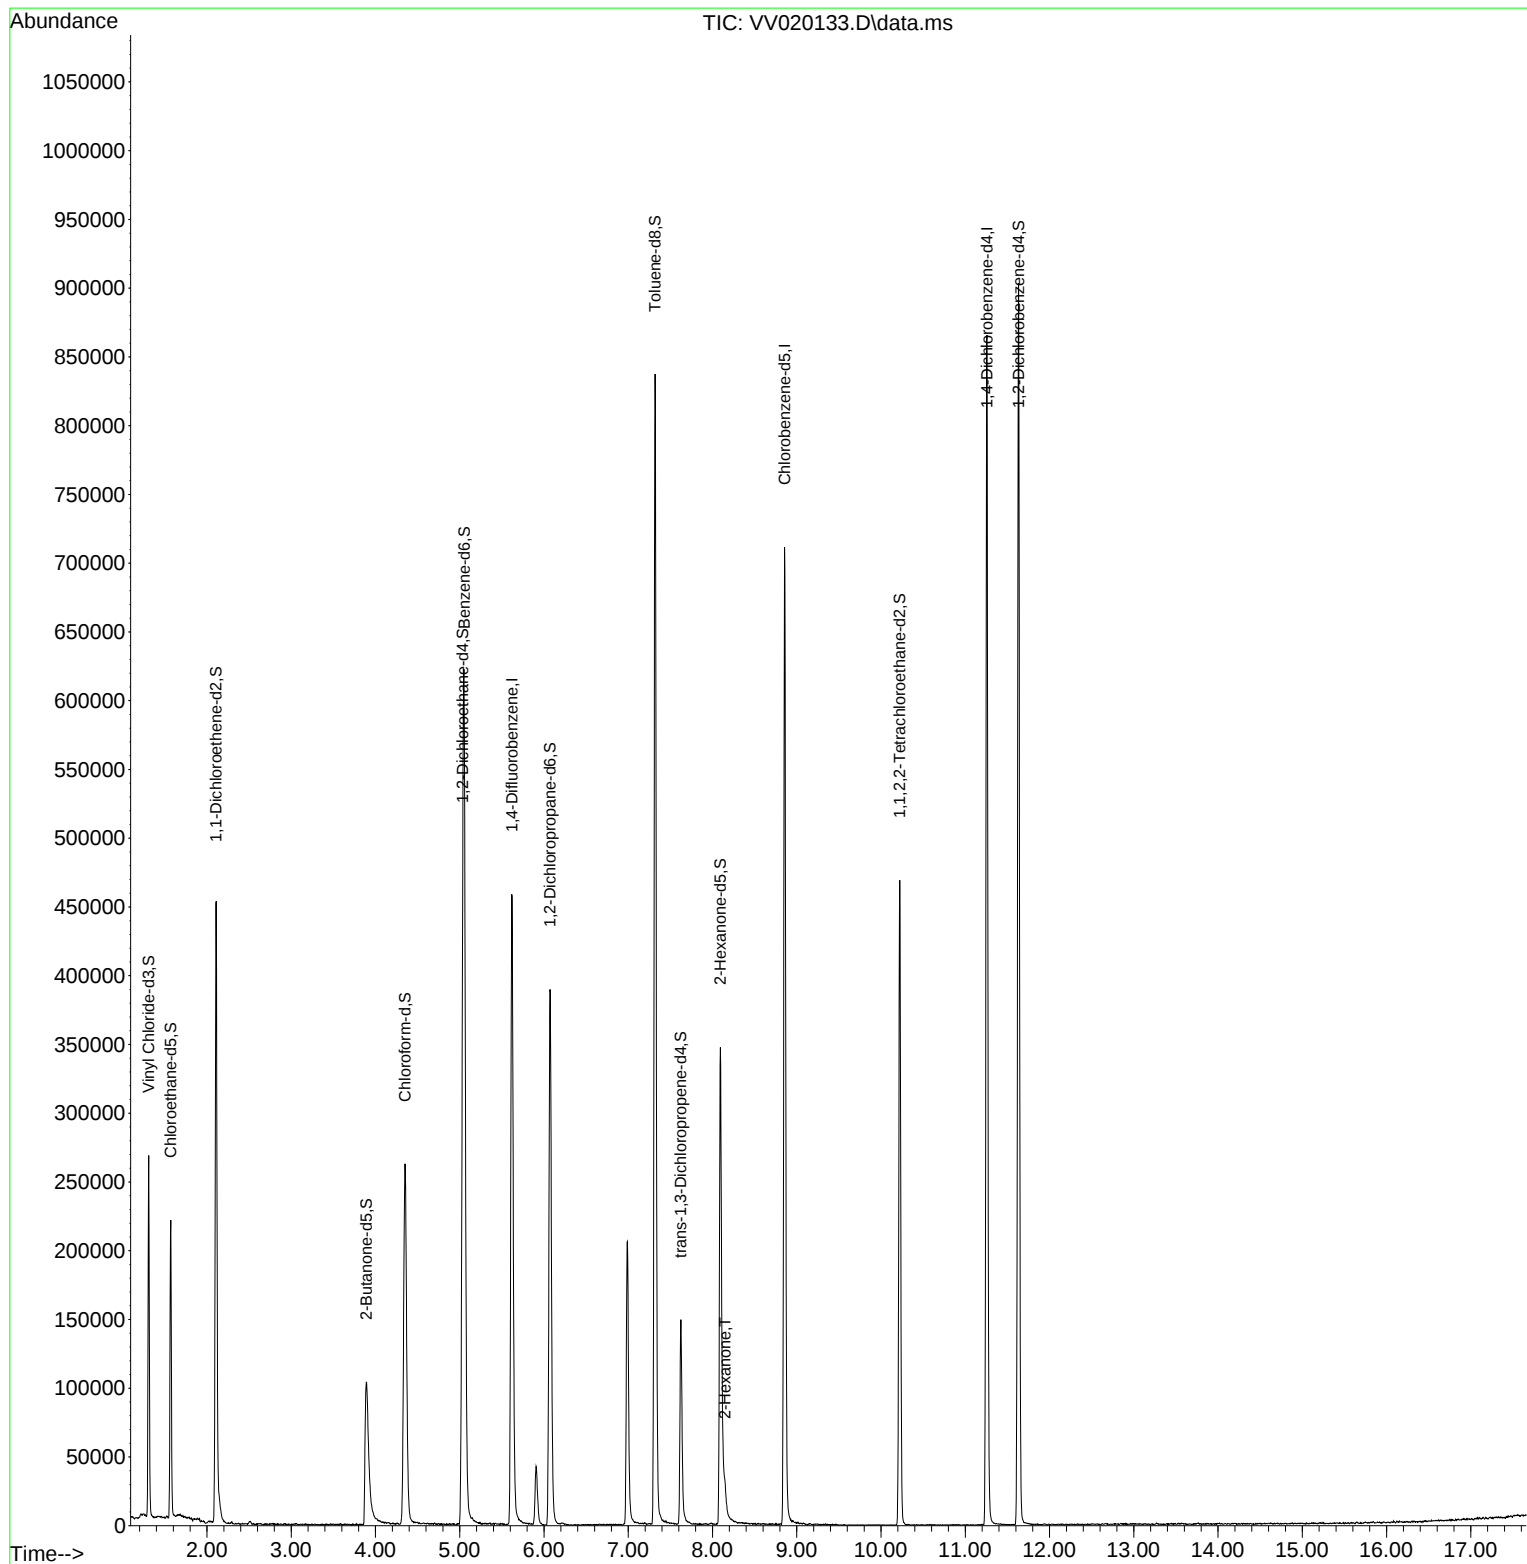

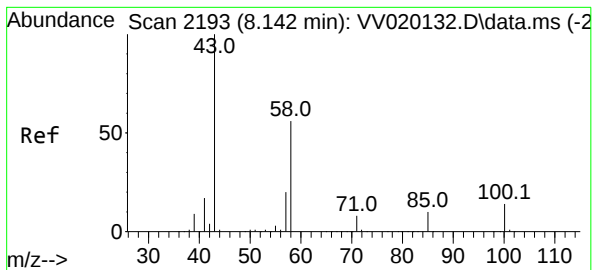

#48
 2-Hexanone
 Concen: 5.11 ug/L
 RT: 8.148 min Scan# 2195
 Delta R.T. 0.006 min
 Lab File: VV020133.D
 Acq: 22 Jan 2021 13:53

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK87

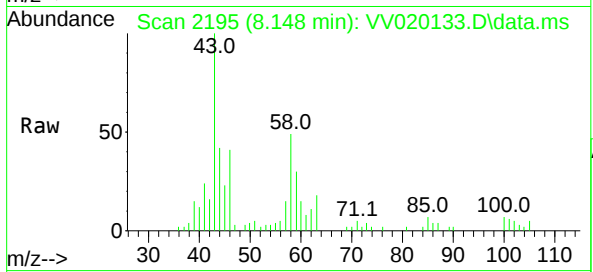

Tgt Ion: 43	Resp: 16436
Ion Ratio	Lower Upper
43	100
58	25.1 41.8 62.6#
57	4.4 15.0 22.4#
100	2.2 8.9 13.3#

