

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020133.D
 Acq On : 22 Jan 2021 13:53
 Operator : SY/MD
 Sample : VV0122WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020133.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	77	rBV	261747	261158	16.36%	2.006%
2	1.569	141	149	161	rBV	216471	246960	15.47%	1.897%
3	2.109	306	317	345	rBV	451024	684666	42.89%	5.258%
4	2.592	464	467	468	rBV	774	339	0.02%	0.003%
5	2.833	540	542	543	rBV	800	344	0.02%	0.003%
6	2.913	565	567	573	rBV3	702	702	0.04%	0.005%
7	3.003	593	595	598	rVB3	495	204	0.01%	0.002%
8	3.023	598	601	604	rBV2	615	451	0.03%	0.003%
9	3.354	701	704	705	rBV3	491	223	0.01%	0.002%
10	3.556	765	767	769	rVB2	611	220	0.01%	0.002%
11	3.569	769	771	772	rBV2	518	174	0.01%	0.001%
12	3.582	772	775	776	rBV	624	369	0.02%	0.003%
13	3.624	785	788	789	rBV3	479	248	0.02%	0.002%
14	3.662	798	800	803	rBV2	382	128	0.01%	0.001%
15	3.733	817	822	825	rVB2	848	735	0.05%	0.006%
16	3.753	825	828	830	rBV	413	273	0.02%	0.002%
17	3.772	830	834	836	rBV4	822	480	0.03%	0.004%
18	3.807	843	845	846	rBV2	518	210	0.01%	0.002%
19	3.891	861	871	904	rBV2	103170	320652	20.09%	2.463%
20	4.351	997	1014	1041	rBV	261881	649529	40.69%	4.988%
21	4.772	1143	1145	1147	rBV2	601	305	0.02%	0.002%
22	4.846	1166	1168	1170	rBV2	494	171	0.01%	0.001%
23	4.968	1203	1206	1209	rBV3	723	553	0.03%	0.004%
24	5.048	1214	1231	1258	rBV2	621810	1596378	100.00%	12.260%
25	5.402	1339	1341	1344	rVB3	978	539	0.03%	0.004%
26	5.418	1344	1346	1354	rBV7	996	1296	0.08%	0.010%
27	5.482	1364	1366	1368	rBV2	1095	590	0.04%	0.005%
28	5.524	1377	1379	1385	rVB4	911	725	0.05%	0.006%
29	5.556	1385	1389	1392	rBV3	661	617	0.04%	0.005%
30	5.617	1396	1408	1434	rBV	457743	927196	58.08%	7.121%
31	5.907	1486	1498	1516	rBV2	42003	85751	5.37%	0.659%
32	6.071	1536	1549	1580	rBV	389385	801455	50.20%	6.155%
33	6.357	1634	1638	1640	rBV	389	271	0.02%	0.002%
34	6.395	1647	1650	1651	rBV	269	122	0.01%	0.001%
35	6.444	1662	1665	1668	rBV2	266	234	0.01%	0.002%
36	6.489	1676	1679	1683	rBV2	365	320	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020133.D
 Acq On : 22 Jan 2021 13:53
 Operator : SY/MD
 Sample : VV0122WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	6.643	1722	1727	1728	rBV2	591	381	0.02%	0.003%
38	6.740	1753	1757	1758	rBV3	495	249	0.02%	0.002%
39	6.826	1782	1784	1788	rVB4	681	377	0.02%	0.003%
40	6.849	1788	1791	1796	rBV2	634	511	0.03%	0.004%
41	6.884	1800	1802	1804	rBV	426	184	0.01%	0.001%
42	6.929	1814	1816	1818	rBV2	200	127	0.01%	0.001%
43	6.945	1818	1821	1824	rBV3	826	785	0.05%	0.006%
44	6.990	1824	1835	1861	rVV	205580	379831	23.79%	2.917%
45	7.318	1925	1937	1964	rBV	836352	1435808	89.94%	11.027%
46	7.624	2021	2032	2052	rBV	148651	256741	16.08%	1.972%
47	7.846	2096	2101	2102	rBV3	1096	815	0.05%	0.006%
48	8.093	2168	2178	2218	rBV2	346027	706322	44.25%	5.425%
49	8.534	2311	2315	2317	rBV2	796	561	0.04%	0.004%
50	8.547	2317	2319	2326	rVB4	837	663	0.04%	0.005%
51	8.749	2380	2382	2386	rVB4	878	585	0.04%	0.004%
52	8.855	2404	2415	2437	rBV	710285	1154798	72.34%	8.869%
53	9.145	2500	2505	2506	rBV3	930	717	0.04%	0.006%
54	9.280	2546	2547	2550	rVB2	408	199	0.01%	0.002%
55	9.299	2550	2553	2554	rBV	373	203	0.01%	0.002%
56	9.415	2587	2589	2590	rBV2	272	124	0.01%	0.001%
57	9.424	2590	2592	2594	rVB	576	220	0.01%	0.002%
58	9.463	2602	2604	2609	rVB2	702	505	0.03%	0.004%
59	9.489	2609	2612	2616	rBV2	334	219	0.01%	0.002%
60	9.550	2628	2631	2633	rVB2	345	190	0.01%	0.001%
61	9.566	2633	2636	2641	rBV2	517	474	0.03%	0.004%
62	9.672	2665	2669	2671	rBV2	207	160	0.01%	0.001%
63	9.717	2677	2683	2687	rBV2	334	240	0.02%	0.002%
64	9.739	2688	2690	2694	rBV	155	121	0.01%	0.001%
65	9.775	2697	2701	2706	rBV2	386	464	0.03%	0.004%
66	9.823	2713	2716	2719	rBV2	195	127	0.01%	0.001%
67	9.874	2730	2732	2736	rBV2	270	243	0.02%	0.002%
68	9.897	2738	2739	2741	rVB	229	50	0.00%	0.000%
69	9.910	2741	2743	2744	rBV	178	76	0.00%	0.001%
70	9.961	2756	2759	2762	rBV	203	198	0.01%	0.002%
71	10.222	2827	2840	2861	rBV	468953	720430	45.13%	5.533%
72	10.370	2881	2886	2890	rBV2	329	310	0.02%	0.002%
73	10.392	2890	2893	2898	rVB3	313	325	0.02%	0.002%
74	10.530	2933	2936	2938	rBV	245	195	0.01%	0.001%
75	10.636	2966	2969	2974	rBV2	378	393	0.02%	0.003%
76	10.733	2994	2999	3002	rBV2	372	296	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020133.D
 Acq On : 22 Jan 2021 13:53
 Operator : SY/MD
 Sample : VV0122WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

77	10.842	3032	3033	3034	rBV	225	73	0.00%	0.001%
78	10.974	3072	3074	3076	rBV	207	125	0.01%	0.001%
79	11.064	3100	3102	3105	rBV	303	184	0.01%	0.001%
80	11.112	3115	3117	3120	rBV	184	103	0.01%	0.001%
81	11.186	3138	3140	3141	rBV	405	145	0.01%	0.001%
82	11.257	3150	3162	3188	rBV	865225	1356629	84.98%	10.419%
83	11.630	3266	3278	3302	rBV	902457	1411272	88.40%	10.839%
84	12.128	3431	3433	3436	rBV	400	258	0.02%	0.002%
85	12.296	3483	3485	3488	rBV2	394	195	0.01%	0.001%
86	13.070	3723	3726	3727	rBV2	619	324	0.02%	0.002%
87	13.968	4002	4005	4007	rBV2	633	346	0.02%	0.003%
88	14.469	4159	4161	4165	rBV4	701	612	0.04%	0.005%
89	15.048	4339	4341	4346	rBV4	930	837	0.05%	0.006%




Sum of corrected areas: 13020908

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020133.D
Acq On : 22 Jan 2021 13:53
Operator : SY/MD
Sample : VV0122WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

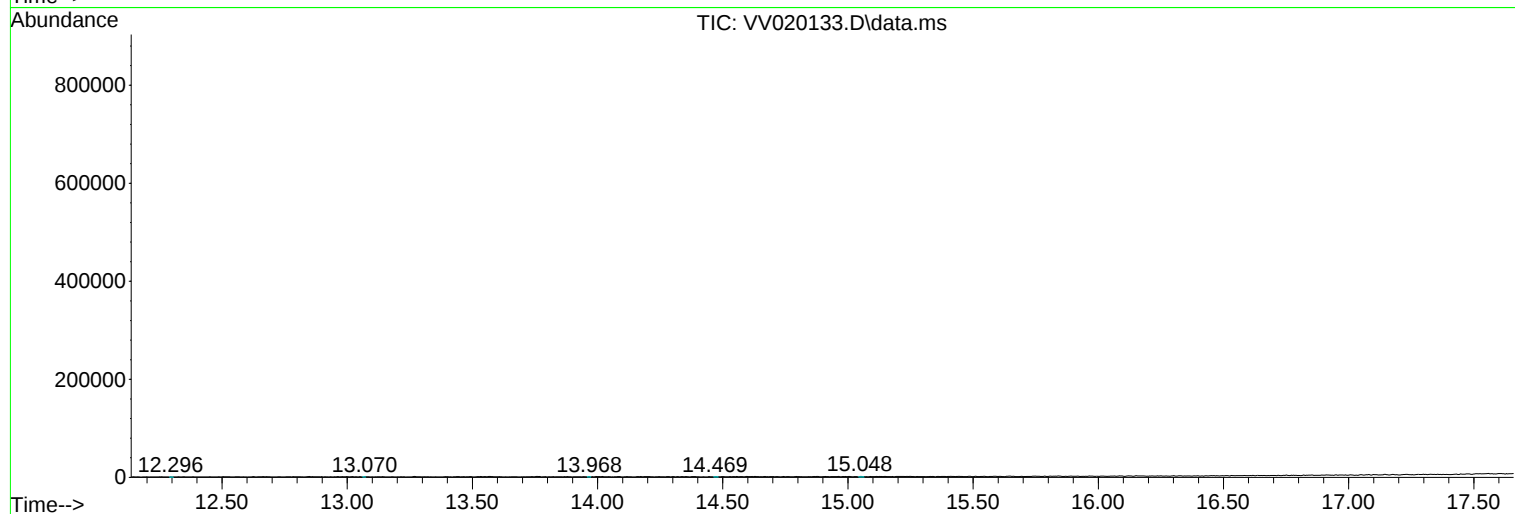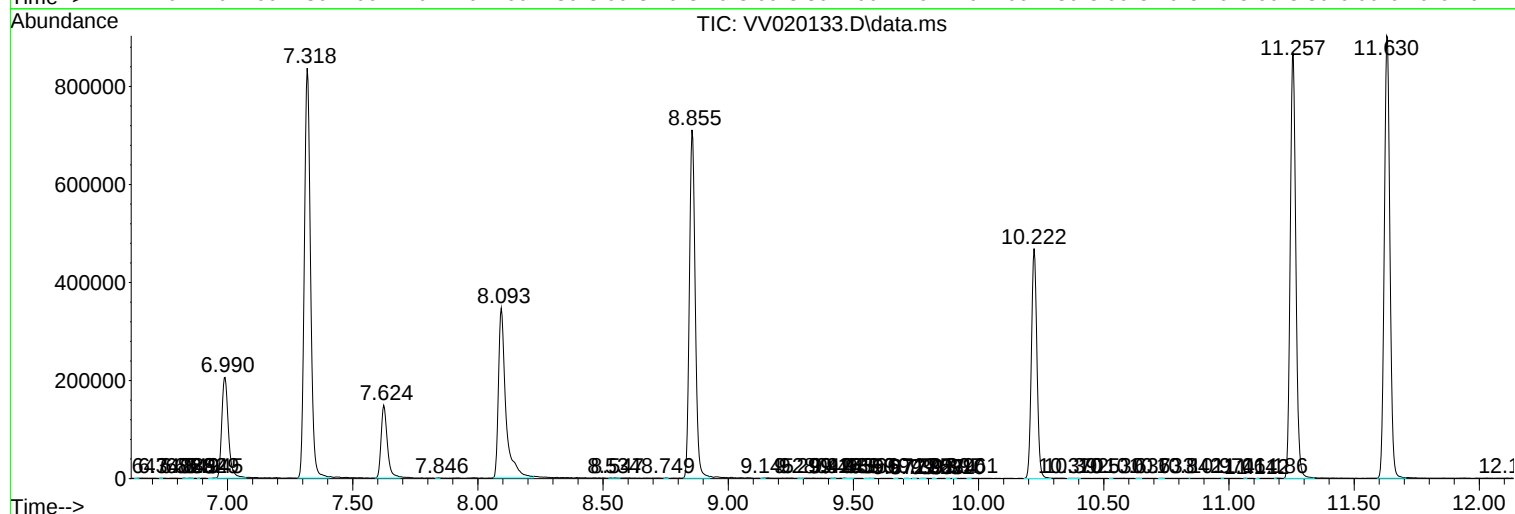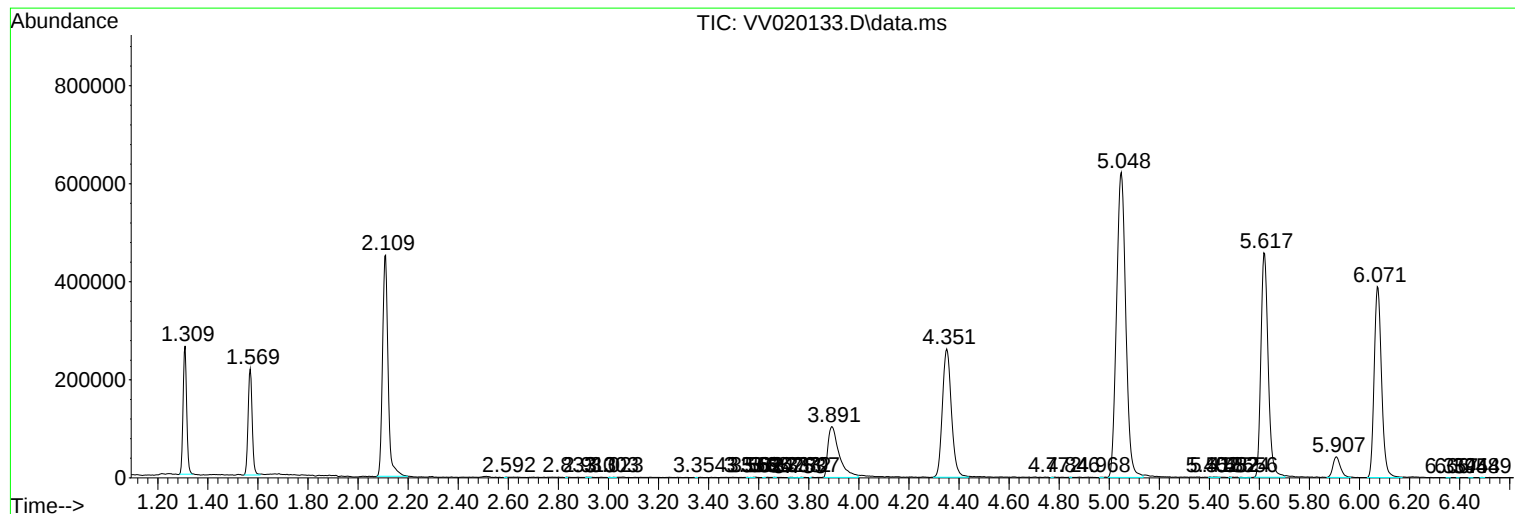

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020133.D
Acq On : 22 Jan 2021 13:53
Operator : SY/MD
Sample : VV0122WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020133.D
Acq On : 22 Jan 2021 13:53
Operator : SY/MD
Sample : VV0122WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
