

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020136.D
 Acq On : 22 Jan 2021 15:28
 Operator : SY/MD
 Sample : M1181-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020136.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	81	rVB	272217	269906	15.52%	1.934%
2	1.569	142	149	162	rVB	207780	232355	13.36%	1.665%
3	2.109	307	317	343	rVB	447146	671162	38.60%	4.810%
4	2.434	415	418	420	rBV2	592	283	0.02%	0.002%
5	2.499	435	438	439	rBV2	935	522	0.03%	0.004%
6	2.605	468	471	477	rVB4	866	786	0.05%	0.006%
7	2.653	483	486	489	rVB3	591	330	0.02%	0.002%
8	2.672	489	492	493	rBV3	865	517	0.03%	0.004%
9	2.717	503	506	510	rBV3	616	326	0.02%	0.002%
10	2.769	513	522	530	rBV8	2664	4566	0.26%	0.033%
11	2.814	535	536	540	rVB3	951	366	0.02%	0.003%
12	2.836	540	543	544	rBV	519	303	0.02%	0.002%
13	2.926	569	571	575	rVB4	334	189	0.01%	0.001%
14	2.949	576	578	583	rVB5	636	274	0.02%	0.002%
15	2.997	591	593	596	rBV	438	156	0.01%	0.001%
16	3.116	629	630	632	rBV	331	154	0.01%	0.001%
17	3.154	639	642	644	rVB2	587	295	0.02%	0.002%
18	3.167	644	646	649	rVB2	837	319	0.02%	0.002%
19	3.193	649	654	657	rBV4	898	731	0.04%	0.005%
20	3.212	657	660	662	rBV3	523	315	0.02%	0.002%
21	3.277	676	680	681	rBV	394	250	0.01%	0.002%
22	3.322	691	694	698	rVV3	352	279	0.02%	0.002%
23	3.505	749	751	752	rBV	410	216	0.01%	0.002%
24	3.572	769	772	779	rVB6	729	893	0.05%	0.006%
25	3.605	779	782	784	rBV2	273	182	0.01%	0.001%
26	3.656	796	798	802	rBV2	493	404	0.02%	0.003%
27	3.743	822	825	828	rVB3	424	182	0.01%	0.001%
28	3.762	828	831	833	rBV2	310	181	0.01%	0.001%
29	3.839	853	855	856	rBV2	457	224	0.01%	0.002%
30	3.894	858	872	904	rBV2	120996	482679	27.76%	3.459%
31	4.286	992	994	997	rBV2	790	384	0.02%	0.003%
32	4.354	997	1015	1042	rBV	273892	681925	39.22%	4.887%
33	4.650	1103	1107	1115	rBV7	945	1141	0.07%	0.008%
34	4.682	1115	1117	1119	rVB2	752	339	0.02%	0.002%
35	4.749	1136	1138	1140	rBV	324	180	0.01%	0.001%
36	4.865	1171	1174	1175	rBV2	675	302	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020136.D
 Acq On : 22 Jan 2021 15:28
 Operator : SY/MD
 Sample : M1181-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	4.923	1188	1192	1193	rBV2	396	304	0.02%	0.002%
38	4.936	1194	1196	1200	rVV3	453	323	0.02%	0.002%
39	4.978	1205	1209	1211	rBV	498	291	0.02%	0.002%
40	5.048	1211	1231	1258	rBV2	672414	1738557	100.00%	12.461%
41	5.299	1306	1309	1312	rBV3	1084	590	0.03%	0.004%
42	5.444	1351	1354	1355	rBV	465	291	0.02%	0.002%
43	5.466	1359	1361	1363	rBV3	492	235	0.01%	0.002%
44	5.547	1384	1386	1390	rBV4	528	288	0.02%	0.002%
45	5.617	1394	1408	1436	rBV	474633	963365	55.41%	6.905%
46	5.913	1487	1500	1518	rBV5	56720	140547	8.08%	1.007%
47	6.074	1536	1550	1570	rBV	385709	792624	45.59%	5.681%
48	6.431	1659	1661	1662	rVB2	518	144	0.01%	0.001%
49	6.550	1696	1698	1701	rVB3	664	287	0.02%	0.002%
50	6.765	1761	1765	1768	rBV4	623	450	0.03%	0.003%
51	6.839	1784	1788	1790	rBV	715	605	0.03%	0.004%
52	6.868	1794	1797	1800	rVB4	720	445	0.03%	0.003%
53	6.945	1818	1821	1822	rBV	440	259	0.01%	0.002%
54	6.987	1823	1834	1860	rVV	187424	343715	19.77%	2.463%
55	7.318	1925	1937	1958	rBV	700490	1215181	69.90%	8.709%
56	7.585	2018	2020	2022	rBV3	345	192	0.01%	0.001%
57	7.624	2022	2032	2052	rBV2	150767	261129	15.02%	1.872%
58	7.977	2129	2142	2161	rBV	599446	1007257	57.94%	7.219%
59	8.093	2168	2178	2208	rBV2	329814	648637	37.31%	4.649%
60	8.572	2325	2327	2330	rBV3	535	384	0.02%	0.003%
61	8.855	2403	2415	2438	rBV	869902	1384992	79.66%	9.926%
62	9.193	2518	2520	2527	rBV3	634	392	0.02%	0.003%
63	9.286	2547	2549	2551	rBV	508	218	0.01%	0.002%
64	9.309	2554	2556	2558	rBV3	449	225	0.01%	0.002%
65	9.360	2569	2572	2576	rVB4	685	414	0.02%	0.003%
66	9.379	2576	2578	2583	rBV3	533	369	0.02%	0.003%
67	9.466	2603	2605	2614	rVB8	627	629	0.04%	0.005%
68	9.511	2617	2619	2621	rBV	535	339	0.02%	0.002%
69	9.736	2687	2689	2690	rBV	540	245	0.01%	0.002%
70	9.804	2707	2710	2712	rBV	655	411	0.02%	0.003%
71	9.923	2741	2747	2749	rBV5	991	857	0.05%	0.006%
72	10.061	2787	2790	2796	rBV5	618	458	0.03%	0.003%
73	10.112	2804	2806	2811	rVB2	831	430	0.02%	0.003%
74	10.148	2813	2817	2822	rBV3	700	709	0.04%	0.005%
75	10.222	2828	2840	2862	rBV	471286	742061	42.68%	5.318%
76	10.389	2884	2892	2902	rVB4	2780	4918	0.28%	0.035%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020136.D
 Acq On : 22 Jan 2021 15:28
 Operator : SY/MD
 Sample : M1181-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

77	10.427	2902	2904	2906	rBV2	628	327	0.02%	0.002%
78	10.569	2944	2948	2949	rBV2	482	283	0.02%	0.002%
79	10.672	2978	2980	2983	rBV	293	192	0.01%	0.001%
80	10.765	3006	3009	3011	rBV2	878	607	0.03%	0.004%
81	10.788	3014	3016	3020	rVB2	469	230	0.01%	0.002%
82	10.894	3047	3049	3050	rVB	697	208	0.01%	0.001%
83	10.919	3056	3057	3059	rBV	576	217	0.01%	0.002%
84	10.987	3076	3078	3081	rBV3	553	343	0.02%	0.002%
85	11.080	3102	3107	3108	rBV3	840	702	0.04%	0.005%
86	11.254	3150	3161	3183	rBV	773391	1201544	69.11%	8.612%
87	11.534	3246	3248	3250	rBV2	522	279	0.02%	0.002%
88	11.630	3266	3278	3298	rBV	718584	1135360	65.30%	8.137%
89	12.183	3448	3450	3454	rBV2	762	444	0.03%	0.003%
90	12.353	3500	3503	3507	rBV2	351	329	0.02%	0.002%
91	12.460	3531	3536	3540	rBV3	422	477	0.03%	0.003%
92	13.144	3745	3749	3750	rBV2	417	287	0.02%	0.002%
93	13.193	3760	3764	3766	rBV	270	236	0.01%	0.002%
94	13.312	3798	3801	3804	rBV4	558	438	0.03%	0.003%
95	13.578	3882	3884	3885	rBV2	374	163	0.01%	0.001%
96	13.964	4000	4004	4006	rBV3	662	455	0.03%	0.003%
97	14.077	4036	4039	4043	rVB2	847	540	0.03%	0.004%
98	14.154	4060	4063	4064	rVB2	758	268	0.02%	0.002%
99	14.382	4132	4134	4137	rBV2	495	229	0.01%	0.002%
100	14.585	4194	4197	4203	rBV4	997	968	0.06%	0.007%




Sum of corrected areas: 13952509

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020136.D
Acq On : 22 Jan 2021 15:28
Operator : SY/MD
Sample : M1181-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

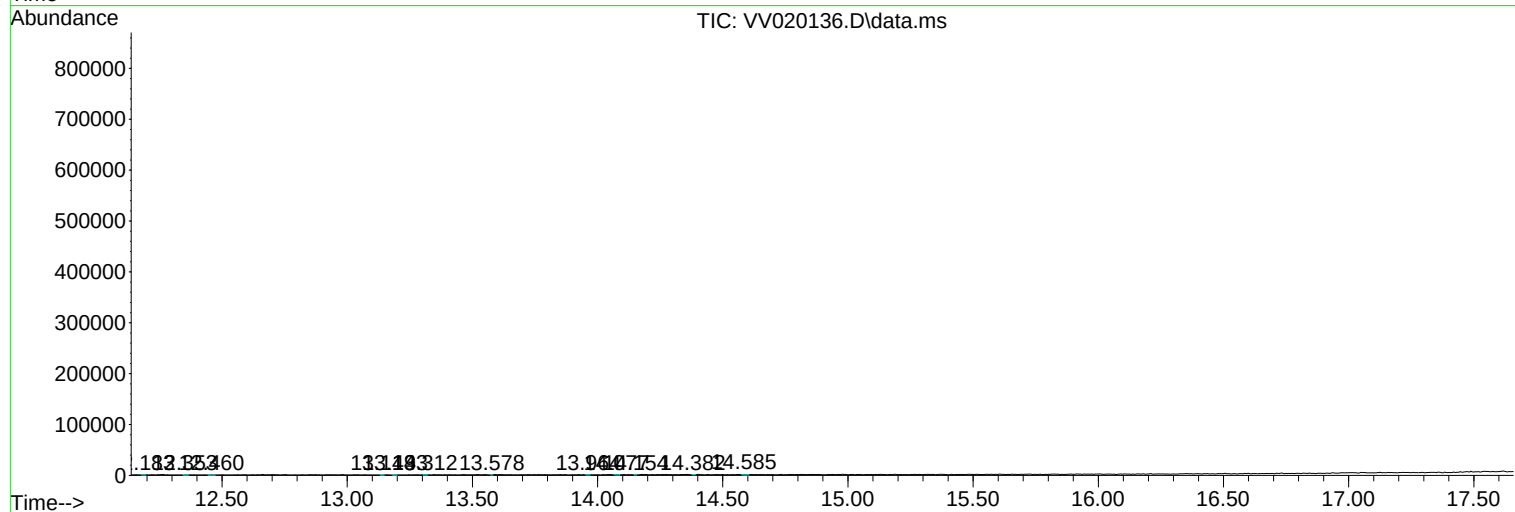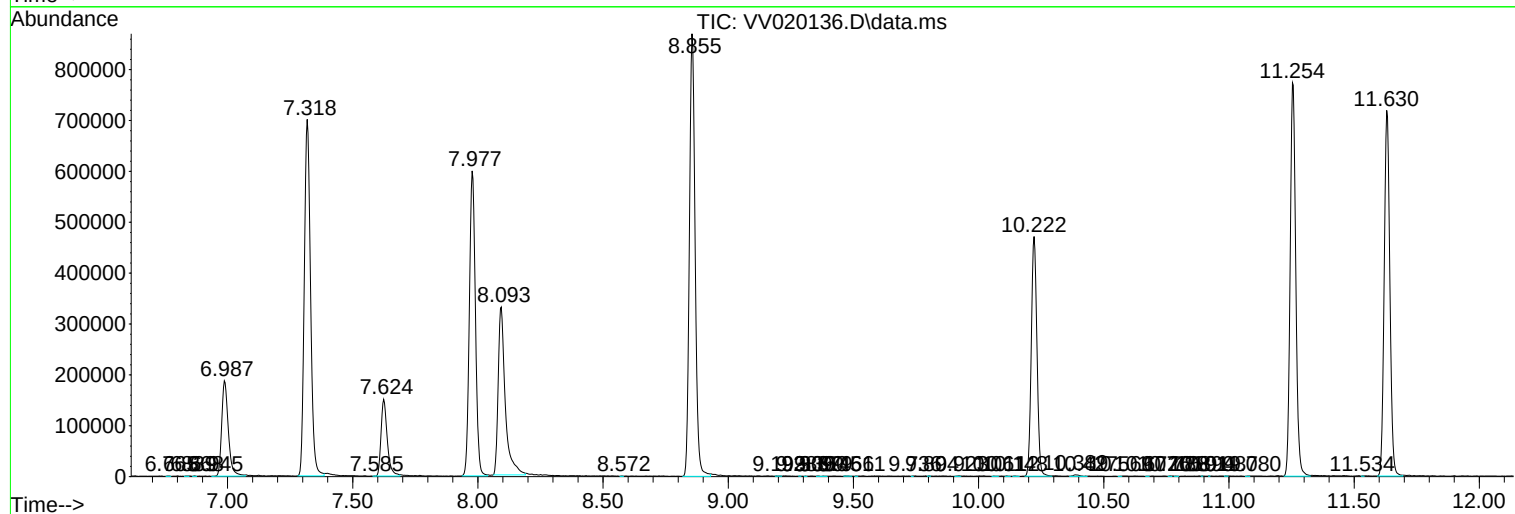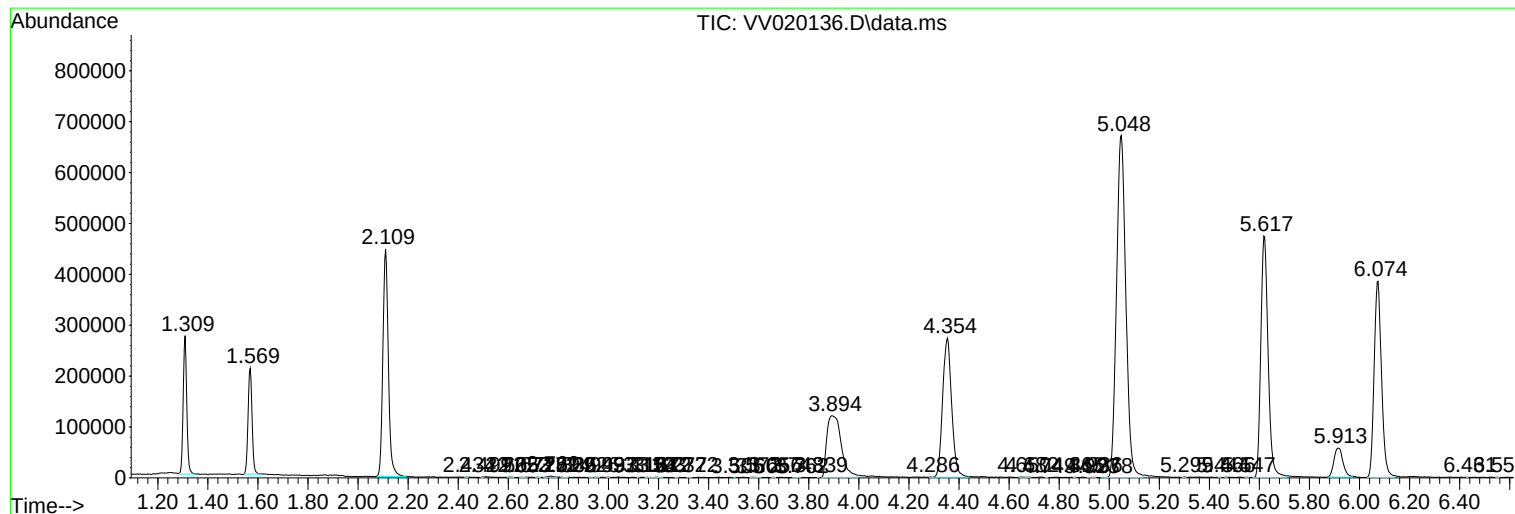

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020136.D
Acq On : 22 Jan 2021 15:28
Operator : SY/MD
Sample : M1181-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020136.D
Acq On : 22 Jan 2021 15:28
Operator : SY/MD
Sample : M1181-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
