

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020137.D
 Acq On : 22 Jan 2021 15:51
 Operator : SY/MD
 Sample : M1181-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	82	rVB	219691	222428	15.33%	1.690%
2	1.569	142	149	161	rBV	179938	204302	14.08%	1.552%
3	2.109	307	317	350	rVB	392197	596621	41.11%	4.532%
4	2.383	400	402	404	rBV2	775	348	0.02%	0.003%
5	2.627	476	478	481	rBV3	581	371	0.03%	0.003%
6	2.666	486	490	492	rBV4	719	503	0.03%	0.004%
7	2.852	546	548	550	rBV2	475	224	0.02%	0.002%
8	3.003	593	595	598	rBV3	588	396	0.03%	0.003%
9	3.122	630	632	634	rBV	390	207	0.01%	0.002%
10	3.171	643	647	651	rVB3	192	159	0.01%	0.001%
11	3.193	651	654	655	rBV2	387	227	0.02%	0.002%
12	3.228	663	665	667	rBV	484	209	0.01%	0.002%
13	3.341	695	700	702	rBV2	477	356	0.02%	0.003%
14	3.389	713	715	717	rBV	329	154	0.01%	0.001%
15	3.482	741	744	748	rBV3	313	277	0.02%	0.002%
16	3.553	762	766	767	rBV2	428	189	0.01%	0.001%
17	3.589	773	777	778	rBV2	416	338	0.02%	0.003%
18	3.630	786	790	795	rBV3	754	623	0.04%	0.005%
19	3.659	795	799	805	rBV4	428	614	0.04%	0.005%
20	3.685	805	807	812	rVB3	572	267	0.02%	0.002%
21	3.733	818	822	824	rBV3	281	233	0.02%	0.002%
22	3.778	834	836	839	rVB	536	262	0.02%	0.002%
23	3.839	853	855	857	rBV	514	245	0.02%	0.002%
24	3.904	861	875	876	rBV	124818	230461	15.88%	1.751%
25	4.354	1000	1015	1037	rBV	235574	586998	40.45%	4.459%
26	4.682	1115	1117	1119	rBV2	554	228	0.02%	0.002%
27	4.724	1127	1130	1135	rVB3	654	462	0.03%	0.004%
28	4.785	1141	1149	1152	rBV6	552	680	0.05%	0.005%
29	4.839	1162	1166	1170	rBV3	577	511	0.04%	0.004%
30	4.900	1183	1185	1190	rVB3	931	448	0.03%	0.003%
31	4.936	1193	1196	1197	rBV	464	255	0.02%	0.002%
32	5.051	1215	1232	1265	rBV2	555530	1445688	99.62%	10.982%
33	5.469	1360	1362	1364	rBV	436	169	0.01%	0.001%
34	5.505	1370	1373	1375	rBV2	688	484	0.03%	0.004%
35	5.621	1397	1409	1433	rBV	464240	930861	64.14%	7.071%
36	5.846	1477	1479	1482	rBV3	397	292	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020137.D
 Acq On : 22 Jan 2021 15:51
 Operator : SY/MD
 Sample : M1181-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	5.920	1487	1502	1526	rVV5	84063	195875	13.50%	1.488%
38	6.077	1537	1551	1577	rBV	346640	701853	48.36%	5.332%
39	6.325	1626	1628	1631	rBV3	418	256	0.02%	0.002%
40	6.344	1631	1634	1638	rVB2	752	574	0.04%	0.004%
41	6.373	1638	1643	1646	rBV5	724	655	0.05%	0.005%
42	6.476	1673	1675	1678	rBV	419	269	0.02%	0.002%
43	6.566	1700	1703	1704	rBV	230	131	0.01%	0.001%
44	6.601	1711	1714	1715	rBV2	253	168	0.01%	0.001%
45	6.627	1721	1722	1725	rVB	638	191	0.01%	0.001%
46	6.649	1725	1729	1731	rBV2	853	857	0.06%	0.007%
47	6.923	1812	1814	1815	rBV	649	201	0.01%	0.002%
48	6.990	1824	1835	1857	rBV	182975	333174	22.96%	2.531%
49	7.186	1893	1896	1898	rBV3	847	490	0.03%	0.004%
50	7.244	1910	1914	1918	rVB3	647	644	0.04%	0.005%
51	7.276	1922	1924	1925	rBV2	435	184	0.01%	0.001%
52	7.321	1926	1938	1961	rBV	702666	1233245	84.98%	9.368%
53	7.627	2023	2033	2053	rBV	127093	221444	15.26%	1.682%
54	7.820	2091	2093	2096	rBV2	781	483	0.03%	0.004%
55	7.884	2111	2113	2115	rVB	406	168	0.01%	0.001%
56	7.981	2129	2143	2165	rBV	872503	1451186	100.00%	11.024%
57	8.093	2169	2178	2214	rVV2	323856	650629	44.83%	4.942%
58	8.534	2311	2315	2320	rBV5	1037	1194	0.08%	0.009%
59	8.559	2320	2323	2324	rBV	383	193	0.01%	0.001%
60	8.588	2330	2332	2334	rBV3	703	399	0.03%	0.003%
61	8.736	2375	2378	2381	rVB2	605	360	0.02%	0.003%
62	8.752	2381	2383	2384	rBV2	475	173	0.01%	0.001%
63	8.784	2390	2393	2394	rBV2	537	381	0.03%	0.003%
64	8.858	2403	2416	2438	rBV	801087	1307829	90.12%	9.935%
65	9.064	2478	2480	2484	rBV3	724	478	0.03%	0.004%
66	9.100	2489	2491	2494	rBV3	719	402	0.03%	0.003%
67	9.225	2527	2530	2533	rBV2	874	454	0.03%	0.003%
68	9.334	2562	2564	2566	rBV2	513	306	0.02%	0.002%
69	9.366	2571	2574	2575	rBV	439	225	0.02%	0.002%
70	9.424	2590	2592	2595	rBV3	499	303	0.02%	0.002%
71	9.665	2665	2667	2671	rBV3	459	222	0.02%	0.002%
72	9.871	2728	2731	2732	rBV3	488	279	0.02%	0.002%
73	9.903	2739	2741	2743	rBV	605	350	0.02%	0.003%
74	9.961	2757	2759	2760	rBV	415	139	0.01%	0.001%
75	10.087	2796	2798	2804	rVB3	200	162	0.01%	0.001%
76	10.164	2815	2822	2823	rBV2	382	326	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020137.D
 Acq On : 22 Jan 2021 15:51
 Operator : SY/MD
 Sample : M1181-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

77	10.222	2828	2840	2865	rVB	425351	670783	46.22%	5.096%
78	10.309	2865	2867	2868	rBV2	417	171	0.01%	0.001%
79	10.325	2868	2872	2874	rBV3	454	466	0.03%	0.004%
80	10.466	2913	2916	2919	rBV2	546	333	0.02%	0.003%
81	10.582	2948	2952	2954	rBV2	902	779	0.05%	0.006%
82	10.659	2974	2976	2978	rBV	403	241	0.02%	0.002%
83	10.698	2986	2988	2991	rBV2	517	258	0.02%	0.002%
84	10.746	3000	3003	3004	rBV	246	140	0.01%	0.001%
85	10.755	3004	3006	3010	rVV2	497	319	0.02%	0.002%
86	10.948	3064	3066	3068	rBV	328	182	0.01%	0.001%
87	11.061	3099	3101	3104	rVB2	675	338	0.02%	0.003%
88	11.099	3109	3113	3116	rBV3	680	491	0.03%	0.004%
89	11.257	3147	3162	3183	rBV	732433	1137087	78.36%	8.638%
90	11.633	3267	3279	3296	rBV	639305	1014609	69.92%	7.707%
91	11.932	3370	3372	3376	rVB	945	492	0.03%	0.004%
92	11.948	3376	3377	3379	rBV	612	209	0.01%	0.002%
93	12.858	3658	3660	3661	rBV	352	166	0.01%	0.001%
94	13.013	3705	3708	3710	rBV	674	463	0.03%	0.004%
95	13.524	3863	3867	3869	rBV3	872	691	0.05%	0.005%
96	13.591	3885	3888	3889	rBV2	753	334	0.02%	0.003%
97	13.787	3947	3949	3951	rVB2	843	311	0.02%	0.002%
98	13.800	3951	3953	3955	rBV	592	168	0.01%	0.001%
99	13.884	3978	3979	3984	rBV4	538	424	0.03%	0.003%
100	13.964	4002	4004	4011	rBV4	969	643	0.04%	0.005%




Sum of corrected areas: 13164040

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020137.D
Acq On : 22 Jan 2021 15:51
Operator : SY/MD
Sample : M1181-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

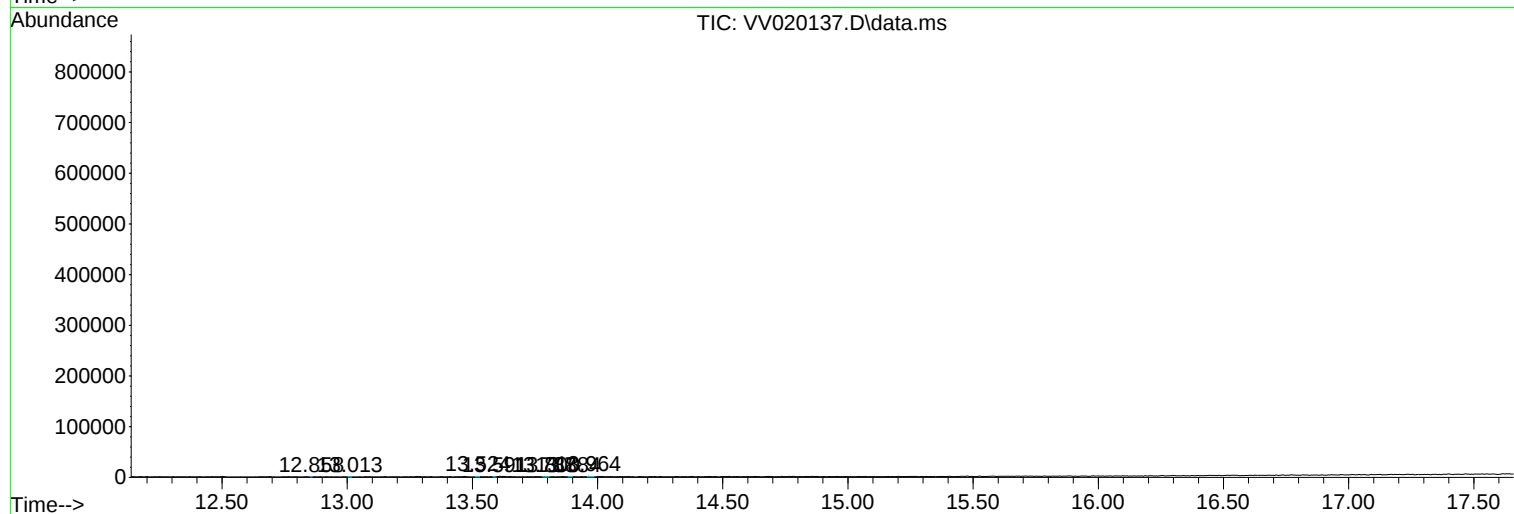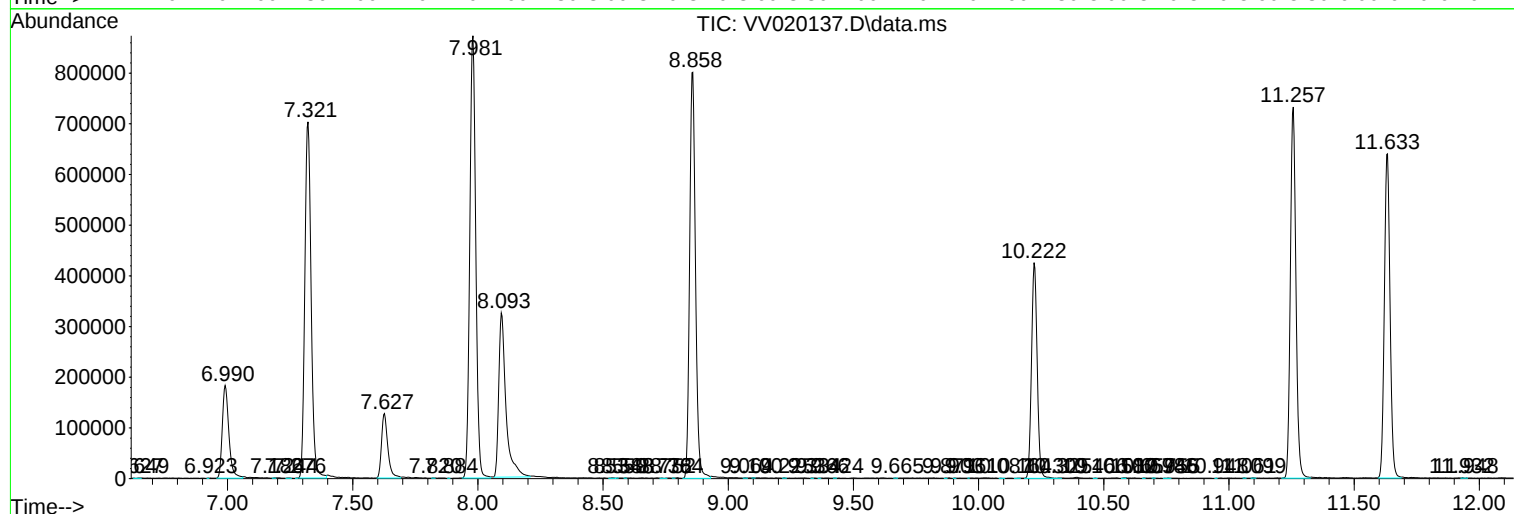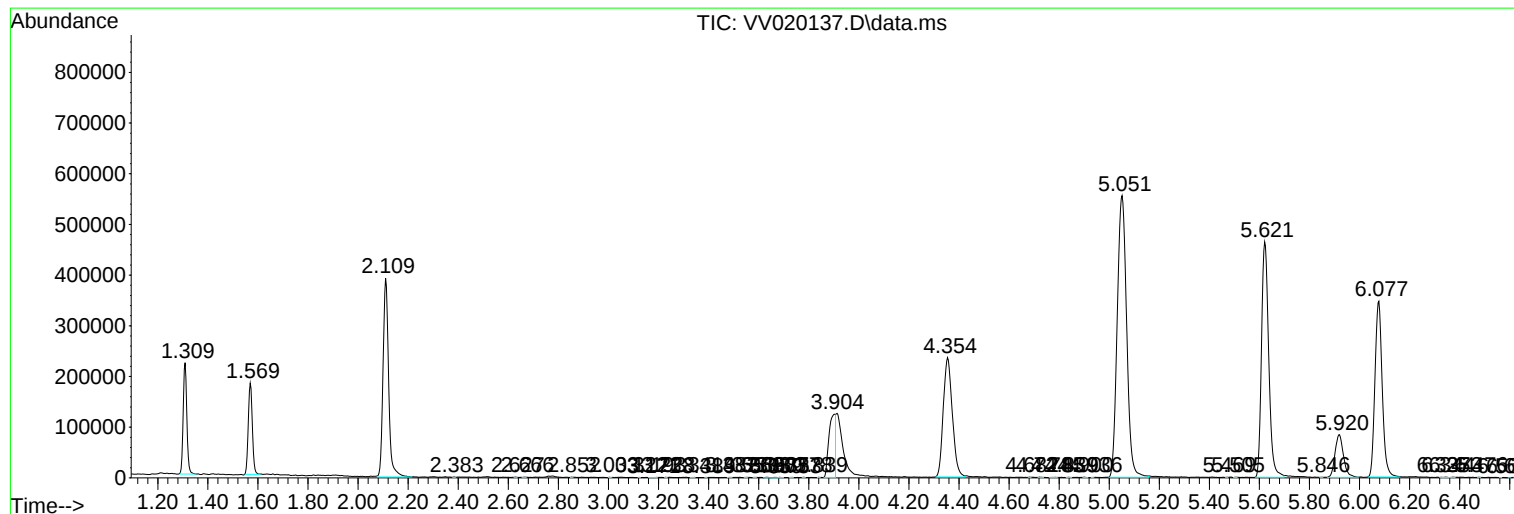

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020137.D
Acq On : 22 Jan 2021 15:51
Operator : SY/MD
Sample : M1181-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020137.D
Acq On : 22 Jan 2021 15:51
Operator : SY/MD
Sample : M1181-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
