

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020138.D
 Acq On : 22 Jan 2021 16:15
 Operator : SY/MD
 Sample : M1181-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020138.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	83	rVB	204074	203398	14.97%	1.836%
2	1.569	142	149	162	rBV	170189	188635	13.88%	1.702%
3	2.110	307	317	337	rBV	337566	505461	37.20%	4.562%
4	2.949	574	578	579	rBV	342	236	0.02%	0.002%
5	2.971	582	585	588	rBV3	579	532	0.04%	0.005%
6	3.065	612	614	616	rBV	430	204	0.02%	0.002%
7	3.110	622	628	631	rBV4	721	746	0.05%	0.007%
8	3.245	667	670	675	rVB5	894	530	0.04%	0.005%
9	3.270	675	678	681	rBV2	820	580	0.04%	0.005%
10	3.296	684	686	689	rBV2	567	306	0.02%	0.003%
11	3.447	731	733	738	rVB4	1029	593	0.04%	0.005%
12	3.579	773	774	776	rBV2	383	130	0.01%	0.001%
13	3.618	783	786	790	rVB5	868	602	0.04%	0.005%
14	3.637	790	792	794	rVB	445	212	0.02%	0.002%
15	3.663	794	800	805	rBV2	662	980	0.07%	0.009%
16	3.682	805	806	810	rVB	655	276	0.02%	0.002%
17	3.698	810	811	814	rVB2	263	122	0.01%	0.001%
18	3.724	814	819	820	rBV2	462	308	0.02%	0.003%
19	3.823	846	850	852	rBV3	503	361	0.03%	0.003%
20	3.852	858	859	860	rBV3	364	117	0.01%	0.001%
21	3.894	860	872	903	rVV2	87918	304856	22.43%	2.751%
22	4.354	997	1015	1041	rBV	218589	544949	40.10%	4.918%
23	4.711	1125	1126	1127	rBV	180	51	0.00%	0.000%
24	4.730	1127	1132	1133	rBV3	556	469	0.03%	0.004%
25	4.846	1166	1168	1174	rBV2	766	639	0.05%	0.006%
26	4.917	1189	1190	1192	rVB2	446	105	0.01%	0.001%
27	4.978	1208	1209	1214	rVB2	294	143	0.01%	0.001%
28	5.052	1214	1232	1262	rBV2	533059	1358930	100.00%	12.264%
29	5.286	1302	1305	1307	rBV3	494	211	0.02%	0.002%
30	5.437	1348	1352	1356	rVB4	566	406	0.03%	0.004%
31	5.457	1356	1358	1361	rVB2	189	66	0.00%	0.001%
32	5.476	1361	1364	1366	rBV	366	194	0.01%	0.002%
33	5.508	1367	1374	1376	rVB3	406	444	0.03%	0.004%
34	5.527	1376	1380	1383	rVB2	316	252	0.02%	0.002%
35	5.544	1383	1385	1388	rBV	330	162	0.01%	0.001%
36	5.621	1395	1409	1439	rBV	426536	863494	63.54%	7.793%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020138.D
 Acq On : 22 Jan 2021 16:15
 Operator : SY/MD
 Sample : M1181-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	5.916	1488	1501	1525	rVB5	49635	119712	8.81%	1.080%
38	6.074	1536	1550	1578	rBV	307942	632344	46.53%	5.707%
39	6.511	1682	1686	1688	rBV3	695	382	0.03%	0.003%
40	6.553	1697	1699	1703	rBV2	854	565	0.04%	0.005%
41	6.640	1724	1726	1727	rBV2	306	131	0.01%	0.001%
42	6.650	1727	1729	1732	rVB3	499	173	0.01%	0.002%
43	6.666	1732	1734	1736	rBV2	1219	698	0.05%	0.006%
44	6.727	1751	1753	1754	rBV2	519	178	0.01%	0.002%
45	6.778	1764	1769	1770	rBV2	588	452	0.03%	0.004%
46	6.891	1801	1804	1806	rBV3	762	528	0.04%	0.005%
47	6.910	1808	1810	1812	rBV2	477	261	0.02%	0.002%
48	6.990	1824	1835	1862	rBV2	142242	264966	19.50%	2.391%
49	7.322	1926	1938	1958	rBV	597693	1043206	76.77%	9.415%
50	7.511	1995	1997	2000	rBV2	687	321	0.02%	0.003%
51	7.627	2023	2033	2059	rBV	110047	199596	14.69%	1.801%
52	7.981	2130	2143	2158	rBV	478578	801189	58.96%	7.230%
53	8.093	2169	2178	2216	rBV2	277395	569503	41.91%	5.140%
54	8.482	2297	2299	2303	rBV3	624	463	0.03%	0.004%
55	8.547	2317	2319	2323	rVB3	939	444	0.03%	0.004%
56	8.598	2333	2335	2337	rBV2	325	131	0.01%	0.001%
57	8.666	2352	2356	2362	rBV4	562	500	0.04%	0.005%
58	8.707	2362	2369	2370	rBV2	347	333	0.02%	0.003%
59	8.859	2404	2416	2441	rBV	666947	1090793	80.27%	9.844%
60	9.354	2568	2570	2575	rVB3	581	376	0.03%	0.003%
61	9.466	2602	2605	2607	rBV3	456	354	0.03%	0.003%
62	9.675	2667	2670	2673	rBV2	278	255	0.02%	0.002%
63	9.694	2673	2676	2678	rVV3	373	227	0.02%	0.002%
64	9.807	2709	2711	2715	rBV2	240	183	0.01%	0.002%
65	9.894	2735	2738	2743	rVB2	443	319	0.02%	0.003%
66	10.055	2785	2788	2791	rBV2	583	294	0.02%	0.003%
67	10.074	2791	2794	2796	rBV2	264	203	0.01%	0.002%
68	10.141	2813	2815	2817	rBV	354	221	0.02%	0.002%
69	10.154	2817	2819	2821	rVV	467	191	0.01%	0.002%
70	10.222	2828	2840	2860	rBV	360124	569749	41.93%	5.142%
71	10.386	2883	2891	2893	rBV6	1339	1452	0.11%	0.013%
72	10.469	2914	2917	2918	rBV2	601	261	0.02%	0.002%
73	10.810	3021	3023	3024	rBV	418	157	0.01%	0.001%
74	10.839	3027	3032	3034	rBV3	953	642	0.05%	0.006%
75	10.920	3055	3057	3060	rBV3	388	194	0.01%	0.002%
76	10.939	3061	3063	3066	rVB4	688	394	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020138.D
Acq On : 22 Jan 2021 16:15
Operator : SY/MD
Sample : M1181-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E47

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Title : VOC Analysis

77	11.083	3106	3108	3109	rBV2	524	227	0.02%	0.002%
78	11.093	3109	3111	3113	rVV	543	227	0.02%	0.002%
79	11.257	3150	3162	3180	rBV	581460	912179	67.12%	8.232%
80	11.559	3254	3256	3257	rBV	631	258	0.02%	0.002%
81	11.630	3266	3278	3302	rBV	556513	884864	65.11%	7.986%
82	12.424	3523	3525	3527	rBV	386	151	0.01%	0.001%
83	14.878	4284	4288	4291	rVB3	1095	888	0.07%	0.008%




Sum of corrected areas: 11080835

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020138.D
Acq On : 22 Jan 2021 16:15
Operator : SY/MD
Sample : M1181-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

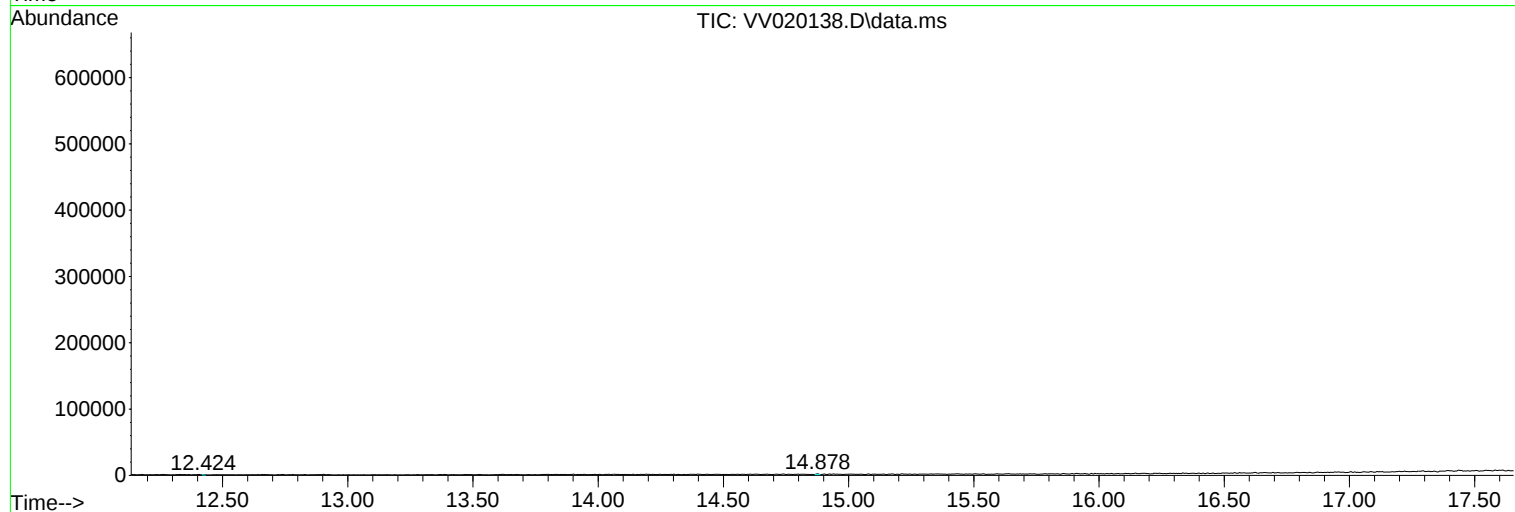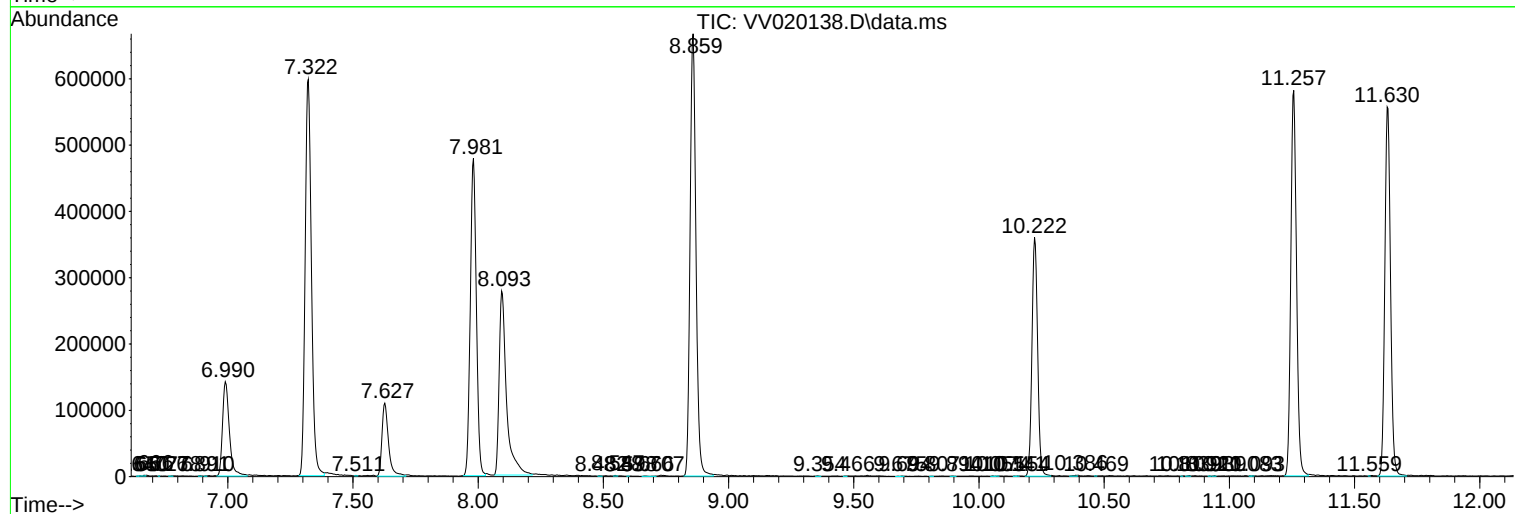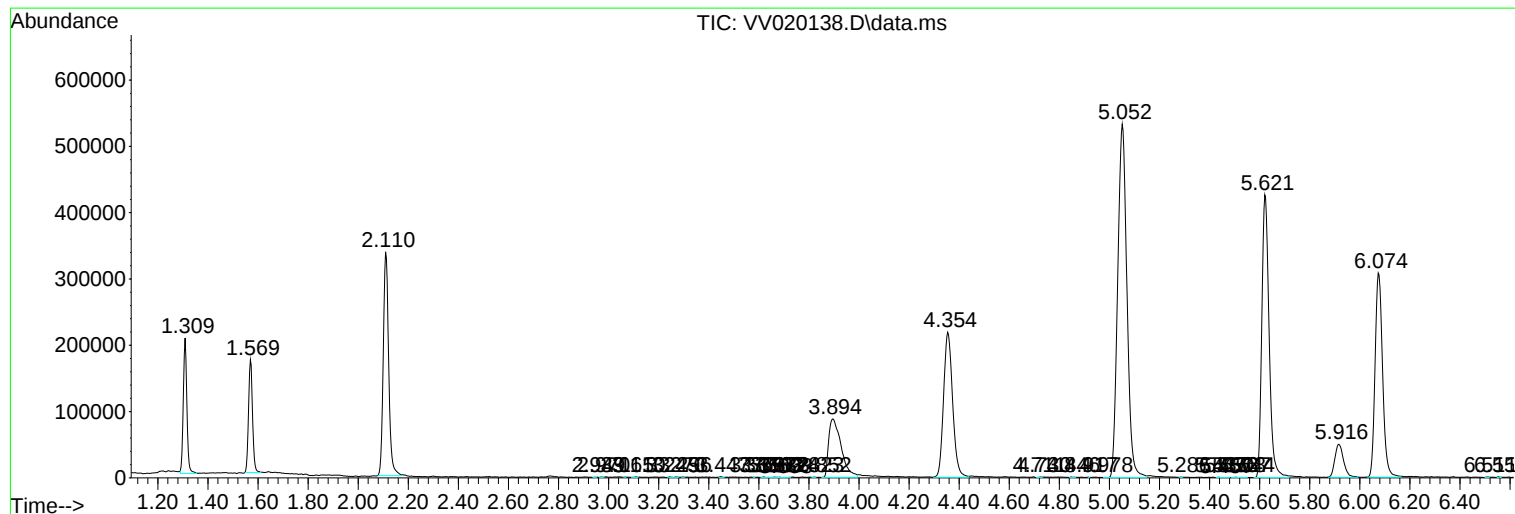

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020138.D
Acq On : 22 Jan 2021 16:15
Operator : SY/MD
Sample : M1181-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020138.D
Acq On : 22 Jan 2021 16:15
Operator : SY/MD
Sample : M1181-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
