

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012221\
 Data File : VW020141.D
 Acq On : 22 Jan 2021 17:25
 Operator : SY/MD
 Sample : M1181-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VW020141.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	86	rVB	242419	250661	15.00%	1.795%
2	1.569	142	149	161	rVB	225066	248555	14.88%	1.780%
3	2.109	307	317	334	rBV	427721	638487	38.22%	4.572%
4	2.637	477	481	482	rBV2	709	432	0.03%	0.003%
5	2.659	485	488	490	rBV	861	433	0.03%	0.003%
6	2.762	511	520	522	rBV4	1794	1521	0.09%	0.011%
7	2.859	547	550	555	rVV3	825	728	0.04%	0.005%
8	2.881	555	557	561	rVV3	669	494	0.03%	0.004%
9	2.917	566	568	572	rBV3	418	322	0.02%	0.002%
10	3.219	657	662	664	rBV4	836	766	0.05%	0.005%
11	3.399	714	718	720	rVV3	569	436	0.03%	0.003%
12	3.441	728	731	734	rVV3	592	435	0.03%	0.003%
13	3.457	734	736	741	rVV4	756	696	0.04%	0.005%
14	3.621	783	787	789	rVB4	482	334	0.02%	0.002%
15	3.643	789	794	796	rBV2	640	487	0.03%	0.003%
16	3.659	796	799	802	rVB5	606	310	0.02%	0.002%
17	3.679	802	805	806	rBV	509	281	0.02%	0.002%
18	3.720	815	818	821	rBV3	365	279	0.02%	0.002%
19	3.884	858	869	905	rBV	111875	340776	20.40%	2.440%
20	4.354	997	1015	1040	rBV	261265	651462	39.00%	4.665%
21	4.711	1125	1126	1130	rVB3	663	376	0.02%	0.003%
22	4.740	1131	1135	1138	rVV4	562	436	0.03%	0.003%
23	4.781	1147	1148	1151	rBV	580	300	0.02%	0.002%
24	4.849	1167	1169	1171	rVB2	661	309	0.02%	0.002%
25	4.871	1171	1176	1179	rBV3	429	386	0.02%	0.003%
26	4.888	1179	1181	1184	rVB2	556	337	0.02%	0.002%
27	5.051	1213	1232	1262	rBV2	619434	1592796	95.34%	11.405%
28	5.334	1318	1320	1323	rBV3	783	480	0.03%	0.003%
29	5.508	1370	1374	1377	rBV4	1008	589	0.04%	0.004%
30	5.531	1379	1381	1382	rBV2	876	313	0.02%	0.002%
31	5.624	1397	1410	1433	rBV	451154	903162	54.06%	6.467%
32	5.916	1488	1501	1524	rBV6	58232	141863	8.49%	1.016%
33	6.000	1524	1527	1531	rVB4	1637	1236	0.07%	0.009%
34	6.074	1537	1550	1573	rBV	359397	734254	43.95%	5.258%
35	6.309	1619	1623	1624	rBV3	882	603	0.04%	0.004%
36	6.437	1659	1663	1664	rBV2	620	373	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020141.D
 Acq On : 22 Jan 2021 17:25
 Operator : SY/MD
 Sample : M1181-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	6.579	1705	1707	1711	rBV3	755	560	0.03%	0.004%
38	6.630	1715	1723	1728	rBV6	926	1085	0.06%	0.008%
39	6.656	1728	1731	1737	rBV5	1265	1424	0.09%	0.010%
40	6.730	1750	1754	1757	rVB4	853	654	0.04%	0.005%
41	6.820	1775	1782	1785	rBV4	478	418	0.03%	0.003%
42	6.878	1795	1800	1804	rVB3	720	695	0.04%	0.005%
43	6.900	1804	1807	1811	rBV2	726	437	0.03%	0.003%
44	6.990	1823	1835	1855	rBV	204498	364910	21.84%	2.613%
45	7.196	1895	1899	1902	rBV5	916	794	0.05%	0.006%
46	7.318	1925	1937	1960	rBV	780524	1339897	80.21%	9.594%
47	7.627	2022	2033	2060	rVV	130658	234037	14.01%	1.676%
48	7.891	2112	2115	2118	rBV	687	499	0.03%	0.004%
49	7.981	2129	2143	2167	rBV	1002765	1670582	100.00%	11.962%
50	8.093	2168	2178	2217	rVV2	389373	758455	45.40%	5.431%
51	8.418	2275	2279	2283	rVB5	958	726	0.04%	0.005%
52	8.527	2311	2313	2315	rBV2	526	308	0.02%	0.002%
53	8.569	2321	2326	2327	rBV2	619	516	0.03%	0.004%
54	8.723	2370	2374	2377	rBV5	919	981	0.06%	0.007%
55	8.855	2404	2415	2441	rBV	702196	1141505	68.33%	8.174%
56	9.128	2497	2500	2503	rBV3	967	525	0.03%	0.004%
57	9.273	2543	2545	2547	rBV2	494	275	0.02%	0.002%
58	9.321	2557	2560	2563	rVB4	969	630	0.04%	0.005%
59	9.347	2566	2568	2571	rVV3	570	268	0.02%	0.002%
60	9.421	2589	2591	2596	rVB3	619	397	0.02%	0.003%
61	9.546	2626	2630	2632	rBV2	720	537	0.03%	0.004%
62	9.556	2632	2633	2636	rVB	935	425	0.03%	0.003%
63	9.630	2652	2656	2658	rVB3	869	692	0.04%	0.005%
64	9.649	2658	2662	2664	rBV3	715	509	0.03%	0.004%
65	9.958	2753	2758	2761	rBV2	511	421	0.03%	0.003%
66	10.106	2799	2804	2806	rBV4	608	638	0.04%	0.005%
67	10.125	2808	2810	2813	rVB2	756	355	0.02%	0.003%
68	10.222	2825	2840	2859	rVV	428051	670511	40.14%	4.801%
69	10.354	2877	2881	2883	rBV2	548	420	0.03%	0.003%
70	10.537	2936	2938	2941	rBV2	1014	615	0.04%	0.004%
71	10.579	2947	2951	2955	rBV3	625	560	0.03%	0.004%
72	10.627	2964	2966	2970	rVB4	554	332	0.02%	0.002%
73	10.649	2970	2973	2975	rBV2	801	534	0.03%	0.004%
74	10.749	2997	3004	3005	rBV3	860	685	0.04%	0.005%
75	10.794	3015	3018	3022	rBV4	357	338	0.02%	0.002%
76	10.884	3044	3046	3050	rVB2	771	405	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020141.D
 Acq On : 22 Jan 2021 17:25
 Operator : SY/MD
 Sample : M1181-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

77	10.942	3062	3064	3065	rBV	729	367	0.02%	0.003%
78	10.993	3073	3080	3085	rBV5	950	1458	0.09%	0.010%
79	11.016	3085	3087	3093	rVB4	828	637	0.04%	0.005%
80	11.048	3093	3097	3100	rVB3	625	420	0.03%	0.003%
81	11.109	3113	3116	3121	rBV4	779	678	0.04%	0.005%
82	11.193	3137	3142	3147	rBV5	1246	1390	0.08%	0.010%
83	11.257	3150	3162	3185	rBV	706655	1090016	65.25%	7.805%
84	11.633	3266	3279	3296	rBV	729346	1148527	68.75%	8.224%
85	11.871	3351	3353	3358	rBV3	595	484	0.03%	0.003%
86	12.099	3421	3424	3429	rBV4	720	604	0.04%	0.004%
87	12.260	3469	3474	3476	rBV4	487	382	0.02%	0.003%
88	12.382	3509	3512	3516	rBV4	751	411	0.02%	0.003%
89	12.479	3537	3542	3545	rVV	670	518	0.03%	0.004%
90	12.559	3563	3567	3568	rBV2	513	328	0.02%	0.002%
91	12.636	3588	3591	3594	rBV2	670	542	0.03%	0.004%
92	12.775	3630	3634	3638	rBV4	859	892	0.05%	0.006%
93	12.826	3646	3650	3653	rBV3	617	487	0.03%	0.003%
94	13.064	3721	3724	3726	rBV	528	304	0.02%	0.002%
95	13.083	3726	3730	3731	rBV3	594	459	0.03%	0.003%
96	13.128	3739	3744	3747	rBV5	658	472	0.03%	0.003%
97	13.270	3785	3788	3790	rBV4	601	392	0.02%	0.003%
98	13.823	3958	3960	3967	rBV3	549	574	0.03%	0.004%
99	13.858	3967	3971	3974	rBV3	478	333	0.02%	0.002%
100	14.437	4149	4151	4155	rBV2	588	424	0.03%	0.003%




Sum of corrected areas: 13965362

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020141.D
Acq On : 22 Jan 2021 17:25
Operator : SY/MD
Sample : M1181-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

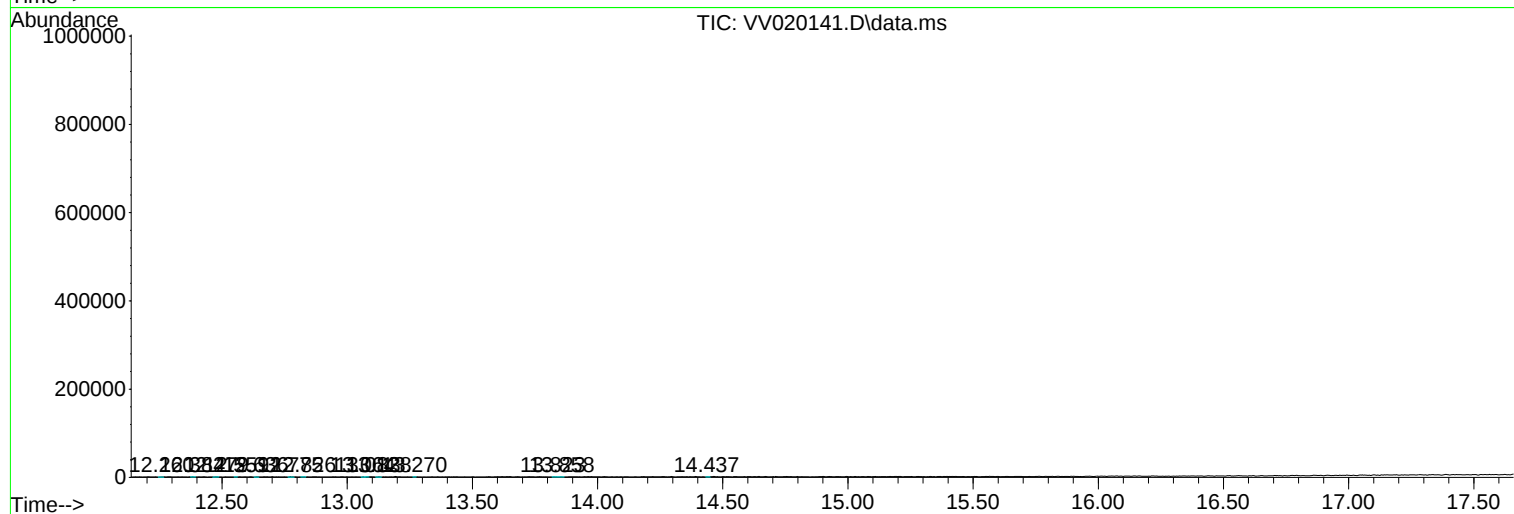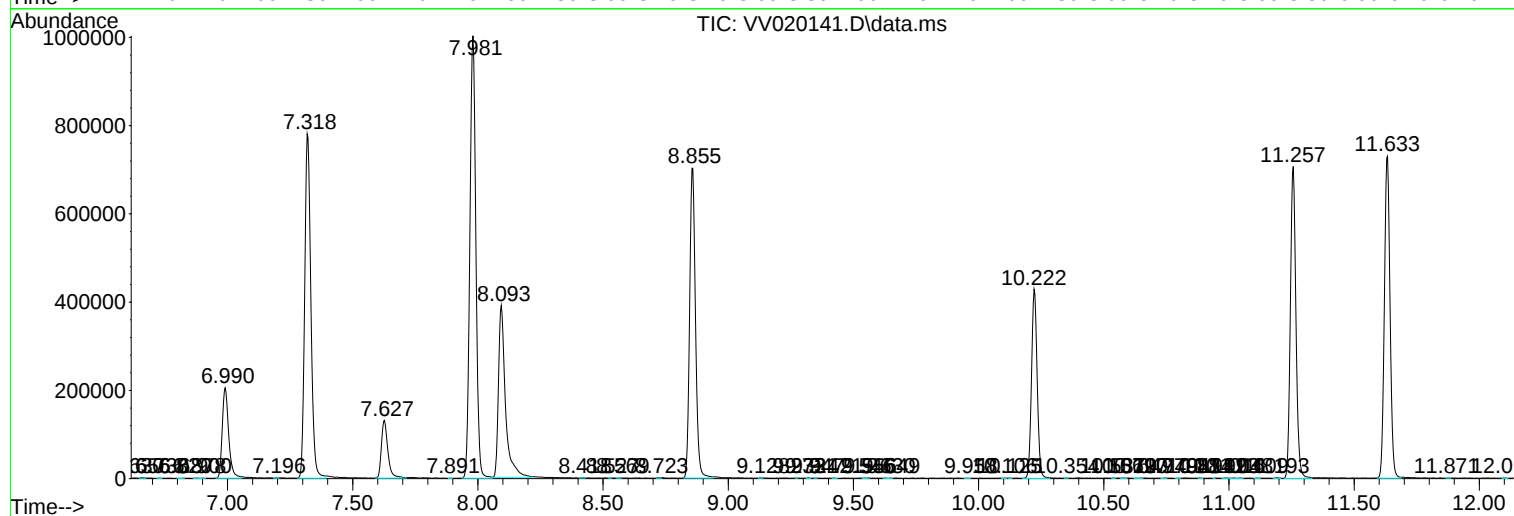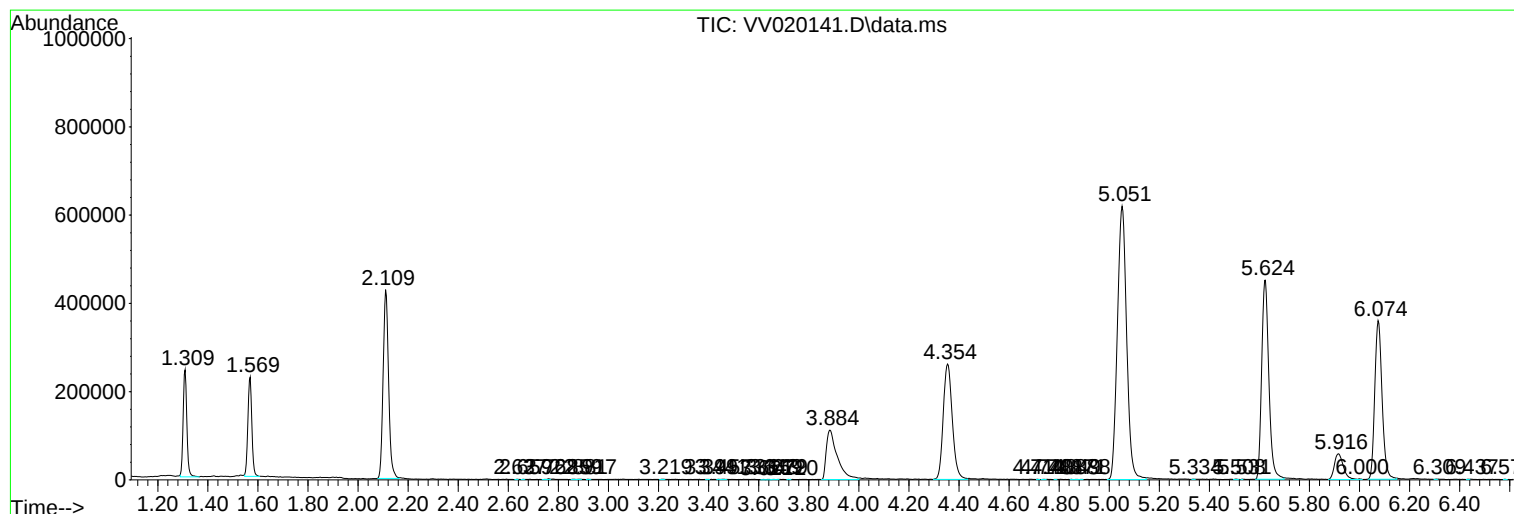

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020141.D
Acq On : 22 Jan 2021 17:25
Operator : SY/MD
Sample : M1181-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020141.D
Acq On : 22 Jan 2021 17:25
Operator : SY/MD
Sample : M1181-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------