

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020142.D
 Acq On : 22 Jan 2021 17:49
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020142.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	87	rVB	221850	227881	14.54%	1.836%
2	1.570	142	149	162	rVB	200990	227360	14.50%	1.832%
3	2.110	306	317	345	rVB	398752	592424	37.79%	4.773%
4	2.322	381	383	384	rBV2	655	282	0.02%	0.002%
5	2.711	501	504	511	rVV4	945	1062	0.07%	0.009%
6	2.750	514	516	521	rVB2	691	476	0.03%	0.004%
7	2.811	531	535	538	rBV2	695	525	0.03%	0.004%
8	2.846	544	546	549	rVB2	697	342	0.02%	0.003%
9	2.862	549	551	554	rVB2	571	278	0.02%	0.002%
10	2.885	556	558	562	rBV	517	360	0.02%	0.003%
11	2.930	570	572	576	rVB4	604	403	0.03%	0.003%
12	3.209	653	659	660	rBV2	344	270	0.02%	0.002%
13	3.254	669	673	674	rBV	573	394	0.03%	0.003%
14	3.315	690	692	695	rBV3	520	309	0.02%	0.002%
15	3.357	703	705	708	rVB4	610	287	0.02%	0.002%
16	3.399	716	718	721	rBV3	449	240	0.02%	0.002%
17	3.415	721	723	724	rBV	574	286	0.02%	0.002%
18	3.470	738	740	743	rVB3	622	382	0.02%	0.003%
19	3.486	743	745	747	rBV3	431	246	0.02%	0.002%
20	3.518	753	755	757	rBV2	838	462	0.03%	0.004%
21	3.624	786	788	790	rBV2	674	369	0.02%	0.003%
22	3.669	798	802	806	rVV3	623	589	0.04%	0.005%
23	3.756	826	829	831	rVB2	580	342	0.02%	0.003%
24	3.778	834	836	841	rVB	880	520	0.03%	0.004%
25	3.814	845	847	850	rBV3	519	293	0.02%	0.002%
26	3.888	860	870	917	rBV	113537	335822	21.42%	2.706%
27	4.354	999	1015	1040	rBV	261483	643295	41.03%	5.183%
28	4.595	1088	1090	1094	rBV3	710	500	0.03%	0.004%
29	4.611	1094	1095	1101	rVB5	772	460	0.03%	0.004%
30	4.933	1192	1195	1203	rVB3	402	392	0.03%	0.003%
31	5.052	1214	1232	1263	rBV2	611037	1567677	100.00%	12.632%
32	5.341	1319	1322	1324	rBV	932	426	0.03%	0.003%
33	5.508	1371	1374	1377	rVB3	605	359	0.02%	0.003%
34	5.531	1377	1381	1385	rBV3	1012	809	0.05%	0.007%
35	5.566	1389	1392	1395	rBV4	898	684	0.04%	0.006%
36	5.621	1396	1409	1440	rBV	529314	1036948	66.15%	8.355%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012221\
 Data File : VW020142.D
 Acq On : 22 Jan 2021 17:49
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	5.910	1488	1499	1514	rBV3	42837	87259	5.57%	0.703%
38	6.007	1527	1529	1533	rBV3	714	353	0.02%	0.003%
39	6.074	1536	1550	1579	rVV	387717	788078	50.27%	6.350%
40	6.257	1605	1607	1615	rVB5	1551	1274	0.08%	0.010%
41	6.370	1638	1642	1646	rBV4	820	734	0.05%	0.006%
42	6.499	1679	1682	1683	rBV	433	237	0.02%	0.002%
43	6.582	1706	1708	1714	rVB2	476	284	0.02%	0.002%
44	6.640	1720	1726	1732	rBV5	1215	1523	0.10%	0.012%
45	6.730	1751	1754	1757	rBV3	406	285	0.02%	0.002%
46	6.782	1767	1770	1775	rBV4	361	371	0.02%	0.003%
47	6.868	1793	1797	1801	rVB4	814	600	0.04%	0.005%
48	6.904	1805	1808	1810	rBV2	470	270	0.02%	0.002%
49	6.991	1823	1835	1860	rBV	192713	354556	22.62%	2.857%
50	7.270	1920	1922	1925	rVB3	664	316	0.02%	0.003%
51	7.322	1925	1938	1965	rBV	667169	1163129	74.19%	9.372%
52	7.566	2010	2014	2016	rBV3	502	350	0.02%	0.003%
53	7.627	2023	2033	2059	rBV	128365	223913	14.28%	1.804%
54	7.801	2084	2087	2089	rBV3	807	559	0.04%	0.005%
55	7.904	2117	2119	2121	rBV	723	394	0.03%	0.003%
56	7.984	2137	2144	2154	rVB7	4733	8398	0.54%	0.068%
57	8.093	2168	2178	2217	rBV2	366679	751428	47.93%	6.055%
58	8.383	2266	2268	2269	rBV2	743	356	0.02%	0.003%
59	8.701	2365	2367	2371	rBV2	313	232	0.01%	0.002%
60	8.859	2403	2416	2440	rBV	864751	1393378	88.88%	11.227%
61	9.087	2481	2487	2489	rBV3	1158	1021	0.07%	0.008%
62	9.373	2573	2576	2580	rVB2	349	279	0.02%	0.002%
63	9.479	2606	2609	2614	rVB3	464	329	0.02%	0.003%
64	9.524	2618	2623	2625	rVB2	480	271	0.02%	0.002%
65	9.775	2699	2701	2706	rBV3	239	233	0.01%	0.002%
66	9.797	2706	2708	2714	rVB2	316	246	0.02%	0.002%
67	10.000	2768	2771	2774	rBV2	345	294	0.02%	0.002%
68	10.145	2813	2816	2817	rBV2	618	329	0.02%	0.003%
69	10.174	2817	2825	2827	rVV5	824	868	0.06%	0.007%
70	10.222	2828	2840	2858	rVV	413313	656075	41.85%	5.286%
71	10.318	2867	2870	2871	rVB3	592	278	0.02%	0.002%
72	10.367	2879	2885	2888	rVV3	785	910	0.06%	0.007%
73	10.396	2892	2894	2897	rVB	569	285	0.02%	0.002%
74	10.453	2909	2912	2916	rBV3	536	526	0.03%	0.004%
75	10.518	2930	2932	2939	rVB4	485	370	0.02%	0.003%
76	10.569	2942	2948	2951	rBV3	837	972	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020142.D
 Acq On : 22 Jan 2021 17:49
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

77	10.611	2959	2961	2964	rVB3	591	389	0.02%	0.003%
78	10.746	3000	3003	3005	rBV3	619	264	0.02%	0.002%
79	10.801	3017	3020	3022	rBV2	824	439	0.03%	0.004%
80	10.823	3022	3027	3028	rBV3	570	347	0.02%	0.003%
81	10.836	3028	3031	3033	rBV2	584	374	0.02%	0.003%
82	10.865	3038	3040	3042	rVB2	1075	489	0.03%	0.004%
83	10.942	3060	3064	3067	rBV3	753	737	0.05%	0.006%
84	10.978	3071	3075	3077	rBV2	700	606	0.04%	0.005%
85	11.257	3149	3162	3181	rBV	762508	1176424	75.04%	9.479%
86	11.431	3214	3216	3220	rVB4	917	567	0.04%	0.005%
87	11.457	3220	3224	3226	rBV4	961	679	0.04%	0.005%
88	11.630	3267	3278	3295	rBV	717143	1139830	72.71%	9.184%
89	11.826	3336	3339	3341	rBV	763	455	0.03%	0.004%
90	11.884	3354	3357	3358	rBV	545	282	0.02%	0.002%
91	11.958	3378	3380	3382	rBV	629	375	0.02%	0.003%
92	12.254	3470	3472	3475	rBV2	552	294	0.02%	0.002%
93	12.376	3506	3510	3512	rVB2	910	525	0.03%	0.004%
94	12.518	3552	3554	3557	rBV2	482	237	0.02%	0.002%
95	12.669	3598	3601	3605	rBV3	478	392	0.03%	0.003%
96	12.948	3686	3688	3689	rBV	603	254	0.02%	0.002%
97	13.170	3756	3757	3763	rBV2	310	256	0.02%	0.002%
98	13.241	3775	3779	3782	rBV3	523	416	0.03%	0.003%
99	13.424	3833	3836	3837	rBV2	628	411	0.03%	0.003%
100	14.006	4014	4017	4021	rBV2	356	372	0.02%	0.003%




Sum of corrected areas: 12410731

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020142.D
Acq On : 22 Jan 2021 17:49
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

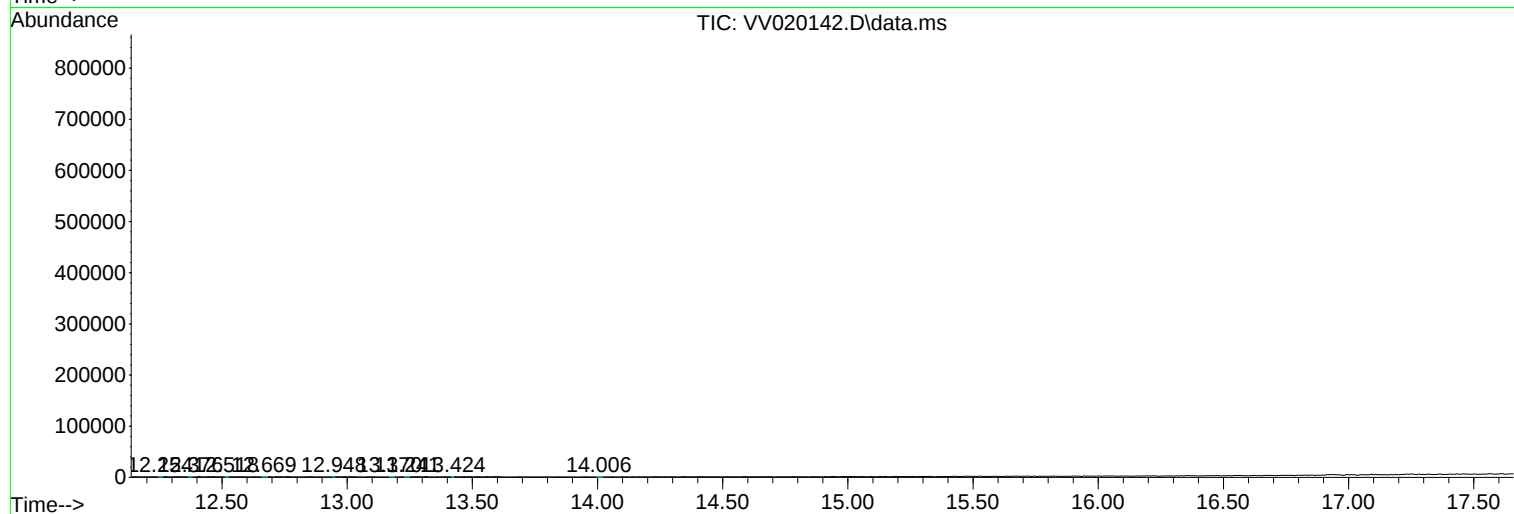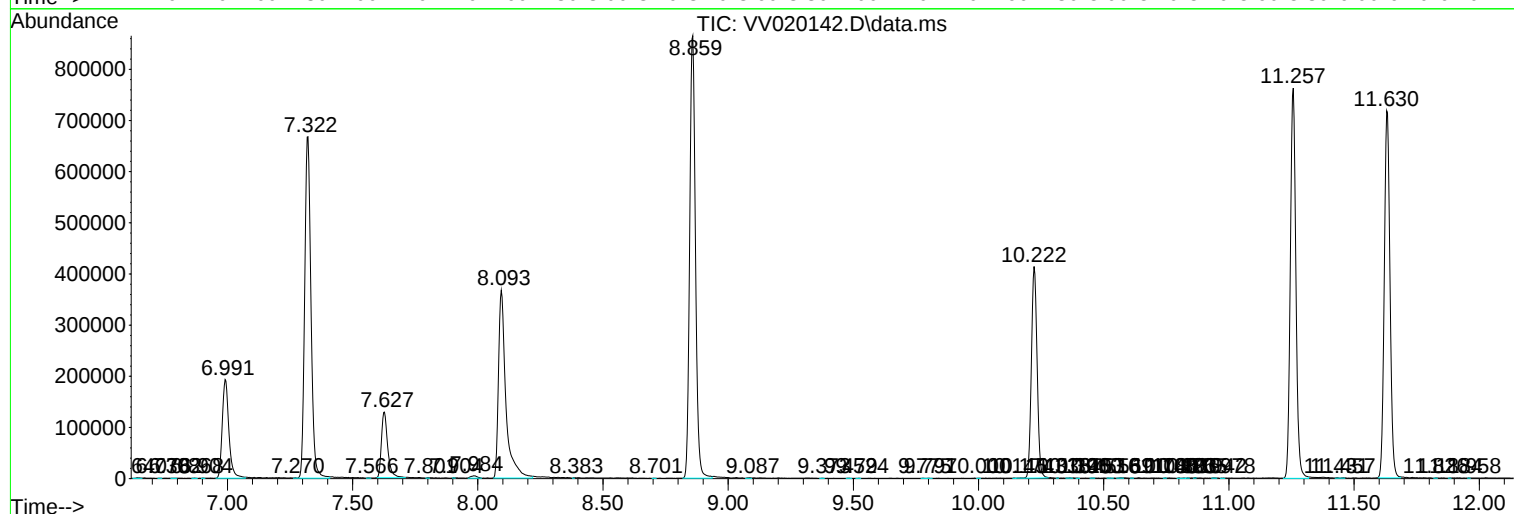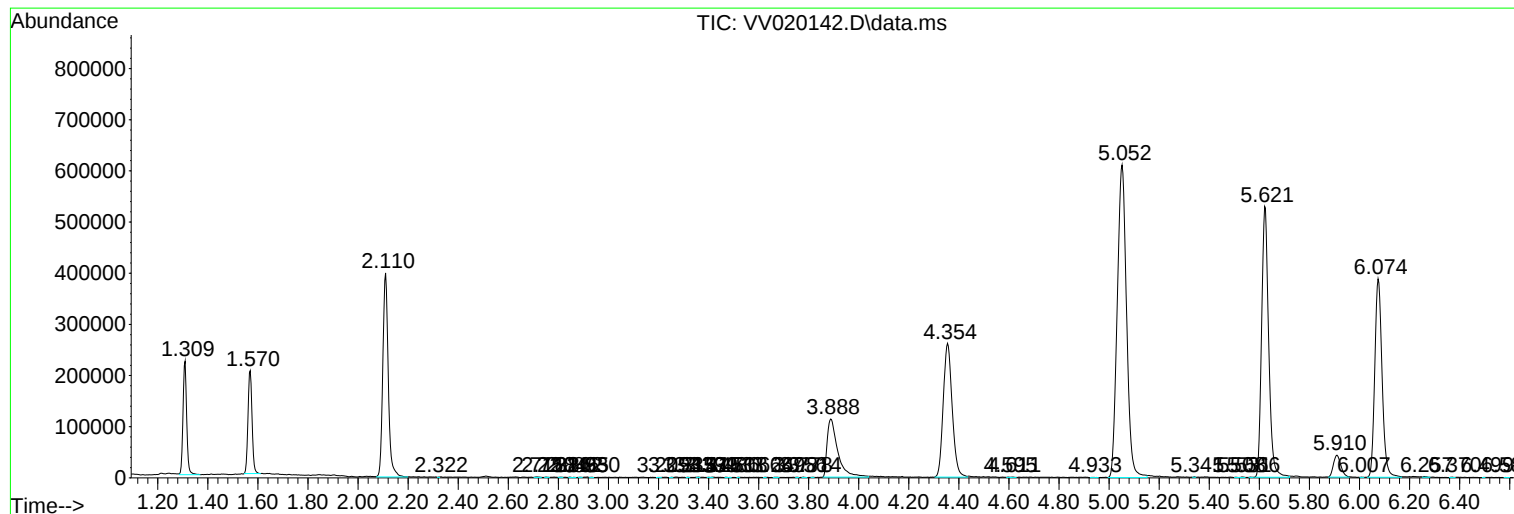

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020142.D
Acq On : 22 Jan 2021 17:49
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020142.D
Acq On : 22 Jan 2021 17:49
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
